

CR87484

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

5/16/2017 12:52

Test: Phenolics-

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	0.981	0.0	0.109	
ICB1	0.002	0.0	0.003	
CCV1	0.974	0.0	0.108	
CCB1	0.001	0.0	0.002	
PB98965BL	-0.001	0.0	0.002	
PB98965BS	0.996	0.0	0.111	
I3147-02	-0.001	0.0	0.002	
I3147-02DUP	-0.002	0.0	0.002	
I3147-02MS	0.823	0.0	0.092	
I3147-02MSD	0.829	0.0	0.093	
I3147-04	0.001	0.0	0.002	
I3147-06	0.002	0.0	0.003	
CCV2	0.967	0.0	0.108	
CCB2	0.001	0.0	0.002	

N	14
Mean	0.398
SD	0.4791
CV%	120.34

C887484

AK

Aquakem v. 7.2AQ1

Results from time period:

Tue May 16 12:03:05 2017

Tue May 16 12:42:55 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0511	mg/l	5/16/2017 12:03:05	
0.1PPM	A	Phenolics-	P	0.102	mg/l	5/16/2017 12:03:06	
0.25PPM	A	Phenolics-	P	0.2536	mg/l	5/16/2017 12:03:07	
0.50PPM	A	Phenolics-	P	0.497	mg/l	5/16/2017 12:03:08	
1.0PPM	A	Phenolics-	P	0.9921	mg/l	5/16/2017 12:03:09	
2.0PPM	A	Phenolics-	P	2.0041	mg/l	5/16/2017 12:03:10	
ICV1	S	Phenolics-	P	0.9808	mg/l	5/16/2017 12:38:27	
ICB1	S	Phenolics-	P	0.0023	mg/l	5/16/2017 12:38:28	
CCV1	S	Phenolics-	P	0.9743	mg/l	5/16/2017 12:38:29	
CCB1	S	Phenolics-	P	0.0012	mg/l	5/16/2017 12:38:30	
PB98965BL	S	Phenolics-	P	-0.001	mg/l	5/16/2017 12:38:31	
PB98965BS	S	Phenolics-	P	0.9957	mg/l	5/16/2017 12:38:32	
I3147-02	S	Phenolics-	P	-0.0009	mg/l	5/16/2017 12:38:33	
I3147-02DUP	S	Phenolics-	P	-0.0017	mg/l	5/16/2017 12:38:34	
I3147-02MS	S	Phenolics-	P	0.8227	mg/l	5/16/2017 12:38:35	
I3147-02MSD	S	Phenolics-	P	0.8289	mg/l	5/16/2017 12:38:36	
I3147-04	S	Phenolics-	P	0.0007	mg/l	5/16/2017 12:38:37	
I3147-06	S	Phenolics-	P	0.0024	mg/l	5/16/2017 12:38:38	
CCV2	S	Phenolics-	P	0.9671	mg/l	5/16/2017 12:42:53	
CCB2	S	Phenolics-	P	0.0006	mg/l	5/16/2017 12:42:54	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AK

5/16/2017 12:10


Test Phenolics-

Accepted 5/16/2017 12:10

Factor 9.176
 Bias 0.002

Coeff. of det. 0.999962

Errors

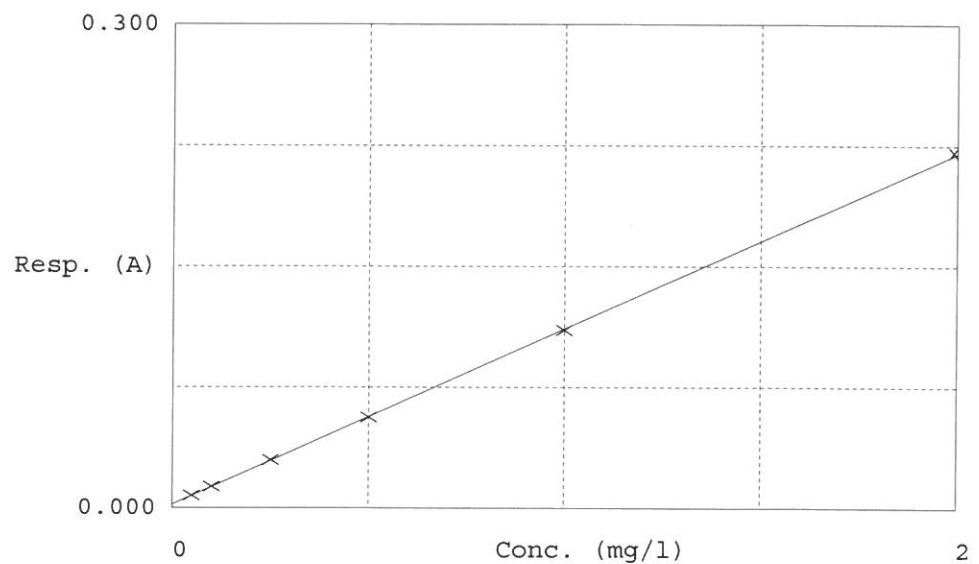

	Calibrator	Response	Calc. con.	Conc.	Errors

1	Phenol-2	0.008	0.0511	0.0500	
2	Phenol-2	0.013	0.1020	0.1000	
3	Phenol-2	0.030	0.2536	0.2500	
4	Phenol-2	0.056	0.4970	0.5000	
5	Phenol-2	0.110	0.9921	1.0000	
6	Phenol-2	0.221	2.0041	2.0000	