


ISM02.4

LB 87530
INSTRUMENT ID: CV2

Linear

 μ Abs.:

4311E

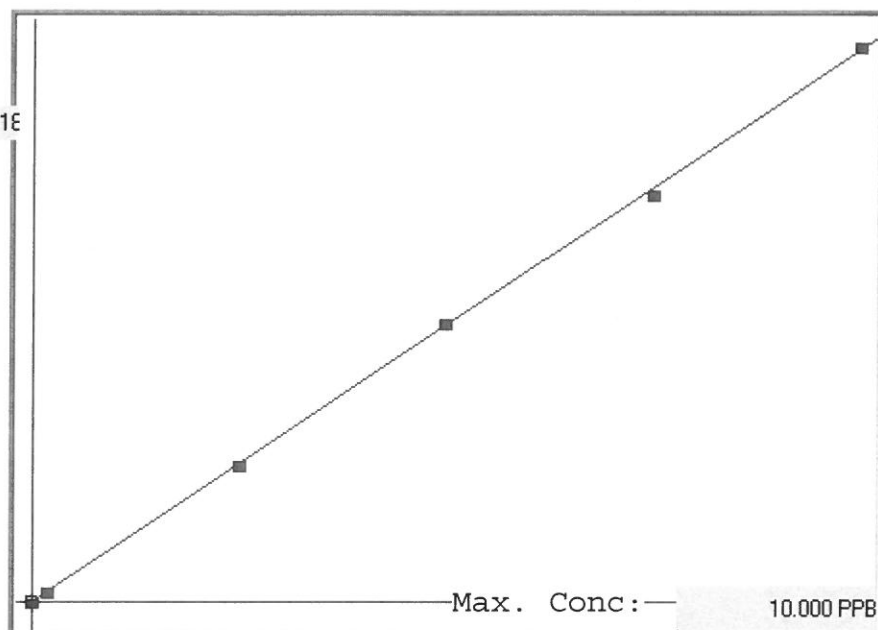

A= 0.0000e+000

B= 2.3308e-004

C= 2.2351e-003

Rho= 0.9998949

Accept=Accepted

slope
 $y = 2.3308 \times 10^{-4} x + 2.2351 \times 10^{-3}$

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.002	0.002	0	0.000	0					0
0.2	0.200	0.203	0.003	861	0.0 %	861					2
2.5	2.500	2.494	-0.006	10692	0.0 %	10692					0
5.0	5.000	5.055	0.055	21679	0.0 %	21679					1
7.5	7.500	7.393	-0.107	31711	0.0 %	31711					1
10.0	10.000	10.052	0.052	43118	0.0 %	43118					1

263
 5/18/17

LB87530
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	0	-		0 ISM02.4	PPB	5/18/2017 11:10	Std
	0.2 S0.2	861	-		0.2 ISM02.4	PPB	5/18/2017 11:12	Std
	2.5 S2.5	10692	-		2.5 ISM02.4	PPB	5/18/2017 11:14	Std
	5 S5	21679	-		5 ISM02.4	PPB	5/18/2017 11:17	Std
	7.5 S7.5	31711	-		7.5 ISM02.4	PPB	5/18/2017 11:19	Std
	10 S10	43118	-		10 ISM02.4	PPB	5/18/2017 11:24	Std
ICV	ICV	15545	3.6254 -		ISM02.4	PPB	5/18/2017 11:26	SMPL
ICB	ICB	-86	-0.0178 -		ISM02.4	PPB	5/18/2017 11:29	SMPL
CCV033	CCV033	21517	5.0174 -		ISM02.4	PPB	5/18/2017 11:31	SMPL
CCB033	CCB033	-65	-0.0129 -		ISM02.4	PPB	5/18/2017 11:33	SMPL
PB99033BL	PBW003	1	0.0025 -		ISM02.4	PPB	5/18/2017 11:36	SMPL
I3067-01	MBDCG9	64	0.0172 -		ISM02.4	PPB	5/18/2017 11:38	SMPL
I3067-02	MBDCG9D	59	0.016 -		ISM02.4	PPB	5/18/2017 11:40	SMPL
I3067-03	MBDCG9S	4329	1.0112 -		ISM02.4	PPB	5/18/2017 11:42	SMPL
I3067-04	MBDCF5	-89	-0.0185 -		ISM02.4	PPB	5/18/2017 11:45	SMPL
I3067-05	MBDCF6	-5	0.0011 -		ISM02.4	PPB	5/18/2017 11:47	SMPL
I3067-06	MBDCF7	135	0.0337 -		ISM02.4	PPB	5/18/2017 11:49	SMPL
I3067-07	MBDCK5	-76	-0.0155 -		ISM02.4	PPB	5/18/2017 11:51	SMPL
I3067-08	MBDCH1	104	0.0265 -		ISM02.4	PPB	5/18/2017 11:54	SMPL
I3067-09	MBDCH2	98	0.0251 -		ISM02.4	PPB	5/18/2017 11:56	SMPL
I3067-10	MBDCK6	-85	-0.0176 -		ISM02.4	PPB	5/18/2017 11:58	SMPL
I3067-11	MBDCC3	-79	-0.0162 -		ISM02.4	PPB	5/18/2017 12:01	SMPL
I3067-12	MBDCC4	2669	0.6243 -		ISM02.4	PPB	5/18/2017 12:03	SMPL
I3067-13	MBDCF9	-97	-0.0204 -		ISM02.4	PPB	5/18/2017 12:05	SMPL
I3067-14	MBDCF8	-92	-0.0192 -		ISM02.4	PPB	5/18/2017 12:07	SMPL
I3067-15	MBDCG0	-70	-0.0141 -		ISM02.4	PPB	5/18/2017 12:10	SMPL
I3067-16	MBDCG1	-59	-0.0115 -		ISM02.4	PPB	5/18/2017 12:12	SMPL
I3067-17	MBDCH3	268	0.0647 -		ISM02.4	PPB	5/18/2017 12:14	SMPL
I3067-18	MBDCK7	-112	-0.0239 -		ISM02.4	PPB	5/18/2017 12:17	SMPL
I3067-19	MBDCC5	168	0.0414 -		ISM02.4	PPB	5/18/2017 12:19	SMPL
CCV034	CCV034	21149	4.9316 -		ISM02.4	PPB	5/18/2017 12:21	SMPL
CCB034	CCB034	-68	-0.0136 -		ISM02.4	PPB	5/18/2017 12:23	SMPL
I3067-20	MBDCC7	51	0.0141 -		ISM02.4	PPB	5/18/2017 12:26	SMPL
I3067-21	MBDCC8	-38	-0.0066 -		ISM02.4	PPB	5/18/2017 12:28	SMPL
I3067-22	MBDCC9	-95	-0.0199 -		ISM02.4	PPB	5/18/2017 12:30	SMPL
PB99034BL	PBW003	-32	-0.0052 -		ISM02.4	PPB	5/18/2017 12:32	SMPL
I3068-01	MBDCR9	37	0.0109 -		ISM02.4	PPB	5/18/2017 12:35	SMPL
I3068-02	MBDCR9D	45	0.0127 -		ISM02.4	PPB	5/18/2017 12:37	SMPL
I3068-03	MBDCR9S	4328	1.011 -		ISM02.4	PPB	5/18/2017 12:39	SMPL
I3068-04	MBDCQ5	-119	-0.0255 -		ISM02.4	PPB	5/18/2017 12:42	SMPL
I3068-05	MBDCQ6	-98	-0.0206 -		ISM02.4	PPB	5/18/2017 12:44	SMPL
I3068-06	MBDCQ7	-85	-0.0176 -		ISM02.4	PPB	5/18/2017 12:46	SMPL
I3068-07	MBDCS1	-58	-0.0113 -		ISM02.4	PPB	5/18/2017 12:48	SMPL
I3068-08	MBDCS2	-58	-0.0113 -		ISM02.4	PPB	5/18/2017 12:51	SMPL
I3068-09	MBDCQ8	-87	-0.018 -		ISM02.4	PPB	5/18/2017 12:53	SMPL
I3068-10	MBDCR0	-94	-0.0197 -		ISM02.4	PPB	5/18/2017 12:55	SMPL

LB87530
INSTRUMENT ID : CV1

I3068-11	MBDCR1	-91	-0.019 -	ISM02.4	PPB	5/18/2017 12:58	SMPL
I3068-12	MBDCS3	-71	-0.0143 -	ISM02.4	PPB	5/18/2017 13:00	SMPL
I3068-14	MBDCM3	-88	-0.0183 -	ISM02.4	PPB	5/18/2017 13:02	SMPL
I3068-15	MBDCM4	1473	0.3456 -	ISM02.4	PPB	5/18/2017 13:04	SMPL
I3068-16	MBDCQ9	-76	-0.0155 -	ISM02.4	PPB	5/18/2017 13:07	SMPL
I3068-17	MBDCM8	-88	-0.0183 -	ISM02.4	PPB	5/18/2017 13:09	SMPL
CCV035	CCV035	21223	4.9488 -	ISM02.4	PPB	5/18/2017 13:11	SMPL
CCB035	CCB035	-91	-0.019 -	ISM02.4	PPB	5/18/2017 13:13	SMPL
I3068-18	MBDCM5	82	0.0213 -	ISM02.4	PPB	5/18/2017 13:16	SMPL
I3068-19	MBDCM7	-97	-0.0204 -	ISM02.4	PPB	5/18/2017 13:18	SMPL
I3068-20	MBDCM9	-83	-0.0171 -	ISM02.4	PPB	5/18/2017 13:20	SMPL
CCV036	CCV036	21354	4.9794 -	ISM02.4	PPB	5/18/2017 13:23	SMPL
CCB036	CCB036	-72	-0.0145 -	ISM02.4	PPB	5/18/2017 13:25	SMPL