


ISM02.4

LB 87638  
INSTRUMENT ID: CVJ

Linear

 $\mu$  Abs.:

44105

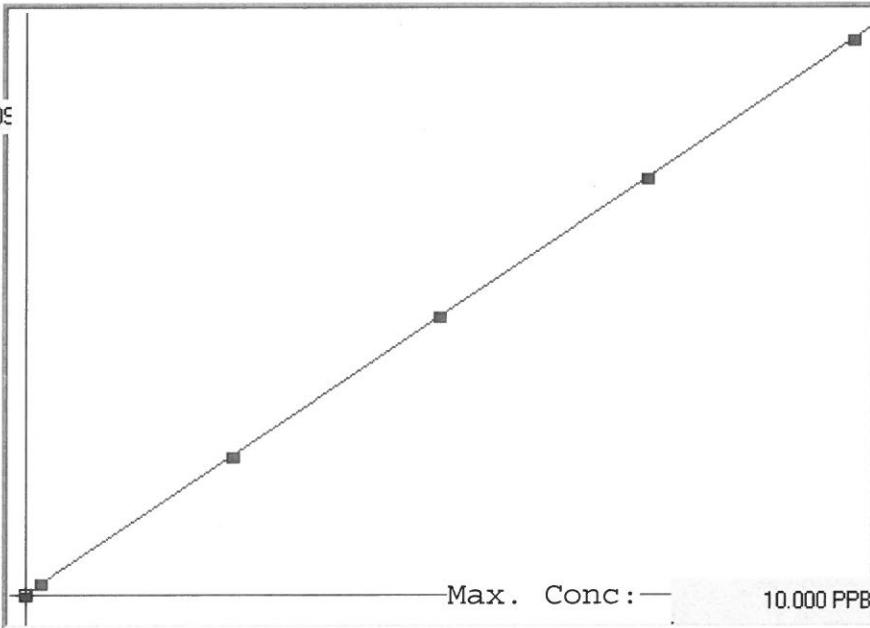

A= 0.0000e+000

B= 2.2666e-004

C= -1.0263e-002

Rho= 0.9999918

Accept=Accepted

slope  
= intercept

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | %OD |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|-----|
| 0.00   | 0.000  | -0.006 | -0.006 | 18    | 0.000      | 18    |       |       |       |       | 1   |
| 0.2    | 0.200  | 0.201  | 0.001  | 931   | 0.0 %      | 931   |       |       |       |       | 1   |
| 2.5    | 2.500  | 2.487  | -0.013 | 11016 | 0.0 %      | 11016 |       |       |       |       | -1  |
| 5.0    | 5.000  | 5.031  | 0.031  | 22242 | 0.0 %      | 22242 |       |       |       |       | 1   |
| 7.5    | 7.500  | 7.500  | 0.000  | 33135 | 0.0 %      | 33135 |       |       |       |       | 0   |
| 10.0   | 10.000 | 9.988  | -0.012 | 44109 | 0.0 %      | 44109 |       |       |       |       | 0   |

NB  
5123113

LB87638

INSTRUMENT ID : CV1

| Sample ID | Extended ID | $\mu$ Abs. | Conc.     | Std Conc | Method      | Units | Date            | Type |
|-----------|-------------|------------|-----------|----------|-------------|-------|-----------------|------|
|           | 0 S0        | 18         | -         |          | 0 ISM02.4   | PPB   | 5/23/2017 12:48 | Std  |
|           | 0.2 S0.2    | 931        | -         |          | 0.2 ISM02.4 | PPB   | 5/23/2017 12:50 | Std  |
|           | 2.5 S2.5    | 11016      | -         |          | 2.5 ISM02.4 | PPB   | 5/23/2017 12:52 | Std  |
|           | 5 S5        | 22242      | -         |          | 5 ISM02.4   | PPB   | 5/23/2017 12:55 | Std  |
|           | 7.5 S7.5    | 33135      | -         |          | 7.5 ISM02.4 | PPB   | 5/23/2017 12:57 | Std  |
|           | 10 S10      | 44109      | -         |          | 10 ISM02.4  | PPB   | 5/23/2017 12:59 | Std  |
| ICV       | ICV         | 17501      | 3.9565 -  |          | ISM02.4     | PPB   | 5/23/2017 13:02 | SMPL |
| ICB       | ICB         | -36        | -0.0184 - |          | ISM02.4     | PPB   | 5/23/2017 13:04 | SMPL |
| CCV083    | CCV083      | 22202      | 5.0221 -  |          | ISM02.4     | PPB   | 5/23/2017 13:06 | SMPL |
| CCB083    | CCB083      | -62        | -0.0243 - |          | ISM02.4     | PPB   | 5/23/2017 13:09 | SMPL |
| PB99218BL | PBS004      | 168        | 0.0278 -  |          | ISM02.4     | PPB   | 5/23/2017 13:11 | SMPL |
| I3251-01  | PTS-02      | 985        | 0.213 -   |          | ISM02.4     | PPB   | 5/23/2017 13:20 | SMPL |
| I3251-01D | PTS-02D     | 944        | 0.2037 -  |          | ISM02.4     | PPB   | 5/23/2017 13:22 | SMPL |
| I3251-01S | PTS-02S     | 12104      | 2.7332 -  |          | ISM02.4     | PPB   | 5/23/2017 13:24 | SMPL |
| CCV084    | CCV084      | 22440      | 5.076 -   |          | ISM02.4     | PPB   | 5/23/2017 13:26 | SMPL |
| CCB084    | CCB084      | -10        | -0.0125 - |          | ISM02.4     | PPB   | 5/23/2017 13:29 | SMPL |