


7470A

LB 87752
INSTRUMENT ID: CV1

Linear

 μ Abs.:

36807

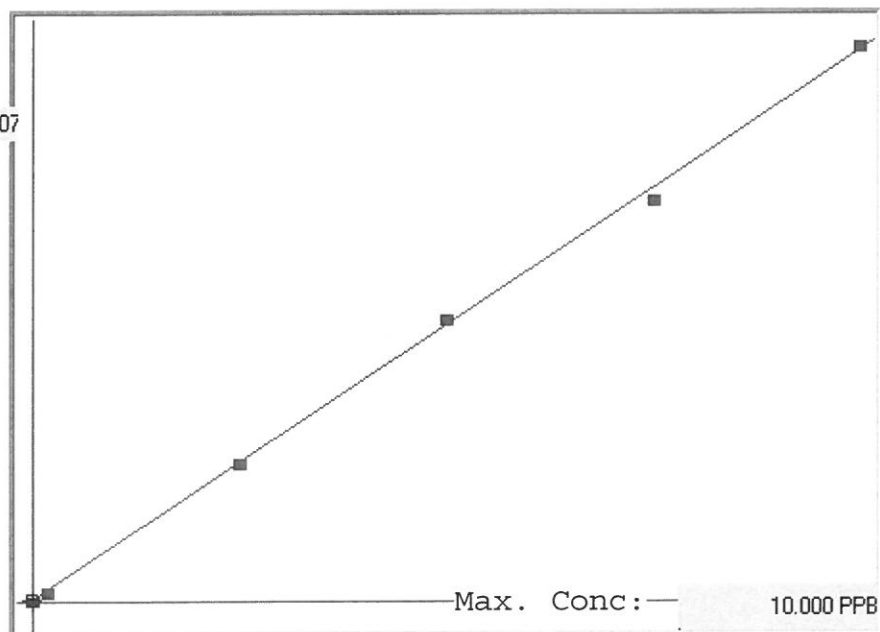

A= 0.0000e+000

B= 2.7470e-004

C= -3.3535e-002

Rho= 0.9996642

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.020	0.020	194	0.000	194				
0.2	0.200	0.170	-0.030	741	0.0 %	741				
2.5	2.500	2.508	0.008	9251	0.0 %	9251				
5.0	5.000	5.112	0.112	18732	0.0 %	18732				
7.5	7.500	7.313	-0.187	26744	0.0 %	26744				
10.0	10.000	10.077	0.077	36807	0.0 %	36807				

LB87752 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 May 2017 12:34:15

Sample ID	Extended ID	µ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	194	-	0.0000	7470A	PPB	30 May 2017 12:36:12	S	Std
0.2 - 1	50.2	741	-	0.2000	7470A	PPB	30 May 2017 12:38:21	S	Std
2.5 - 1	52.5	9251	-	2.5000	7470A	PPB	30 May 2017 12:40:29	S	Std
5.0 - 1	55	18732	-	5.0000	7470A	PPB	30 May 2017 12:42:38	S	Std
7.5 - 1	57.5	26744	-	7.5000	7470A	PPB	30 May 2017 12:44:45	S	Std
10.0 - 1	510	36807	-	10.0000	7470A	PPB	30 May 2017 12:46:52	S	Std
ICV78 - 1	ICV78	14573	3.9697	-	7470A	PPB	30 May 2017 12:49:31	U	SMPL
ICB78 - 1	ICB78	216	0.0258	-	7470A	PPB	30 May 2017 12:51:37	U	SMPL
CCV34 - 1	CCV34	18480	5.0429	-	7470A	PPB	30 May 2017 12:53:44	U	SMPL
CCB34 - 1	CCB34	212	0.0247	-	7470A	PPB	30 May 2017 12:55:50	U	SMPL
CRA - 1	CRA	734	0.1681	-	7470A	PPB	30 May 2017 12:57:57	U	SMPL
HighStd - 1	HighStd	36821	10.0812	-	7470A	PPB	30 May 2017 13:00:04	U	SMPL
ChkStd - 1	ChkStd	25178	6.8829	-	7470A	PPB	30 May 2017 13:02:10	U	SMPL
PB99364BL - 1	PBW	139	0.0046	-	7470A	PPB	30 May 2017 13:04:18	U	SMPL
PB99364BS - 1	LCSW	14139	3.8504	-	7470A	PPB	30 May 2017 13:06:25	U	SMPL
PB99364TB - 1	PB99396TB	119	-0.0008	-	7470A	PPB	30 May 2017 13:08:33	U	SMPL
I3340-07 - 1	SP-1	157	0.0096	-	7470A	PPB	30 May 2017 13:10:41	U	SMPL
I3340-11 - 1	265563	164	0.0115	-	7470A	PPB	30 May 2017 13:12:49	U	SMPL
I3340-16 - 1	DRUM-1-DRUM-2-COMP	199	0.0211	-	7470A	PPB	30 May 2017 13:14:58	U	SMPL
I3345-07 - 1	DUCT-BANK	160	0.0104	-	7470A	PPB	30 May 2017 13:17:05	U	SMPL
CCV35 - 1	CCV35	18563	5.0657	-	7470A	PPB	30 May 2017 13:19:12	U	SMPL
CCB35 - 1	CCB35	230	0.0296	-	7470A	PPB	30 May 2017 13:21:18	U	SMPL
I3347-04 - 1	72-11931/VNJ-208/153/341/132	135	0.0035	-	7470A	PPB	30 May 2017 13:23:25	U	SMPL
I3347-06 - 1	284-CONCRETE	143	0.0057	-	7470A	PPB	30 May 2017 13:25:32	U	SMPL
I3348-03 - 1	VNJ-225/289/330/139/15532/VNJ-230	160	0.0104	-	7470A	PPB	30 May 2017 13:27:39	U	SMPL
I3349-02 - 1	TP-4	154	0.0088	-	7470A	PPB	30 May 2017 13:29:46	U	SMPL
I3365-03 - 1	SB-03-COMP	160	0.0104	-	7470A	PPB	30 May 2017 13:31:53	U	SMPL
I3371-02 - 1	A598	148	0.0071	-	7470A	PPB	30 May 2017 13:34:01	U	SMPL
I3371-02DUP - 1	A598DUP	157	0.0096	-	7470A	PPB	30 May 2017 13:36:09	U	SMPL
I3371-02MS - 1	A598MS	13735	3.7395	-	7470A	PPB	30 May 2017 13:38:17	U	SMPL
I3371-02MSD - 1	A598MSD	14058	3.8282	-	7470A	PPB	30 May 2017 13:40:26	U	SMPL
CCV36 - 1	CCV36	18867	5.1492	-	7470A	PPB	30 May 2017 13:42:32	U	SMPL
CCB36 - 1	CCB36	226	0.0285	-	7470A	PPB	30 May 2017 13:44:39	U	SMPL
I3371-02LX5 - 1		211	0.0244	-	7470A	PPB	30 May 2017 13:46:46	U	SMPL
I3371-02A - 1		14718	4.0095	-	7470A	PPB	30 May 2017 13:48:53	U	SMPL
CCV37 - 1	CCV37	18653	5.0904	-	7470A	PPB	30 May 2017 13:51:00	U	SMPL
CCB37 - 1	CCB37	111	-0.0030	-	7470A	PPB	30 May 2017 13:53:07	U	SMPL