


7470A

LB87967
INSTRUMENT ID: CV1

Linear

 μ Abs.:

37539

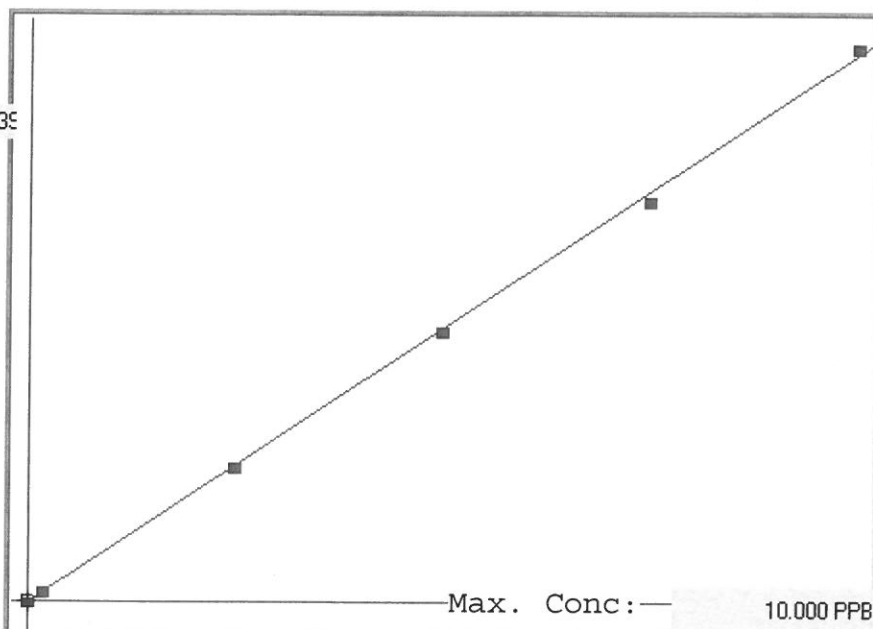

A= 0.0000e+000

B= 2.6901e-004

C= 3.2142e-002

Rho= 0.9997103

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.050	0.050	66	0.000	66				
0.2	0.200	0.214	0.014	675	0.0 %	675				
2.5	2.500	2.489	-0.011	9134	0.0 %	9134				
5.0	5.000	4.981	-0.019	18397	0.0 %	18397				
7.5	7.500	7.335	-0.165	27148	0.0 %	27148				
10.0	10.000	10.131	0.131	37539	0.0 %	37539				

LB87767 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 31 May 2017 10:29:49					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	66	-	0.0000	7470A	PPB	31 May 2017 10:33:01	S	Std
0.2 - 1	52.5	675	-	0.2000	7470A	PPB	31 May 2017 10:35:09	S	Std
2.5 - 1	52.5	9134	-	2.5000	7470A	PPB	31 May 2017 10:37:17	S	Std
5.0 - 1	55	18397	-	5.0000	7470A	PPB	31 May 2017 10:39:26	S	Std
7.5 - 1	57.5	27148	-	7.5000	7470A	PPB	31 May 2017 10:41:34	S	Std
10.0 - 1	510	37539	-	10.0000	7470A	PPB	31 May 2017 10:43:41	S	Std
ICV79 - 1	ICV79	13751	3.7313	-	7470A	PPB	31 May 2017 10:46:34	U	SMPL
ICB79 - 1	ICB79	54	0.0467	-	7470A	PPB	31 May 2017 10:48:40	U	SMPL
CCV38 - 1	CCV38	18303	4.9559	-	7470A	PPB	31 May 2017 10:50:47	U	SMPL
CCB38 - 1	CCB38	97	0.0582	-	7470A	PPB	31 May 2017 10:52:54	U	SMPL
CRA - 1	CRA	671	0.2126	-	7470A	PPB	31 May 2017 10:55:00	U	SMPL
HighStd - 1	HighStd	36716	9.9092	-	7470A	PPB	31 May 2017 10:57:07	U	SMPL
ChkStd - 1	ChkStd	24939	6.7410	-	7470A	PPB	31 May 2017 10:59:14	U	SMPL
PB99378BL - 1	PBW	-12	0.0289	-	7470A	PPB	31 May 2017 11:01:21	U	SMPL
PB99378BS - 1	LCSW	14377	3.8997	-	7470A	PPB	31 May 2017 11:03:29	U	SMPL
I3306-01 - 1	DSK-EB	-93	0.0071	-	7470A	PPB	31 May 2017 11:05:37	U	SMPL
I3306-06 - 1	DSK-MW-LS	88	0.0558	-	7470A	PPB	31 May 2017 11:12:21	U	SMPL
I3306-06DUP - 1	DSK-MW-LSDUP	28	0.0397	-	7470A	PPB	31 May 2017 11:14:29	U	SMPL
I3306-07 - 1	I3306-06MS	14951	4.0542	-	7470A	PPB	31 May 2017 11:16:38	U	SMPL
I3306-08 - 1	I3306-06MSD	14926	4.0474	-	7470A	PPB	31 May 2017 11:18:44	U	SMPL
CCV39 - 1	CCV39	18237	4.9381	-	7470A	PPB	31 May 2017 11:20:51	U	SMPL
CCB39 - 1	CCB39	146	0.0714	-	7470A	PPB	31 May 2017 11:22:58	U	SMPL
I3306-09 - 1	DSK-MW-LW	232	0.0946	-	7470A	PPB	31 May 2017 11:25:05	U	SMPL
I3306-11 - 1	DSK-MW-LN	-8	0.0300	-	7470A	PPB	31 May 2017 11:27:11	U	SMPL
I3340-09 - 1	265563	2636	0.7413	-	7470A	PPB	31 May 2017 11:29:18	U	SMPL
I3340-13 - 1	DRUM-1-DRUM-2-COMP	61327	16.5299	-	7470A	PPB	31 May 2017 11:31:25	U	SMPL
I3371-01 - 1	A598	594	0.1919	-	7470A	PPB	31 May 2017 11:33:33	U	SMPL
I3383-02 - 1	GROUNDWATER	376	0.1333	-	7470A	PPB	31 May 2017 11:35:42	U	SMPL
I3393-01 - 1	TW-01	871	0.2665	-	7470A	PPB	31 May 2017 11:37:50	U	SMPL
PB99381BL - 1	PBW	133	0.0679	-	7470A	PPB	31 May 2017 11:45:52	U	SMPL
PB99381BS - 1	LCSW	14339	3.8895	-	7470A	PPB	31 May 2017 11:48:00	U	SMPL
PB99381TB - 1	PB99342TB	215	0.0900	-	7470A	PPB	31 May 2017 11:50:07	U	SMPL
CCV40 - 1	CCV40	18131	4.9096	-	7470A	PPB	31 May 2017 11:52:14	U	SMPL
CCB40 - 1	CCB40	155	0.0738	-	7470A	PPB	31 May 2017 11:54:21	U	SMPL
I3383-01 - 1	SOILCUTTINGS	471	0.1588	-	7470A	PPB	31 May 2017 11:56:28	U	SMPL
I3388-05 - 1	WC-B43-B50-002	318	0.1177	-	7470A	PPB	31 May 2017 11:58:34	U	SMPL
I3388-06 - 1	WC-B29-B35-002	328	0.1204	-	7470A	PPB	31 May 2017 12:00:41	U	SMPL
I3388-06DUP - 1	WC-B29-B35-002DUP	244	0.0978	-	7470A	PPB	31 May 2017 12:02:48	U	SMPL
I3388-06MS - 1	WC-B29-B35-002MS	13468	3.6552	-	7470A	PPB	31 May 2017 12:04:56	U	SMPL
I3388-06MSD - 1	WC-B29-B35-002MSD	13320	3.6154	-	7470A	PPB	31 May 2017 12:07:04	U	SMPL
I3306-06LX5 - 1		135	0.0685	-	7470A	PPB	31 May 2017 12:09:12	U	SMPL
I3306-06A - 1		15068	4.0856	-	7470A	PPB	31 May 2017 12:11:20	U	SMPL
I3388-06LX5 - 1		166	0.0768	-	7470A	PPB	31 May 2017 12:13:29	U	SMPL
I3388-06A - 1		15662	4.2454	-	7470A	PPB	31 May 2017 12:15:36	U	SMPL
CCV41 - 1	CCV41	18285	4.9510	-	7470A	PPB	31 May 2017 12:17:43	U	SMPL
CCB41 - 1	CCB41	108	0.0612	-	7470A	PPB	31 May 2017 12:19:50	U	SMPL
I3340-13DLX5 - 1		11314	3.0758	-	7470A	PPB	31 May 2017 12:21:57	U	SMPL
CCV42 - 1	CCV42	18594	5.0342	-	7470A	PPB	31 May 2017 12:24:04	U	SMPL
CCB42 - 1	CCB42	245	0.0980	-	7470A	PPB	31 May 2017 12:26:11	U	SMPL