


7471A

LB87793
INSTRUMENT ID: CV1

Linear

 μ Abs.:

44937

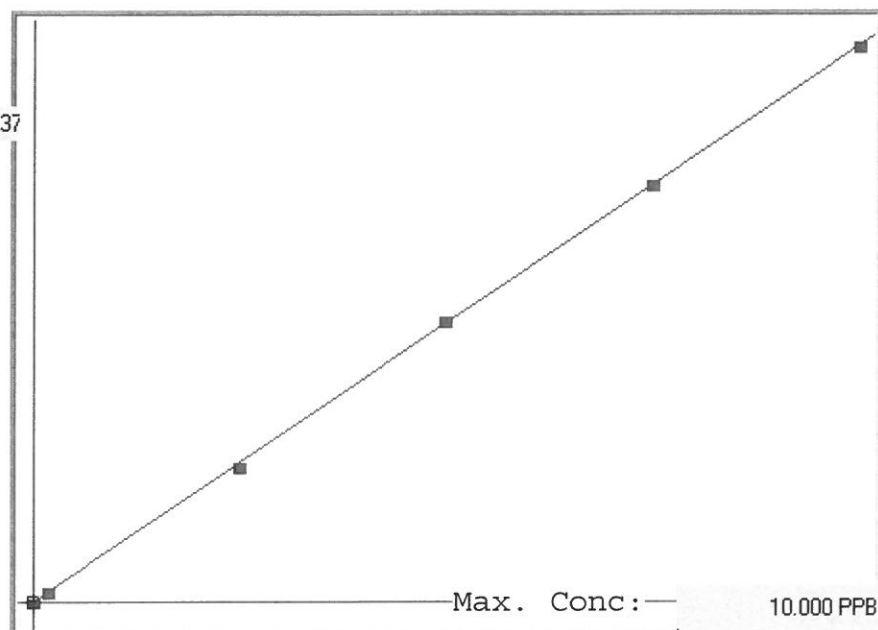

A= 0.0000e+000

B= 2.2188e-004

C= 4.0086e-003

Rho= 0.9999463

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.021	0.021	75	0.000	75				
0.2	0.200	0.193	-0.007	853	0.0 %	853				
2.5	2.500	2.438	-0.062	10969	0.0 %	10969				
5.0	5.000	5.060	0.060	22788	0.0 %	22788				
7.5	7.500	7.513	0.013	33843	0.0 %	33843				
10.0	10.000	9.975	-0.025	44937	0.0 %	44937				

LB87793 INSTRUMENT ID : CV1

Method: 7471A		Operator: Admin		Date of Analysis: 01 Jun 2017 12:55:00				
Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	75	-	0.00007471A	PPB	01 Jun 2017 14:04:04	S	Std
0.2 - 1	50-2	853	-	0.20007471A	PPB	01 Jun 2017 14:06:22	S	Std
2.5 - 1	52-5	10969	-	2.50007471A	PPB	01 Jun 2017 14:08:39	S	Std
5.0 - 1	55	22788	-	5.00007471A	PPB	01 Jun 2017 14:10:56	S	Std
7.5 - 1	57-5	33843	-	7.50007471A	PPB	01 Jun 2017 14:15:50	S	Std
10.0 - 1	510	44937	-	10.00007471A	PPB	01 Jun 2017 14:23:10	S	Std
ICV80 - 1	ICV80	17315	3.8459	-7471A	PPB	01 Jun 2017 14:25:49	U	SMPL
ICB80 - 1	ICB80	16	0.0076	-7471A	PPB	01 Jun 2017 14:28:05	U	SMPL
CCV48 - 1	CCV48	21448	4.7630	-7471A	PPB	01 Jun 2017 14:30:20	U	SMPL
CCB48 - 1	CCB48	-1	0.0038	-7471A	PPB	01 Jun 2017 14:32:36	U	SMPL
CRA - 1	CRA	841	0.1906	-7471A	PPB	01 Jun 2017 14:34:52	U	SMPL
HighStd - 1	HighStd	45350	10.0664	-7471A	PPB	01 Jun 2017 14:37:08	U	SMPL
ChkStd - 1	ChkStd	30646	6.8038	-7471A	PPB	01 Jun 2017 14:39:24	U	SMPL
PB99397BL - 1	PBS	-15	0.0007	-7471A	PPB	01 Jun 2017 14:41:41	U	SMPL
PB99397BS - 1	LCSS	15315	3.4021	-7471A	PPB	01 Jun 2017 14:43:57	U	SMPL
I3396-12 - 1	OIL-DRUM	76	0.0209	-7471A	PPB	01 Jun 2017 14:46:14	U	SMPL
I3405-01 - 1	R1-SB-1D1011	1517	0.3406	-7471A	PPB	01 Jun 2017 14:48:31	U	SMPL
I3405-02 - 1	R1-SB-2D1213	1393	0.3131	-7471A	PPB	01 Jun 2017 14:50:49	U	SMPL
I3405-03 - 1	R1-SB-3D910	1188	0.2676	-7471A	PPB	01 Jun 2017 14:53:07	U	SMPL
I3405-03DUP - 1	R1-SB-3D910DUP	1214	0.2734	-7471A	PPB	01 Jun 2017 14:55:23	U	SMPL
CCV49 - 1	CCV49	21754	4.8309	-7471A	PPB	01 Jun 2017 14:57:39	U	SMPL
CCB49 - 1	CCB49	24	0.0093	-7471A	PPB	01 Jun 2017 14:59:55	U	SMPL
I3405-03MS - 1	R1-SB-3D910MS	16758	3.7223	-7471A	PPB	01 Jun 2017 15:02:11	U	SMPL
I3405-03MSD - 1	R1-SB-3D910MSD	16717	3.7132	-7471A	PPB	01 Jun 2017 15:04:27	U	SMPL
I3405-04 - 1	R1-SB-4D12	4510	1.0047	-7471A	PPB	01 Jun 2017 15:06:43	U	SMPL
I3405-05 - 1	R1-SB-5D1314	3772	0.8410	-7471A	PPB	01 Jun 2017 15:09:00	U	SMPL
I3405-06 - 1	R1-SB-6D12	1550	0.3479	-7471A	PPB	01 Jun 2017 15:11:17	U	SMPL
I3412-01 - 1	TP-1-TP-2-COMP	4837	1.0773	-7471A	PPB	01 Jun 2017 15:13:34	U	SMPL
I3412-05 - 1	TP-3-TP-4-COMP	3049	0.6805	-7471A	PPB	01 Jun 2017 15:15:51	U	SMPL
I3412-09 - 1	TP-5-COMP	2230	0.4988	-7471A	PPB	01 Jun 2017 15:18:09	U	SMPL
I3413-01 - 1	R4-COMP	1129	0.2545	-7471A	PPB	01 Jun 2017 15:20:27	U	SMPL
I3415-01 - 1	E2-U6-SSW	43377	9.6286	-7471A	PPB	01 Jun 2017 15:22:43	U	SMPL
CCV50 - 1	CCV50	21592	4.7949	-7471A	PPB	01 Jun 2017 15:24:59	U	SMPL
CCB50 - 1	CCB50	23	0.0091	-7471A	PPB	01 Jun 2017 15:27:16	U	SMPL
I3415-02 - 1	E2-T6-BASE	427108	HIGH	-7471A	PPB	01 Jun 2017 15:29:32	X	
I3415-03 - 1	E2-T6-ESW	43850	9.7336	-7471A	PPB	01 Jun 2017 15:31:23	U	SMPL
I3415-04 - 1	E2-CONCRETE-BATCH-12	7828	1.7409	-7471A	PPB	01 Jun 2017 15:33:40	U	SMPL
I3420-01 - 1	TP-3-TP-4	421	0.0974	-7471A	PPB	01 Jun 2017 15:35:57	U	SMPL
I3420-06 - 1	TP-1-TP-2	1879	0.4209	-7471A	PPB	01 Jun 2017 15:38:14	U	SMPL
I3415-02DLX10 - 1		62879	13.9558	-7471A	PPB	01 Jun 2017 15:40:30	U	SMPL
I3405-03LX5 - 1		249	0.0593	-7471A	PPB	01 Jun 2017 15:42:48	U	SMPL
I3405-03A - 1		19513	4.3336	-7471A	PPB	01 Jun 2017 15:45:05	U	SMPL
I3415-02DL2X50 - 1		12467	2.7702	-7471A	PPB	01 Jun 2017 15:48:30	U	SMPL
CCV51 - 1	CCV51	21769	4.8342	-7471A	PPB	01 Jun 2017 15:50:45	U	SMPL
CCB51 - 1	CCB51	37	0.0122	-7471A	PPB	01 Jun 2017 15:53:02	U	SMPL