

LB87973

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

6/9/2017 10:13

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.586	0.0	0.095	
ICB1	0.538	0.0	0.004	
CCV1	238.217	0.0	0.231	
CCB1	0.684	0.0	0.004	
PB99611BL	0.481	0.0	0.004	
PB99611BS	96.654	0.0	0.096	
LOWPB99611	10.900	0.0	0.014	
HIGHPB99611	488.457	0.0	0.471	
I3559-15	0.795	0.0	0.004	
I3559-15DUP	3.361	0.0	0.007	
I3559-15MS	35.426	0.0	0.037	
I3559-15MSD	36.519	0.0	0.038	
I3563-01	0.574	0.0	0.004	
CCV2	255.876	0.0	0.248	
CCB2	0.238	0.0	0.004	

N	15
Mean	84.287
SD	140.2664
CV%	166.42

UB89973

Aquakem v. 7.2AQ1

Results from time period:

Fri Jun 09 09:05:39 2017

AK

Fri Jun 09 10:03:08 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.9839	µg/l	6/9/2017 9:05:39	
5.0PPBCN	A	Total CN	P	4.597	µg/l	6/9/2017 9:05:40	
10PPBCN	A	Total CN	P	10.5242	µg/l	6/9/2017 9:05:41	
50PPBCN	A	Total CN	P	49.2223	µg/l	6/9/2017 9:05:42	
100PPBCN	A	Total CN	P	99.576	µg/l	6/9/2017 9:05:43	
250PPBCN	A	Total CN	P	249.881	µg/l	6/9/2017 9:05:44	
500PPBCN	A	Total CN	P	500.2156	µg/l	6/9/2017 9:05:45	
ICV1	S	Total CN	P	95.5864	µg/l	6/9/2017 9:39:09	
ICB1	S	Total CN	P	0.5382	µg/l	6/9/2017 9:39:10	
CCV1	S	Total CN	P	238.2165	µg/l	6/9/2017 9:39:11	
CCB1	S	Total CN	P	0.6837	µg/l	6/9/2017 9:39:12	
PB99611BL	S	Total CN	P	0.4807	µg/l	6/9/2017 9:39:13	
PB99611BS	S	Total CN	P	96.6538	µg/l	6/9/2017 9:39:14	
LOWPB99611	S	Total CN	P	10.9	µg/l	6/9/2017 9:39:15	
HIGHPB99611	S	Total CN	P	488.4575	µg/l	6/9/2017 9:39:16	
I3559-15	S	Total CN	P	0.7945	µg/l	6/9/2017 9:39:17	
I3559-15DUP	S	Total CN	P	3.3606	µg/l	6/9/2017 9:39:18	
I3559-15MS	S	Total CN	P	35.4263	µg/l	6/9/2017 10:03:04	
I3559-15MSD	S	Total CN	P	36.5191	µg/l	6/9/2017 10:03:05	
I3563-01	S	Total CN	P	0.5735	µg/l	6/9/2017 10:03:06	
CCV2	S	Total CN	P	255.8763	µg/l	6/9/2017 10:03:07	
CCB2	S	Total CN	P	0.2381	µg/l	6/9/2017 10:03:08	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

6/9/2017 9:14


Test Total CN

Accepted 6/9/2017 9:14

Factor 1046
Bias 0.003

Coeff. of det. 0.999989

Errors

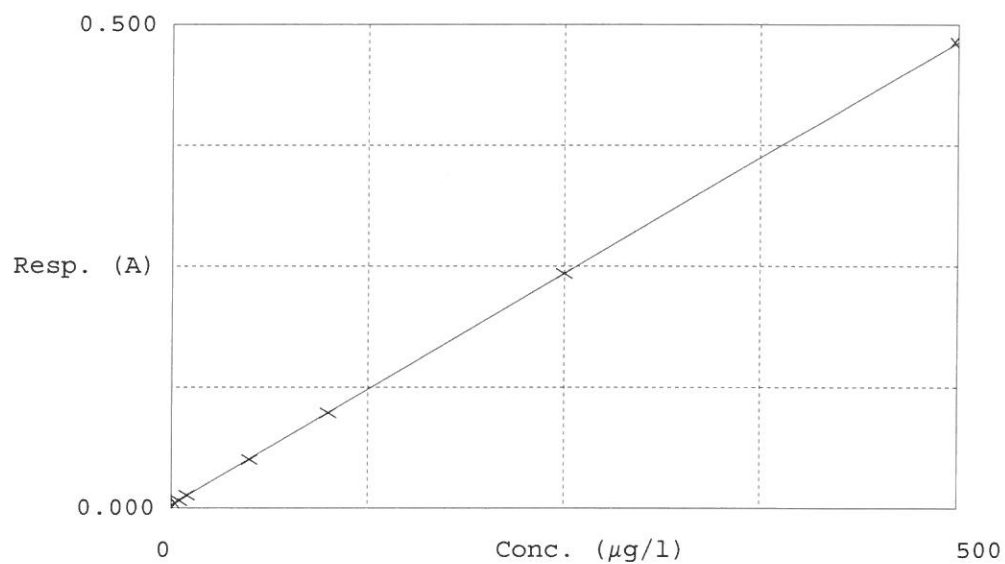

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.9839	0.0000	
2	5.0PPBCN	0.008	4.5970	5.0000	
3	10PPBCN	0.013	10.5242	10.0000	
4	50PPBCN	0.051	49.2223	50.0000	
5	100PPBCN	0.099	99.5760	100.0000	
6	250PPBCN	0.242	249.8810	250.0000	
7	500PPBCN	0.482	500.2156	500.0000	