


ISM02.4

LB88029
INSTRUMENT ID: CV2

Linear

 μ Abs.:

48584

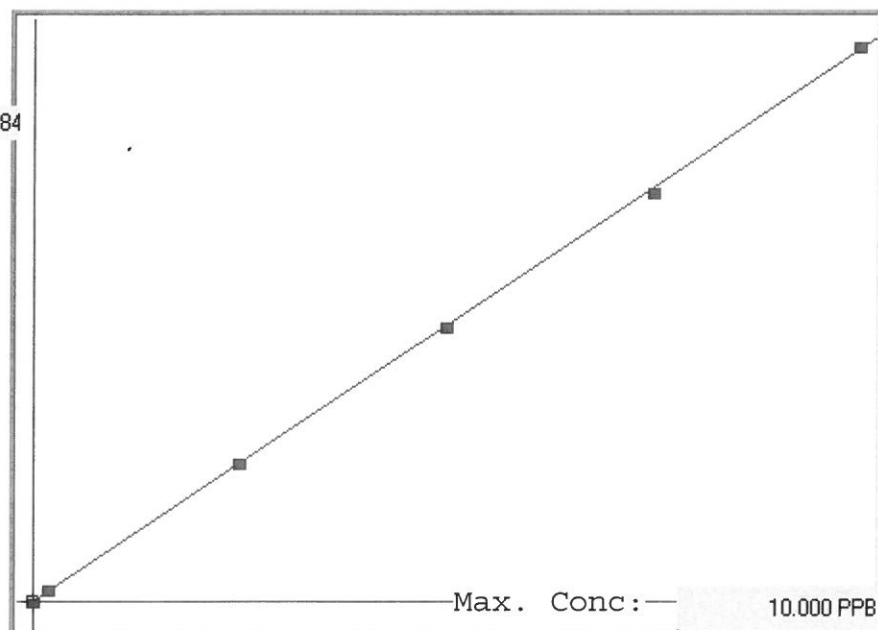

A= 0.0000e+000

B= 2.0695e-004

C= 2.4884e-003

Rho= 0.9999431

Accept=Accepted

slope
y=intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%OD
0.00	0.000	0.004	0.004	7	0.000	7					-
0.2	0.200	0.213	0.013	1016	0.0 %	1016					6
2.5	2.500	2.509	0.009	12112	0.0 %	12112					0
5.0	5.000	4.993	-0.007	24117	0.0 %	24117					0
7.5	7.500	7.424	-0.076	35862	0.0 %	35862					-1
10.0	10.000	10.057	0.057	48584	0.0 %	48584					1

RB
6/12/17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	7	-		0 ISM02.4	PPB	6/12/2017 17:54	Std
	0.2 S0.2	1016	-		0.2 ISM02.4	PPB	6/12/2017 17:57	Std
	2.5 S2.5	12112	-		2.5 ISM02.4	PPB	6/12/2017 17:59	Std
	5 S5	24117	-		5 ISM02.4	PPB	6/12/2017 18:01	Std
	7.5 S7.5	35862	-		7.5 ISM02.4	PPB	6/12/2017 18:04	Std
	10 S10	48584	-		10 ISM02.4	PPB	6/12/2017 18:06	Std
ICV	ICV	17454	3.6145 -		ISM02.4	PPB	6/12/2017 18:19	SMPL
ICB	ICB	-53	-0.0085 -		ISM02.4	PPB	6/12/2017 18:22	SMPL
CCV029	CCV029	22808	4.7225 -		ISM02.4	PPB	6/12/2017 18:24	SMPL
CCB029	CCB029	-52	-0.0083 -		ISM02.4	PPB	6/12/2017 18:26	SMPL
PB99688BL	PBS004	-5	0.0015 -		ISM02.4	PPB	6/12/2017 18:28	SMPL
I3572-01	MH2TR6	624	0.1316 -		ISM02.4	PPB	6/12/2017 18:31	SMPL
I3572-02	MH2TR6D	495	0.1049 -		ISM02.4	PPB	6/12/2017 18:33	SMPL
I3572-03	MH2TR6S	12014	2.4888 -		ISM02.4	PPB	6/12/2017 18:35	SMPL
CCV030	CCV030	22800	4.7209 -		ISM02.4	PPB	6/12/2017 18:37	SMPL
CCB030	CCB030	-51	-0.0081 -		ISM02.4	PPB	6/12/2017 18:40	SMPL