


7470A

LB88140
INSTRUMENT ID: CV2

Linear

 μ Abs.:

36915

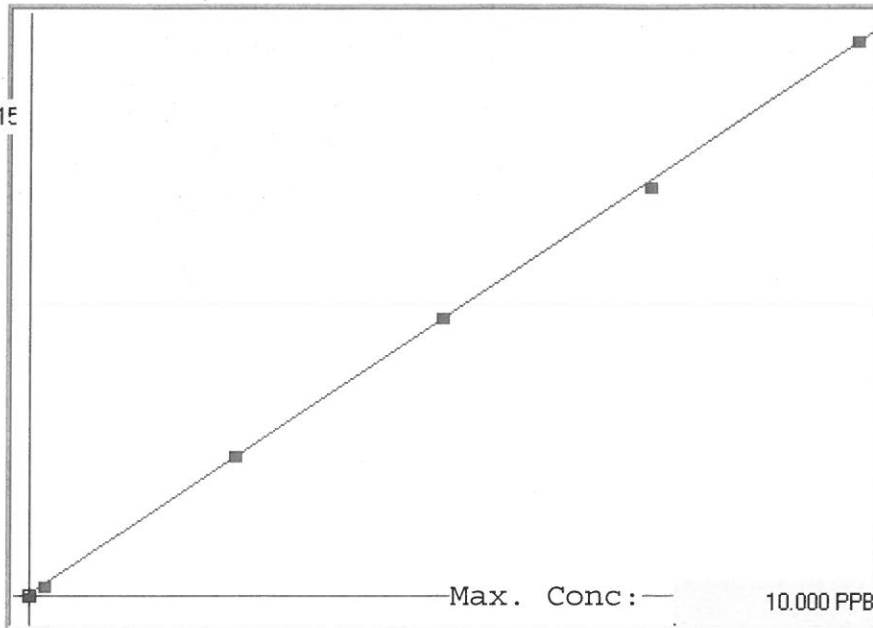

A= 0.0000e+000

B= 2.7216e-004

C= -1.2962e-002

Rho= 0.9999204

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.012	-0.012	2	0.000	2				
0.2	0.200	0.184	-0.016	724	0.0 %	724				
2.5	2.500	2.539	0.039	9378	0.0 %	9378				
5.0	5.000	5.044	0.044	18581	0.0 %	18581				
7.5	7.500	7.411	-0.089	27277	0.0 %	27277				
10.0	10.000	10.034	0.034	36915	0.0 %	36915				

LB88140 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Jun 2017 14:10:35

Sample ID	Extended ID	µ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	2	-	0.00007470A	PPB		16 Jun 2017 14:13:09	S	Std
0.2 - 1	50.2	724	-	0.20007470A	PPB		16 Jun 2017 14:15:17	S	Std
2.5 - 1	52.5	9378	-	2.50007470A	PPB		16 Jun 2017 14:17:25	S	Std
5.0 - 1	55	18581	-	5.00007470A	PPB		16 Jun 2017 14:19:33	S	Std
7.5 - 1	57.5	27277	-	7.50007470A	PPB		16 Jun 2017 14:21:41	S	Std
10.0 - 1	510	36915	-	10.00007470A	PPB		16 Jun 2017 14:23:48	S	Std
ICV03 - 1	ICV03	14088	3.8213	-7470A	PPB		16 Jun 2017 14:26:17	U	SMPL
ICB03 - 1	ICB03	-48	-0.0260	-7470A	PPB		16 Jun 2017 14:28:23	U	SMPL
CCV65 - 1	CCV65	18405	4.9962	-7470A	PPB		16 Jun 2017 14:30:29	U	SMPL
CCB65 - 1	CCB65	-61	-0.0296	-7470A	PPB		16 Jun 2017 14:32:36	U	SMPL
CRA - 1	CRA	660	0.1667	-7470A	PPB		16 Jun 2017 14:34:42	U	SMPL
HighStd - 1	HighStd	35928	9.7653	-7470A	PPB		16 Jun 2017 14:36:49	U	SMPL
ChkStd - 1	ChkStd	26518	7.2043	-7470A	PPB		16 Jun 2017 14:38:56	U	SMPL
PB99807BL - 1	PBW	-56	-0.0282	-7470A	PPB		16 Jun 2017 14:41:04	U	SMPL
PB99807BS - 1	LCSW	14608	3.9628	-7470A	PPB		16 Jun 2017 14:43:11	U	SMPL
I3644-01 - 1	DRUMS-M47409-COMP	20180	5.4793	-7470A	PPB		16 Jun 2017 14:45:19	U	SMPL
I3661-01 - 1	FT-265434-265578-COMP	-62	-0.0298	-7470A	PPB		16 Jun 2017 14:47:27	U	SMPL
I3672-01 - 1	MW-3D-R2	-28	-0.0206	-7470A	PPB		16 Jun 2017 14:49:35	U	SMPL
I3672-02 - 1	MW-3-R2	-28	-0.0206	-7470A	PPB		16 Jun 2017 14:51:44	U	SMPL
I3672-02DUP - 1	MW-3-R2DUP	-24	-0.0195	-7470A	PPB		16 Jun 2017 14:53:50	U	SMPL
CCV66 - 1	CCV66	18266	4.9584	-7470A	PPB		16 Jun 2017 14:55:57	U	SMPL
CCB66 - 1	CCB66	-39	-0.0236	-7470A	PPB		16 Jun 2017 14:58:04	U	SMPL
I3672-02MS - 1	MW-3-R2MS	14879	4.0366	-7470A	PPB		16 Jun 2017 15:00:11	U	SMPL
I3672-02MSD - 1	MW-3-R2MSD	14693	3.9859	-7470A	PPB		16 Jun 2017 15:02:18	U	SMPL
I3672-03 - 1	MW-2-R2	-33	-0.0219	-7470A	PPB		16 Jun 2017 15:04:25	U	SMPL
I3672-04 - 1	MW-2D-R2	-42	-0.0244	-7470A	PPB		16 Jun 2017 15:06:32	U	SMPL
I3672-05 - 1	MW-6A-R2	-56	-0.0282	-7470A	PPB		16 Jun 2017 15:08:39	U	SMPL
I3672-06 - 1	MW-6B-R2	-52	-0.0271	-7470A	PPB		16 Jun 2017 15:10:47	U	SMPL
I3672-07 - 1	FB-061217	-67	-0.0312	-7470A	PPB		16 Jun 2017 15:12:54	U	SMPL
I3672-08 - 1	MW-4A-R2	130	0.0224	-7470A	PPB		16 Jun 2017 15:15:03	U	SMPL
I3672-09 - 1	MW-4D-R2	-57	-0.0285	-7470A	PPB		16 Jun 2017 15:17:12	U	SMPL
I3672-10 - 1	MW-5A-R2	-115	-0.0443	-7470A	PPB		16 Jun 2017 15:19:18	U	SMPL
CCV67 - 1	CCV67	18046	4.8985	-7470A	PPB		16 Jun 2017 15:21:25	U	SMPL
CCB67 - 1	CCB67	-45	-0.0252	-7470A	PPB		16 Jun 2017 15:23:33	U	SMPL
I3672-11 - 1	MW-5B-R2	-25	-0.0198	-7470A	PPB		16 Jun 2017 15:25:39	U	SMPL
I3672-12 - 1	MW-5D-R2	-15	-0.0170	-7470A	PPB		16 Jun 2017 15:27:46	U	SMPL
I3672-13 - 1	MW-1-R2	-27	-0.0203	-7470A	PPB		16 Jun 2017 15:29:53	U	SMPL
I3672-14 - 1	MW-1D-R2	-9	-0.0154	-7470A	PPB		16 Jun 2017 15:32:00	U	SMPL
I3672-15 - 1	DUP-R2	-23	-0.0192	-7470A	PPB		16 Jun 2017 15:34:08	U	SMPL
I3672-16 - 1	FB-061317	-52	-0.0271	-7470A	PPB		16 Jun 2017 15:36:15	U	SMPL
I3691-01 - 1	A1013	1091	0.2840	-7470A	PPB		16 Jun 2017 15:38:24	U	SMPL
I3725-01 - 1	A-598-FRAC-TANK	-50	-0.0266	-7470A	PPB		16 Jun 2017 15:40:32	U	SMPL
PB99808BL - 1	PBW	-2	-0.0135	-7470A	PPB		16 Jun 2017 15:42:40	U	SMPL
PB99808BS - 1	LCSW	15289	4.1482	-7470A	PPB		16 Jun 2017 15:44:47	U	SMPL
CCV68 - 1	CCV68	18064	4.9034	-7470A	PPB		16 Jun 2017 15:46:55	U	SMPL
CCB68 - 1	CCB68	-58	-0.0287	-7470A	PPB		16 Jun 2017 15:49:02	U	SMPL
PB99808TB - 1	PB99791TB	-4	-0.0141	-7470A	PPB		16 Jun 2017 15:51:09	U	SMPL
I3661-04 - 1	FT-265434-265578-COMP	-7	-0.0149	-7470A	PPB		16 Jun 2017 15:53:16	U	SMPL
I3661-04DUP - 1	FT-265434-265578-COMPDUP	-1	-0.0132	-7470A	PPB		16 Jun 2017 15:55:23	U	SMPL
I3661-04MS - 1	FT-265434-265578-COMPMS	15022	4.0755	-7470A	PPB		16 Jun 2017 15:57:30	U	SMPL
I3661-04MSD - 1	FT-265434-265578-COMPMSD	13876	3.7636	-7470A	PPB		16 Jun 2017 15:59:38	U	SMPL
I3680-03 - 1	TR-05-061317	-66	-0.0309	-7470A	PPB		16 Jun 2017 16:01:45	U	SMPL
I3681-06 - 1	RO-272031-72-11978-COMP	-10	-0.0157	-7470A	PPB		16 Jun 2017 16:03:53	U	SMPL
I3684-03 - 1	ROCKY-ROAD-COMP	-11	-0.0160	-7470A	PPB		16 Jun 2017 16:06:01	U	SMPL
I3684-07 - 1	SOIL-ROAD-COMP	-14	-0.0168	-7470A	PPB		16 Jun 2017 16:08:09	U	SMPL
I3689-07 - 1	BAYWAY-SWITCH-A	0	-0.0130	-7470A	PPB		16 Jun 2017 16:10:16	U	SMPL
CCV69 - 1	CCV69	18294	4.9660	-7470A	PPB		16 Jun 2017 16:12:23	U	SMPL
CCB69 - 1	CCB69	-54	-0.0277	-7470A	PPB		16 Jun 2017 16:14:30	U	SMPL
I3689-14 - 1	BAYWAY-SWITCH-B	88	0.0110	-7470A	PPB		16 Jun 2017 16:16:38	U	SMPL
I3691-02 - 1	A1013	-26	-0.0200	-7470A	PPB		16 Jun 2017 16:18:45	U	SMPL
I3672-02LX5 - 1		-29	-0.0209	-7470A	PPB		16 Jun 2017 16:20:52	U	SMPL
I3672-02A - 1		14712	3.9911	-7470A	PPB		16 Jun 2017 16:22:59	U	SMPL
I3661-04LX5 - 1		-33	-0.0219	-7470A	PPB		16 Jun 2017 16:25:06	U	SMPL
I3661-04A - 1		14420	3.9116	-7470A	PPB		16 Jun 2017 16:27:14	U	SMPL
CCV70 - 1	CCV70	18542	5.0335	-7470A	PPB		16 Jun 2017 16:29:22	U	SMPL
CCB70 - 1	CCB70	-49	-0.0263	-7470A	PPB		16 Jun 2017 16:31:30	U	SMPL