


7470A

LB88172
INSTRUMENT ID: CV4

Linear

 μ Abs.:

37549

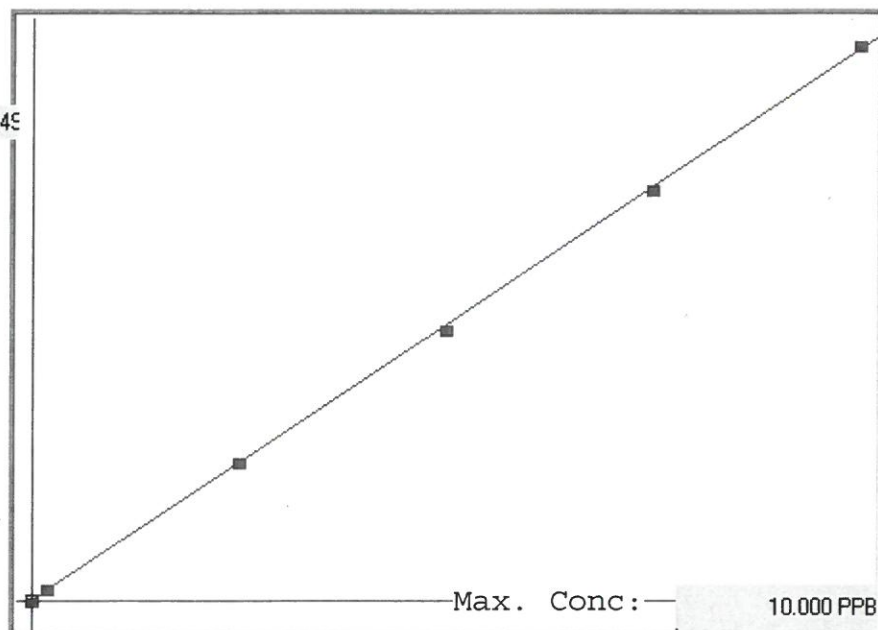

A= 0.0000e+000

B= 2.6810e-004

C= -3.3794e-003

Rho= 0.9999237

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.021	0.021	91	0.000	91				
0.2	0.200	0.219	0.019	828	0.0 %	828				
2.5	2.500	2.514	0.014	9389	0.0 %	9389				
5.0	5.000	4.923	-0.077	18377	0.0 %	18377				
7.5	7.500	7.460	-0.040	27838	0.0 %	27838				
10.0	10.000	10.063	0.063	37549	0.0 %	37549				

LB88172 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 19 Jun 2017 09:22:02

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc.	Method	Units	Date	Type	Type
0.0 - 1	80	91	-	0.0000	7470A	PPB	19 Jun 2017 10:54:46	S	Std
0.2 - 1	50.2	828	-	0.2000	7470A	PPB	19 Jun 2017 10:56:55	S	Std
2.5 - 1	52.5	9389	-	2.5000	7470A	PPB	19 Jun 2017 10:59:03	S	Std
5.0 - 1	55	18377	-	5.0000	7470A	PPB	19 Jun 2017 11:01:11	S	Std
7.5 - 1	57.5	27838	-	7.5000	7470A	PPB	19 Jun 2017 11:03:19	S	Std
10.0 - 1	510	37549	-	10.0000	7470A	PPB	19 Jun 2017 11:05:26	S	Std
ICV04 - 1	ICV04	15065	4.0355	-	7470A	PPB	19 Jun 2017 11:08:02	U	SMPL
ICB04 - 1	ICB04	81	0.0183	-	7470A	PPB	19 Jun 2017 11:10:08	U	SMPL
CCV71 - 1	CCV71	19348	5.1837	-	7470A	PPB	19 Jun 2017 11:12:15	U	SMPL
CCB71 - 1	CCB71	107	0.0253	-	7470A	PPB	19 Jun 2017 11:14:22	U	SMPL
CRA - 1	CRA	839	0.2216	-	7470A	PPB	19 Jun 2017 11:16:28	U	SMPL
HighStd - 1	HighStd	37322	10.0025	-	7470A	PPB	19 Jun 2017 11:18:35	U	SMPL
ChkStd - 1	ChkStd	25373	6.7990	-	7470A	PPB	19 Jun 2017 11:20:42	U	SMPL
PB99861BL - 1	PBW	60	0.0127	-	7470A	PPB	19 Jun 2017 11:22:49	U	SMPL
PB99861BS - 1	LCSW	14303	3.8312	-	7470A	PPB	19 Jun 2017 11:24:57	U	SMPL
PB99861TB - 1	PB99810TB	63	0.0135	-	7470A	PPB	19 Jun 2017 11:27:05	U	SMPL
I3693-03 - 1	PL-01-061417-A	80	0.0181	-	7470A	PPB	19 Jun 2017 11:29:13	U	SMPL
I3693-06 - 1	PL-01-061417-B	78	0.0175	-	7470A	PPB	19 Jun 2017 11:31:21	U	SMPL
I3693-09 - 1	PL-01-061417-C	49	0.0098	-	7470A	PPB	19 Jun 2017 11:33:30	U	SMPL
I3693-12 - 1	PL-01-061417-D	52	0.0106	-	7470A	PPB	19 Jun 2017 11:35:37	U	SMPL
CCV72 - 1	CCV72	19310	5.1735	-	7470A	PPB	19 Jun 2017 11:37:43	U	SMPL
CCB72 - 1	CCB72	26	0.0036	-	7470A	PPB	19 Jun 2017 11:39:49	U	SMPL
I3694-03 - 1	NB-08-061417-A	81	0.0183	-	7470A	PPB	19 Jun 2017 11:41:56	U	SMPL
I3694-03DUP - 1	NB-08-061417-ADUP	99	0.0232	-	7470A	PPB	19 Jun 2017 11:44:02	U	SMPL
I3694-03MS - 1	NB-08-061417-AMS	13956	3.7382	-	7470A	PPB	19 Jun 2017 11:46:09	U	SMPL
I3694-03MSD - 1	NB-08-061417-AMSD	13691	3.6671	-	7470A	PPB	19 Jun 2017 11:48:16	U	SMPL
I3694-06 - 1	NB-08-061417-B	100	0.0234	-	7470A	PPB	19 Jun 2017 11:50:23	U	SMPL
I3694-09 - 1	NB-08-061417-C	94	0.0218	-	7470A	PPB	19 Jun 2017 11:52:31	U	SMPL
I3695-03 - 1	BU-02-061417	94	0.0218	-	7470A	PPB	19 Jun 2017 11:54:39	U	SMPL
I3696-03 - 1	NB-RO-72-11935	89	0.0205	-	7470A	PPB	19 Jun 2017 11:56:47	U	SMPL
I3725-02 - 1	A-598-FRAC-TANK	78	0.0175	-	7470A	PPB	19 Jun 2017 11:58:56	U	SMPL
PB99862BL - 1	PBW	87	0.0199	-	7470A	PPB	19 Jun 2017 12:01:03	U	SMPL
CCV73 - 1	CCV73	19323	5.1770	-	7470A	PPB	19 Jun 2017 12:03:09	U	SMPL
CCB73 - 1	CCB73	25	0.0033	-	7470A	PPB	19 Jun 2017 12:05:16	U	SMPL
PB99862BS - 1	LCSW	15019	4.0231	-	7470A	PPB	19 Jun 2017 12:07:23	U	SMPL
I3657-01 - 1	MW-FIELDBLANK	21	0.0023	-	7470A	PPB	19 Jun 2017 12:09:30	U	SMPL
I3657-02 - 1	MW-106S	78	0.0175	-	7470A	PPB	19 Jun 2017 12:11:36	U	SMPL
I3657-03 - 1	MW-106I	87	0.0199	-	7470A	PPB	19 Jun 2017 12:13:43	U	SMPL
I3657-04 - 1	MW-106D	97	0.0226	-	7470A	PPB	19 Jun 2017 12:15:50	U	SMPL
I3657-05 - 1	MW-107S	54	0.0111	-	7470A	PPB	19 Jun 2017 12:17:58	U	SMPL
I3657-07 - 1	MW-104I	97	0.0226	-	7470A	PPB	19 Jun 2017 12:20:05	U	SMPL
I3657-08 - 1	MW-104D	234	0.0594	-	7470A	PPB	19 Jun 2017 12:22:14	U	SMPL
I3657-09 - 1	MW-105S	74	0.0165	-	7470A	PPB	19 Jun 2017 12:24:22	U	SMPL
I3657-10 - 1	MW-105I	129	0.0312	-	7470A	PPB	19 Jun 2017 12:26:29	U	SMPL
CCV74 - 1	CCV74	18720	5.0154	-	7470A	PPB	19 Jun 2017 12:28:36	U	SMPL
CCB74 - 1	CCB74	68	0.0149	-	7470A	PPB	19 Jun 2017 12:30:43	U	SMPL
I3657-11 - 1	MW-105D	72	0.0159	-	7470A	PPB	19 Jun 2017 12:32:50	U	SMPL
I3657-12 - 1	MW-103S	109	0.0258	-	7470A	PPB	19 Jun 2017 12:34:57	U	SMPL
I3657-13 - 1	MW-103I	93	0.0216	-	7470A	PPB	19 Jun 2017 12:37:04	U	SMPL
I3657-14 - 1	MW-103D	52	0.0106	-	7470A	PPB	19 Jun 2017 12:39:11	U	SMPL
I3657-14DUP - 1	MW-103DDUP	34	0.0057	-	7470A	PPB	19 Jun 2017 12:41:19	U	SMPL
I3657-15 - 1	I3657-14MS	16113	4.3164	-	7470A	PPB	19 Jun 2017 12:43:26	U	SMPL
I3657-16 - 1	I3657-14MSD	15612	4.1821	-	7470A	PPB	19 Jun 2017 12:45:34	U	SMPL
I3657-20 - 1	MW-102S	-95	-0.0288	-	7470A	PPB	19 Jun 2017 12:47:42	U	SMPL
I3657-21 - 1	MW-102I	-21	-0.0090	-	7470A	PPB	19 Jun 2017 12:49:51	U	SMPL
I3657-22 - 1	MW-102D	-30	-0.0114	-	7470A	PPB	19 Jun 2017 12:51:58	U	SMPL
CCV75 - 1	CCV75	18054	4.8368	-	7470A	PPB	19 Jun 2017 12:54:05	U	SMPL
CCB75 - 1	CCB75	-104	-0.0313	-	7470A	PPB	19 Jun 2017 12:56:11	U	SMPL
I3657-23 - 1	MW-101S	706	0.1859	-	7470A	PPB	19 Jun 2017 12:58:19	U	SMPL
I3694-03LX5 - 1		-51	-0.0171	-	7470A	PPB	19 Jun 2017 13:00:26	U	SMPL
I3694-03A - 1		13976	3.7435	-	7470A	PPB	19 Jun 2017 13:02:33	U	SMPL
I3657-14LX5 - 1		-56	-0.0184	-	7470A	PPB	19 Jun 2017 13:18:13	U	SMPL
I3657-14A - 1		15092	4.0427	-	7470A	PPB	19 Jun 2017 13:20:19	U	SMPL
CCV76 - 1	CCV76	18684	5.0057	-	7470A	PPB	19 Jun 2017 13:22:27	U	SMPL
CCB76 - 1	CCB76	-75	-0.0235	-	7470A	PPB	19 Jun 2017 13:24:35	U	SMPL