


7470A

LB88426
INSTRUMENT ID: CV1

Linear

 μ Abs.:

41551

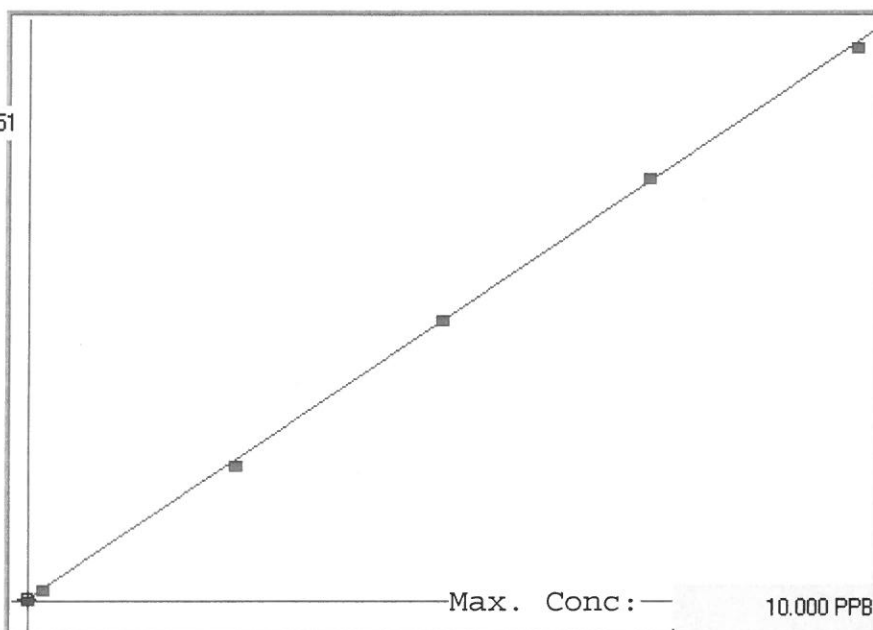

A= 0.0000e+000

B= 2.3925e-004

C= -2.8347e-002

Rho= 0.9998433

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.016	0.016	184	0.000	184				
0.2	0.200	0.183	-0.017	885	0.0 %	885				
2.5	2.500	2.432	-0.068	10284	0.0 %	10284				
5.0	5.000	5.060	0.060	21269	0.0 %	21269				
7.5	7.500	7.596	0.096	31868	0.0 %	31868				
10.0	10.000	9.913	-0.087	41551	0.0 %	41551				

LB88426 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Jun 2017 10:45:12				
Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	S0	184	-	0.0000	7470A	PPB	29 Jun 2017 10:50:30	S Std
0.2 - 1	S0.2	885	-	0.2000	7470A	PPB	29 Jun 2017 10:52:39	S Std
2.5 - 1	S2.5	10284	-	2.5000	7470A	PPB	29 Jun 2017 10:54:47	S Std
5.0 - 1	S5	21269	-	5.0000	7470A	PPB	29 Jun 2017 10:56:55	S Std
7.5 - 1	S7.5	31868	-	7.5000	7470A	PPB	29 Jun 2017 11:04:24	S Std
10.0 - 1	S10	41551	-	10.0000	7470A	PPB	29 Jun 2017 11:06:31	S Std
ICV44 - 1	ICV44	15842	3.7618	-	7470A	PPB	29 Jun 2017 11:09:06	U SMPL
ICB44 - 1	ICB44	98	-0.0049	-	7470A	PPB	29 Jun 2017 11:11:12	U SMPL
CCV87 - 1	CCV87	20855	4.9612	-	7470A	PPB	29 Jun 2017 11:13:20	U SMPL
CCB87 - 1	CCB87	114	-0.0011	-	7470A	PPB	29 Jun 2017 11:15:26	U SMPL
CRA - 1	CRA	915	0.1906	-	7470A	PPB	29 Jun 2017 11:17:34	U SMPL
HighStd - 1	HighStd	41621	9.9294	-	7470A	PPB	29 Jun 2017 11:19:40	U SMPL
ChkStd - 1	ChkStd	29291	6.9795	-	7470A	PPB	29 Jun 2017 11:21:47	U SMPL
PB100245BL - 1	PBW	-120	-0.0571	-	7470A	PPB	29 Jun 2017 11:23:56	U SMPL
PB100245BS - 1	LCSW	16951	4.0271	-	7470A	PPB	29 Jun 2017 11:26:05	U SMPL
PB100245TB - 1	PB100211TB	-110	-0.0547	-	7470A	PPB	29 Jun 2017 11:28:13	U SMPL
I3930-13 - 1	B2-0-2	-53	-0.0410	-	7470A	PPB	29 Jun 2017 11:30:21	U SMPL
I3930-13DUP - 1	B2-0-2DUP	5	-0.0272	-	7470A	PPB	29 Jun 2017 11:32:29	U SMPL
I3930-13MS - 1	B2-0-2MS	14527	3.4472	-	7470A	PPB	29 Jun 2017 11:34:38	U SMPL
I3930-13MSD - 1	B2-0-2MSD	15870	3.7685	-	7470A	PPB	29 Jun 2017 11:36:45	U SMPL
CCV88 - 1	CCV88	21415	5.0951	-	7470A	PPB	29 Jun 2017 11:38:51	U SMPL
CCB88 - 1	CCB88	90	-0.0068	-	7470A	PPB	29 Jun 2017 11:40:59	U SMPL
I3930-14 - 1	B2-2-4	-42	-0.0384	-	7470A	PPB	29 Jun 2017 11:43:06	U SMPL
I3930-15 - 1	B2-4-6	-23	-0.0338	-	7470A	PPB	29 Jun 2017 11:45:13	U SMPL
I3930-16 - 1	B2-6-8	17	-0.0243	-	7470A	PPB	29 Jun 2017 11:47:19	U SMPL
I3930-17 - 1	B2-8-10	35	-0.0200	-	7470A	PPB	29 Jun 2017 11:49:27	U SMPL
I3930-18 - 1	B2-10-12.5	53	-0.0157	-	7470A	PPB	29 Jun 2017 11:51:35	U SMPL
I3930-19 - 1	B2-12.5-15	22	-0.0231	-	7470A	PPB	29 Jun 2017 11:53:42	U SMPL
I3930-20 - 1	B3-0-2	17	-0.0243	-	7470A	PPB	29 Jun 2017 11:55:50	U SMPL
I3930-21 - 1	B3-2-4	-16	-0.0322	-	7470A	PPB	29 Jun 2017 11:57:58	U SMPL
I3930-22 - 1	B3-4-6	9	-0.0262	-	7470A	PPB	29 Jun 2017 12:00:06	U SMPL
I3930-23 - 1	B3-6-8.5	-38	-0.0374	-	7470A	PPB	29 Jun 2017 12:02:13	U SMPL
CCV89 - 1	CCV89	20880	4.9671	-	7470A	PPB	29 Jun 2017 12:04:20	U SMPL
CCB89 - 1	CCB89	143	0.0059	-	7470A	PPB	29 Jun 2017 12:06:27	U SMPL
I3930-24 - 1	B3-8.5-11	32	-0.0207	-	7470A	PPB	29 Jun 2017 12:08:35	U SMPL
I3935-03 - 1	JFK-SOIL-06-26-17(COMPOSITE)	89	-0.0071	-	7470A	PPB	29 Jun 2017 12:10:42	U SMPL
I3937-01 - 1	ATP-2(B)	70	-0.0116	-	7470A	PPB	29 Jun 2017 12:12:48	U SMPL
I3941-02 - 1	LSS-DEBRIS-COMP	18	-0.0240	-	7470A	PPB	29 Jun 2017 12:14:55	U SMPL
I3941-04 - 1	LSS-STONE-COMP-1	-5	-0.0295	-	7470A	PPB	29 Jun 2017 12:17:03	U SMPL
I3941-06 - 1	LSS-STONE-COMP-2	0	-0.0283	-	7470A	PPB	29 Jun 2017 12:19:11	U SMPL
I3947-02 - 1	TP1-TP2-COMP	14	-0.0250	-	7470A	PPB	29 Jun 2017 12:21:19	U SMPL
I3949-05 - 1	TP-H1-(0-8)	105	-0.0032	-	7470A	PPB	29 Jun 2017 12:23:27	U SMPL
I3949-11 - 1	TP-C2-(0-8)	82	-0.0087	-	7470A	PPB	29 Jun 2017 12:25:36	U SMPL
I3951-02 - 1	DUCT-BANK	69	-0.0118	-	7470A	PPB	29 Jun 2017 12:27:43	U SMPL
CCV90 - 1	CCV90	20737	4.9329	-	7470A	PPB	29 Jun 2017 12:29:50	U SMPL
CCB90 - 1	CCB90	256	0.0329	-	7470A	PPB	29 Jun 2017 12:31:57	U SMPL
I3952-05 - 1	23MC-WC-2(COMP)	129	0.0025	-	7470A	PPB	29 Jun 2017 12:34:05	U SMPL
I3955-02 - 1	A1022C	87	-0.0075	-	7470A	PPB	29 Jun 2017 12:36:12	U SMPL
I3930-13LX5 - 1		216	0.0233	-	7470A	PPB	29 Jun 2017 12:38:19	U SMPL
I3930-13A - 1		16243	3.8578	-	7470A	PPB	29 Jun 2017 12:40:26	U SMPL
CCV91 - 1	CCV91	21034	5.0040	-	7470A	PPB	29 Jun 2017 12:42:34	U SMPL
CCB91 - 1	CCB91	173	0.0130	-	7470A	PPB	29 Jun 2017 12:44:41	U SMPL