

L388692


7470A

INSTRUMENT ID: CV1

Linear

μ Abs.:

32945

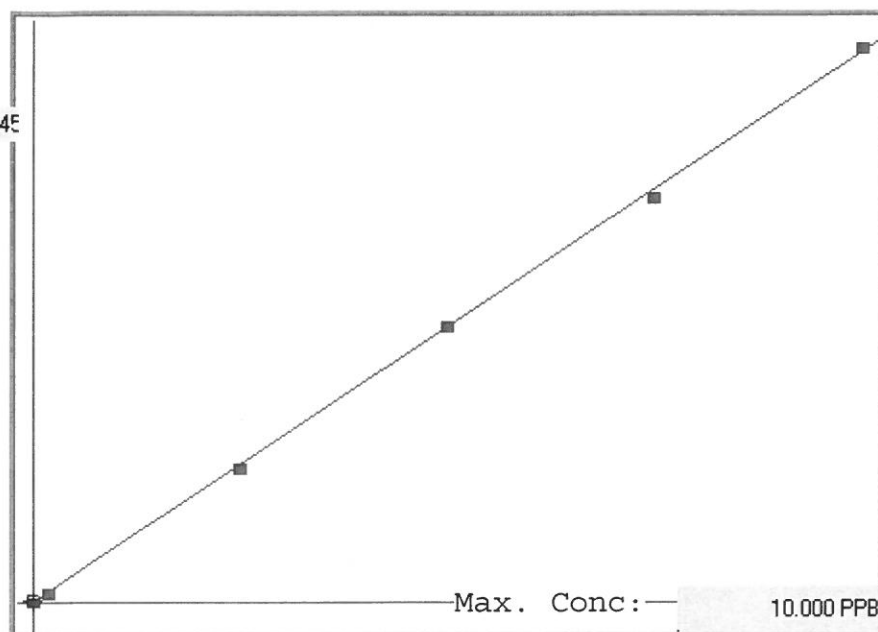

A= 0.0000e+000

B= 3.0590e-004

C= 5.0926e-003

Rho= 0.9998256

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.046	0.046	134	0.000	134				
0.2	0.200	0.194	-0.006	618	0.0 %	618				
2.5	2.500	2.467	-0.033	8047	0.0 %	8047				
5.0	5.000	5.040	0.040	16459	0.0 %	16459				
7.5	7.500	7.370	-0.130	24078	0.0 %	24078				
10.0	10.000	10.083	0.083	32945	0.0 %	32945				

LB88692 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Jul 2017 13:56:54

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	134	-	0.00007470A	PPB		13 Jul 2017 13:59:22	S	Std
0.2 - 1	50.2	618	-	0.20007470A	PPB		13 Jul 2017 14:01:31	S	Std
2.5 - 1	52.5	8047	-	2.50007470A	PPB		13 Jul 2017 14:03:39	S	Std
5.0 - 1	55	16459	-	5.00007470A	PPB		13 Jul 2017 14:05:47	S	Std
7.5 - 1	57.5	24078	-	7.50007470A	PPB		13 Jul 2017 14:07:56	S	Std
10.0 - 1	510	32945	-	10.00007470A	PPB		13 Jul 2017 14:10:04	S	Std
ICV61 - 1	ICV61	12999	3.9814	-7470A	PPB		13 Jul 2017 14:12:37	U	SMPL
ICB61 - 1	ICB61	-49	-0.0099	-7470A	PPB		13 Jul 2017 14:14:43	U	SMPL
CCV13 - 1	CCV13	16353	5.0074	-7470A	PPB		13 Jul 2017 14:16:51	U	SMPL
CCB13 - 1	CCB13	-7	0.0030	-7470A	PPB		13 Jul 2017 14:18:57	U	SMPL
CRA - 1	CRA	636	0.1996	-7470A	PPB		13 Jul 2017 14:21:04	U	SMPL
HighStd - 1	HighStd	33086	10.1260	-7470A	PPB		13 Jul 2017 14:23:11	U	SMPL
ChkStd - 1	ChkStd	23120	7.0774	-7470A	PPB		13 Jul 2017 14:25:18	U	SMPL
PB100615BL - 1	PBW	83	0.0305	-7470A	PPB		13 Jul 2017 14:27:27	U	SMPL
PB100615BS - 1	LCSW	13243	4.0561	-7470A	PPB		13 Jul 2017 14:29:35	U	SMPL
I4145-09 - 1	BASEMENT-WATER	1280	0.3966	-7470A	PPB		13 Jul 2017 14:31:43	U	SMPL
I4150-01 - 1	A3591	2502	0.7704	-7470A	PPB		13 Jul 2017 14:33:51	U	SMPL
I4157-02 - 1	TD071117-2-2S	176	0.0589	-7470A	PPB		13 Jul 2017 14:36:00	U	SMPL
I4157-02DUP - 1	TD071117-2-2SDUP	174	0.0583	-7470A	PPB		13 Jul 2017 14:38:08	U	SMPL
I4157-02MS - 1	TD071117-2-2SMS	12865	3.9404	-7470A	PPB		13 Jul 2017 14:40:15	U	SMPL
CCV14 - 1	CCV14	16340	5.0034	-7470A	PPB		13 Jul 2017 14:42:22	U	SMPL
CCB14 - 1	CCB14	-9	0.0023	-7470A	PPB		13 Jul 2017 14:44:30	U	SMPL
I4157-02MSD - 1	TD071117-2-2SMSD	12545	3.8426	-7470A	PPB		13 Jul 2017 14:46:37	U	SMPL
I4172-09 - 1	E2-FB-7-12-17	-176	-0.0487	-7470A	PPB		13 Jul 2017 14:48:43	U	SMPL
PB100616BL - 1	PBW	-3	0.0042	-7470A	PPB		13 Jul 2017 14:50:50	U	SMPL
PB100616BS - 1	LCSW	11822	3.6214	-7470A	PPB		13 Jul 2017 14:52:57	U	SMPL
PB100616TB - 1	PB100573TB	-83	-0.0203	-7470A	PPB		13 Jul 2017 14:55:05	U	SMPL
I4144-04 - 1	TP1-0-3	-37	-0.0062	-7470A	PPB		13 Jul 2017 14:57:12	U	SMPL
I4144-05 - 1	TP2-0-3	-12	0.0014	-7470A	PPB		13 Jul 2017 14:59:21	U	SMPL
I4144-06 - 1	TP3-0-3	-6	0.0033	-7470A	PPB		13 Jul 2017 15:01:29	U	SMPL
I4145-07 - 1	TRANSFORMER-3-4-5-COMP	2	0.0057	-7470A	PPB		13 Jul 2017 15:03:37	U	SMPL
I4145-11 - 1	BASEMENT-WATER	0	0.0051	-7470A	PPB		13 Jul 2017 15:05:44	U	SMPL
CCV15 - 1	CCV15	16931	5.1842	-7470A	PPB		13 Jul 2017 15:07:51	U	SMPL
CCB15 - 1	CCB15	60	0.0234	-7470A	PPB		13 Jul 2017 15:09:58	U	SMPL
I4148-07 - 1	POLE-1-2-3-4-COMP	-20	-0.0010	-7470A	PPB		13 Jul 2017 15:12:05	U	SMPL
I4149-03 - 1	OR-01-071117	12	0.0088	-7470A	PPB		13 Jul 2017 15:14:12	U	SMPL
I4150-02 - 1	A3591	-12	0.0014	-7470A	PPB		13 Jul 2017 15:16:18	U	SMPL
I4163-03 - 1	SU-04-071217	8	0.0075	-7470A	PPB		13 Jul 2017 15:18:25	U	SMPL
I4164-03 - 1	72-11975-COMP	0	0.0051	-7470A	PPB		13 Jul 2017 15:20:32	U	SMPL
I4166-06 - 1	COMP-1-2-3	13	0.0091	-7470A	PPB		13 Jul 2017 15:22:40	U	SMPL
I4166-12 - 1	COMP-4-5-6	16	0.0100	-7470A	PPB		13 Jul 2017 15:24:48	U	SMPL
I4166-12DUP - 1	COMP-4-5-6DUP	20	0.0112	-7470A	PPB		13 Jul 2017 15:26:56	U	SMPL
I4166-12MS - 1	COMP-4-5-6MS	11826	3.6226	-7470A	PPB		13 Jul 2017 15:29:04	U	SMPL
I4166-12MSD - 1	COMP-4-5-6MSD	12258	3.7548	-7470A	PPB		13 Jul 2017 15:31:11	U	SMPL
CCV16 - 1	CCV16	16859	5.1622	-7470A	PPB		13 Jul 2017 15:33:18	U	SMPL
CCB16 - 1	CCB16	-66	-0.0151	-7470A	PPB		13 Jul 2017 15:35:26	U	SMPL
I4157-02LX5 - 1		73	0.0274	-7470A	PPB		13 Jul 2017 15:37:34	U	SMPL
I4157-02A - 1		13800	4.2265	-7470A	PPB		13 Jul 2017 15:39:41	U	SMPL
I4166-12LX5 - 1		-21	-0.0013	-7470A	PPB		13 Jul 2017 15:41:47	U	SMPL
I4166-12A - 1		13219	4.0487	-7470A	PPB		13 Jul 2017 15:43:55	U	SMPL
CCV17 - 1	CCV17	16789	5.1408	-7470A	PPB		13 Jul 2017 15:46:02	U	SMPL
CCB17 - 1	CCB17	-23	-0.0019	-7470A	PPB		13 Jul 2017 15:48:09	U	SMPL