

M 3.00. P

Ad

07/15/18


Clear table

ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-11	7/11/17 10:41
STD2	0.1180	0.2030	0.2310	0.5890	0.1680	0.0270	1.1600	2017-07-11	7/11/17 11:10
STD3	0.3720	0.6110	0.6240	2.0280	0.5170	0.9480	3.1350	2017-07-11	7/11/17 11:39
STD4	0.7960	1.1730	1.1580	3.9610	0.9930	2.2080	5.8440	2017-07-11	7/11/17 12:08
STD5	2.0290	2.9370	2.8980	9.8240	2.4170	5.1920	14.3810	2017-07-11	7/11/17 12:37
STD6	3.9780	5.9980	5.9920	20.1380	4.9970	9.9380	29.9690	2017-07-11	7/11/17 13:06
STD7	5.0080	7.5280	7.5480	24.9600	6.2820	12.4370	37.7610	2017-07-11	7/11/17 13:35
ICV	2.0900	2.9830	3.0120	10.2660	2.5270	5.3330	14.7140	2017-07-11	7/11/17 15:03
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-11	7/11/17 15:32
CCV	2.1370	2.9580	2.8750	9.9250	2.4010	5.0420	14.5620	2017-07-13	7/13/17 10:41
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-13	7/13/17 11:17
LB88715BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-13	7/13/17 11:46
LB88715BSW	2.1570	2.9230	2.8580	9.8530	2.4270	5.4060	14.3770	2017-07-13	7/13/17 12:15
I4177-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-13	7/13/17 13:08
I4178-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-13	7/13/17 13:36
I4179-01	0.0000	0.0000	0.0000	0.0000	0.1980	0.0000	0.0000	2017-07-13	7/13/17 14:05
I4179-01DUP	0.0000	0.0000	0.0000	0.0000	0.1990	0.0000	0.0000	2017-07-13	7/13/17 14:34
I4179-01MS	2.1730	3.1710	3.1400	10.2530	2.6980	5.4780	15.2940	2017-07-13	7/13/17 15:03
CCV	2.1510	3.0450	2.9290	9.8460	2.4030	5.4830	14.7230	2017-07-13	7/13/17 15:32
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-13	7/13/17 16:01

IC-1
7-11-17

CALIBRATION OF COMPONENT F-

Method: ANIONS 07-11-17.mtw
Equation: $Q = 0.861053 \cdot A + 1.10647$
RSD: 1.232 %
Correlation coefficient: 0.999938

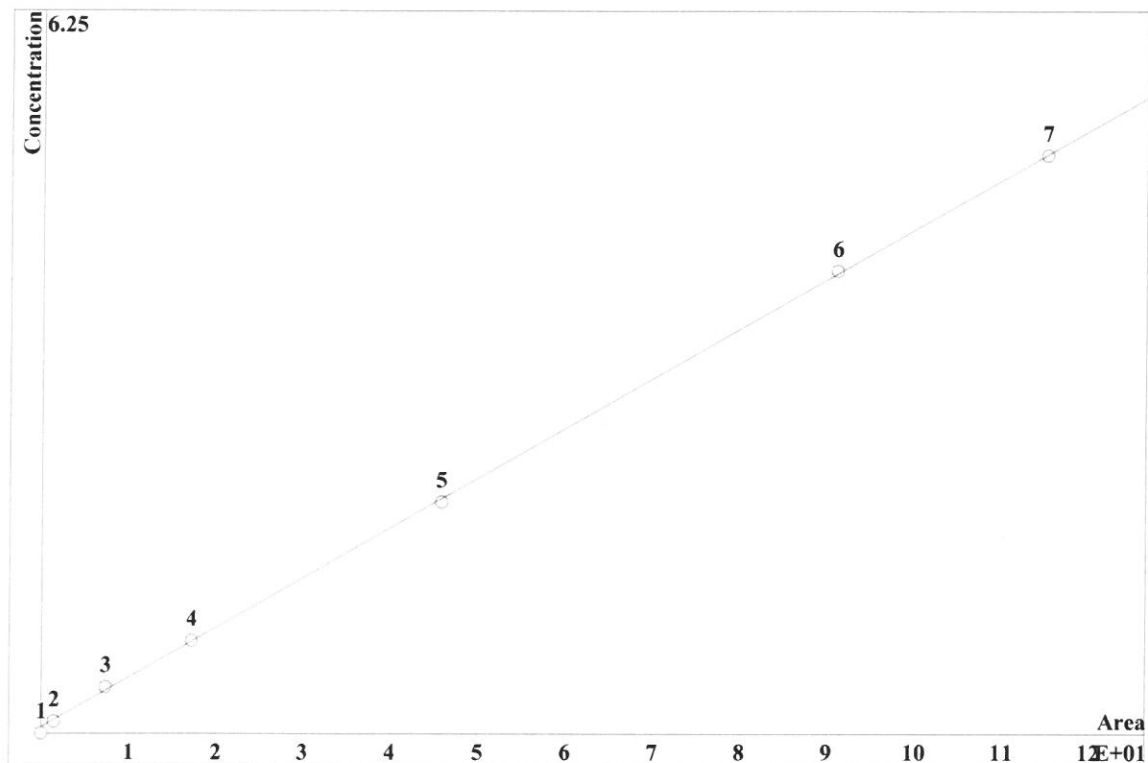


K3 = 0 K2 = 0 K1 = 0.861053 K0 = 1.10647
Base: Area
Ref.channel: Cond
ISTD:
Formula: Linear
Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.06832	1.446	0.1	20	5.72	Yes	
3	0.3217	7.345	0.4	20	5.72	Yes	
4	0.7336	17.2	0.8	20	5.72	Yes	
5	1.996	45.84	2	20	5.72	Yes	
6	4.193	91.1	4	20	5.72	Yes	
7	5.265	115	5	20	5.72	Yes	

CALIBRATION OF COMPONENT CL-

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 1.32378 \cdot A + 1.02533$
 RSD: 1.499 %
 Correlation coefficient: 0.999908

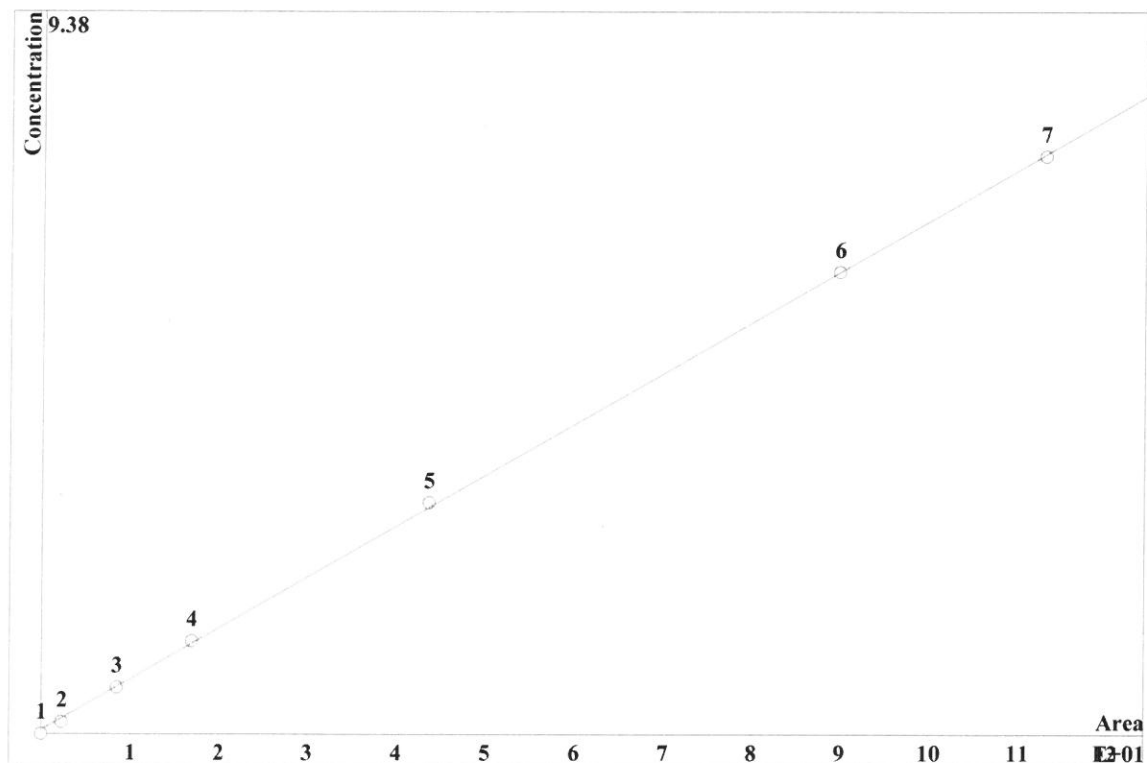


K3 = 0 K2 = 0 K1 = 1.32378 K0 = 1.02533
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.1087	2.297	0.15	20	8.411	Yes	
3	0.4389	8.457	0.6	20	8.411	Yes	
4	0.8963	16.94	1.2	20	8.411	Yes	
5	2.313	43.6	3	20	8.411	Yes	
6	4.834	89.84	6	20	8.411	Yes	
7	6.056	113	7.5	20	8.411	Yes	

CALIBRATION OF COMPONENT NO2

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 0.562432 \cdot A + 2.94942$
 RSD: 2.396 %
 Correlation coefficient: 0.999766

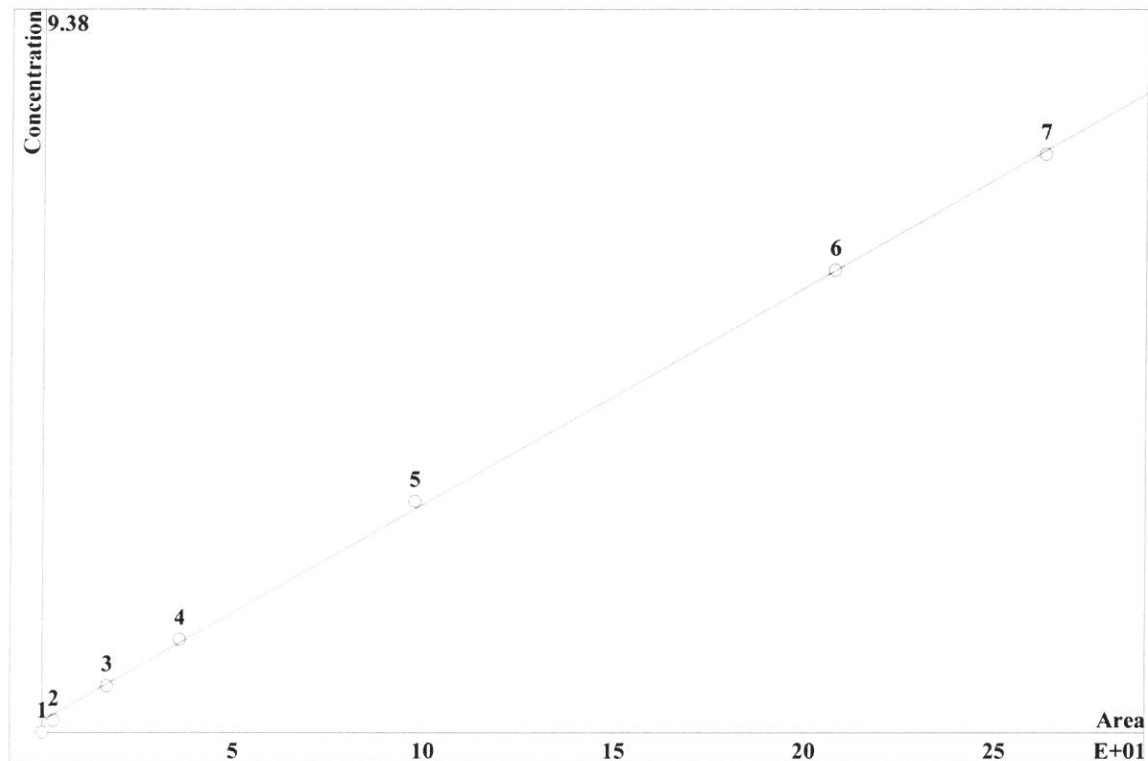


K3 = 0 K2 = 0 K1 = 0.562432 K0 = 2.94942
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.1363	2.964	0.15	20	9.95	Yes	
3	0.7893	16.95	0.6	20	9.95	Yes	
4	1.72	35.93	1.2	20	9.95	Yes	
5	4.769	97.8	3	20	9.95	Yes	
6	10.21	207.8	6	20	9.95	Yes	
7	12.73	263.2	7.5	20	9.95	Yes	

CALIBRATION OF COMPONENT BR-

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 3.08748 \cdot A - 9.48858$
 RSD: 1.211 %
 Correlation coefficient: 0.999940

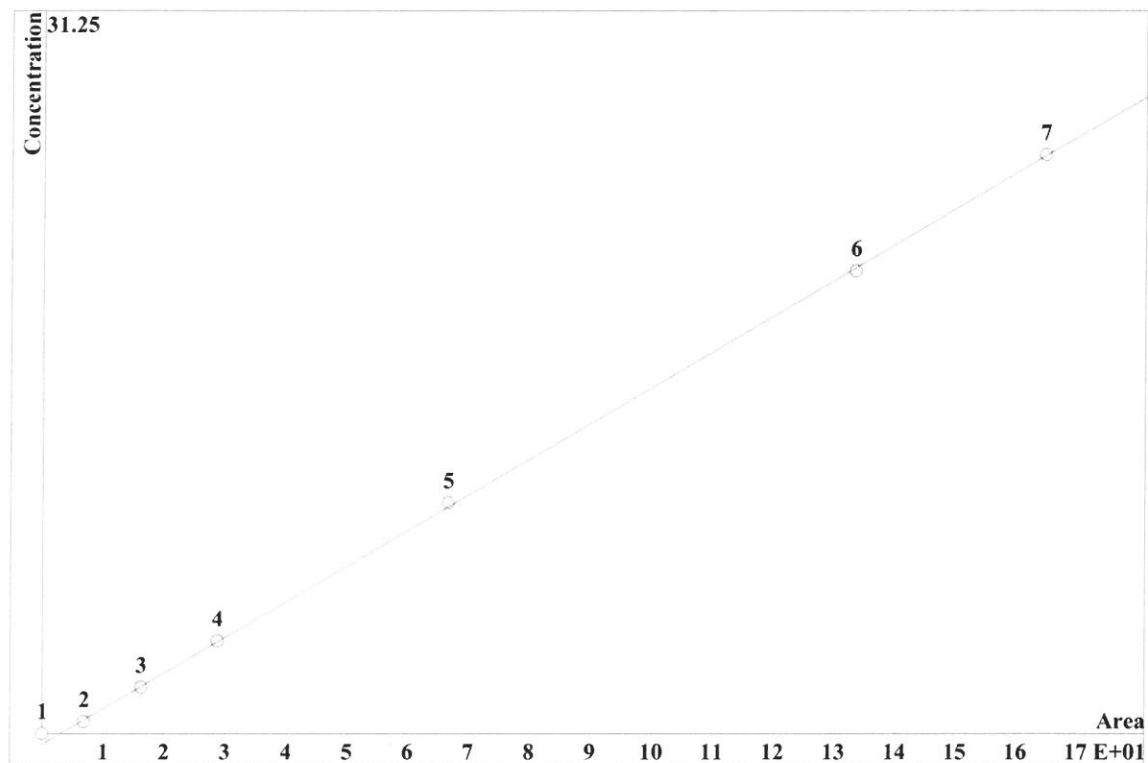


K3 = 0 K2 = 0 K1 = 3.08748 K0 = -9.48858
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.1874	6.887	0.5	20	12.61	Yes	
3	0.4669	16.21	2	20	12.61	Yes	
4	0.8161	28.73	4	20	12.61	Yes	
5	1.778	66.71	10	20	12.61	Yes	
6	3.237	133.5	20	20	12.61	Yes	
7	3.857	164.8	25	20	12.61	Yes	

CALIBRATION OF COMPONENT NO3

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 0.521641 \cdot A + 1.78354$
 RSD: 1.957 %
 Correlation coefficient: 0.999844

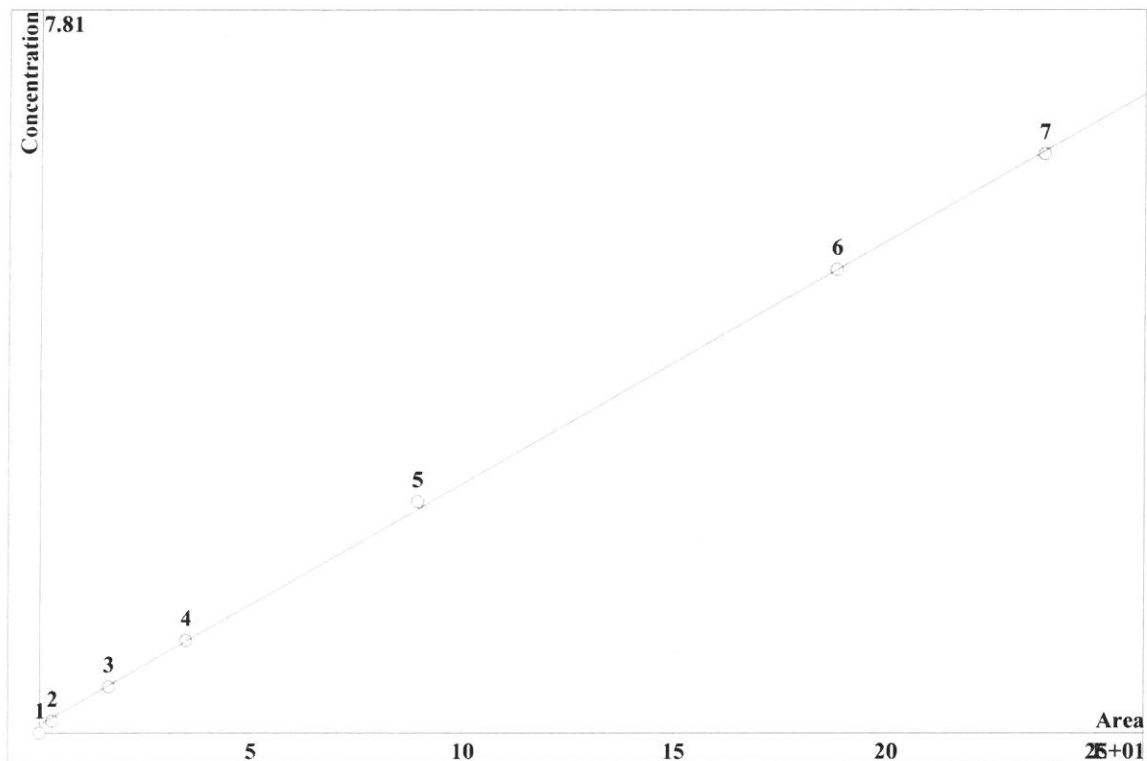


K3 = 0 K2 = 0 K1 = 0.521641 K0 = 1.78354
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.1166	3.012	0.125	20	14.11	Yes	
3	0.637	16.42	0.5	20	14.11	Yes	
4	1.334	34.64	1	20	14.11	Yes	
5	3.498	89.27	2.5	20	14.11	Yes	
6	7.391	188.2	5	20	14.11	Yes	
7	9.285	237.5	6.25	20	14.11	Yes	

±□;

CALIBRATION OF COMPONENT HPO4

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 1.42734 \cdot A - 5.10864$
 RSD: 3.656 %
 Correlation coefficient: 0.999454

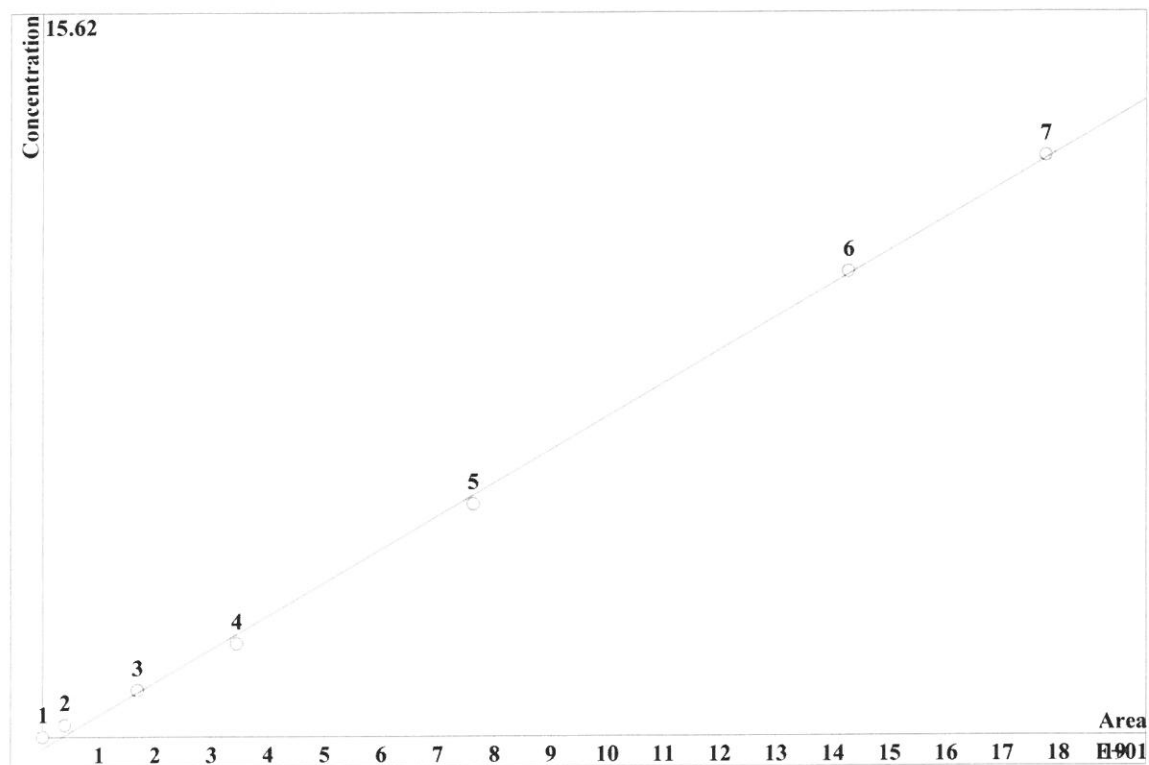


K3 = 0 K2 = 0 K1 = 1.42734 K0 = -5.10864
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0	0		No
2	0.06101	3.957	0.25	20	20.8	Yes	
3	0.2755	16.87	1	20	20.8	Yes	
4	0.5854	34.51	2	20	20.8	Yes	
5	1.384	76.34	5	20	20.8	Yes	
6	2.746	142.8	10	20	20.8	Yes	
7	3.493	177.8	12.5	20	20.8	Yes	

CALIBRATION OF COMPONENT SO4

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 1.69309 \cdot A + 8.53567$
 RSD: 2.648 %
 Correlation coefficient: 0.999714

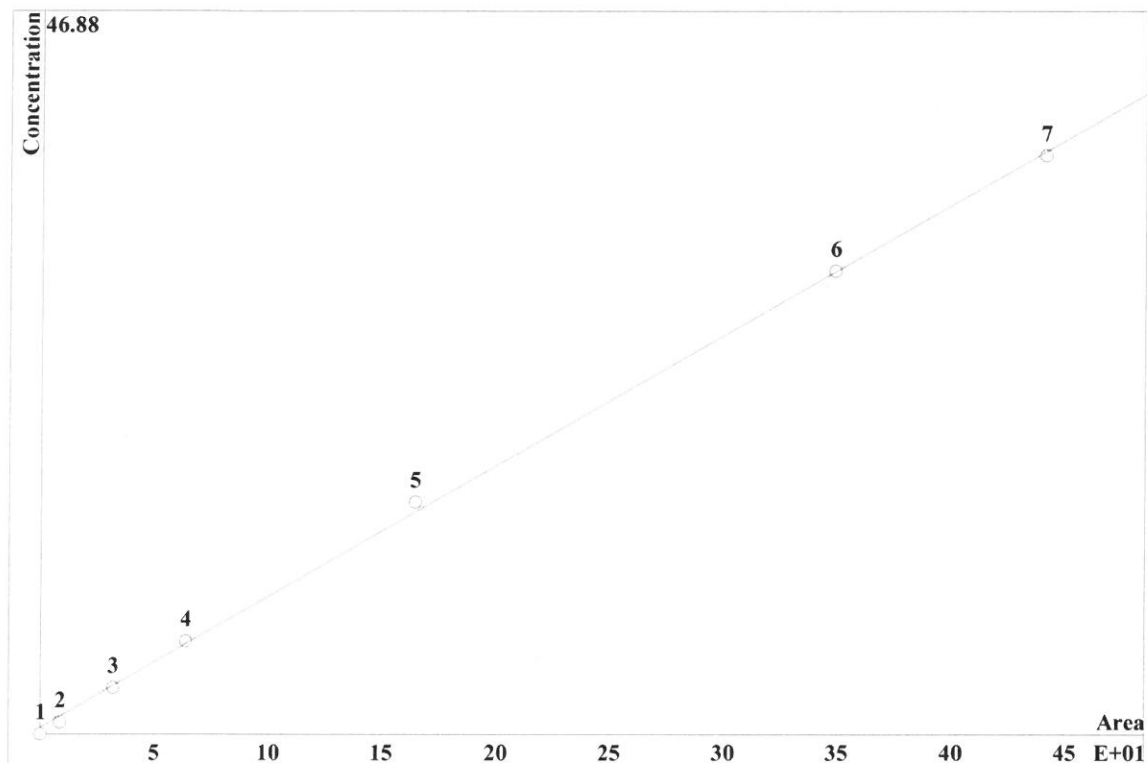

K3 = 0 K2 = 0 K1 = 1.69309 K0 = 8.53567
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0		0	0	0		No
2	0.2149	8.665	0.75	20	23.28	Yes	
3	0.8445	32	3	20	23.28	Yes	
4	1.728	63.99	6	20	23.28	Yes	
5	4.535	164.8	15	20	23.28	Yes	
6	9.788	349	30	20	23.28	Yes	
7	12.4	441	37.5	20	23.28	Yes	

Report date: 7/11/2017 2:05:17 PM
Printed by: wet


Ident: STD1
Analysis from: 7/11/2017 10:41:58 AM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58337

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
:
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

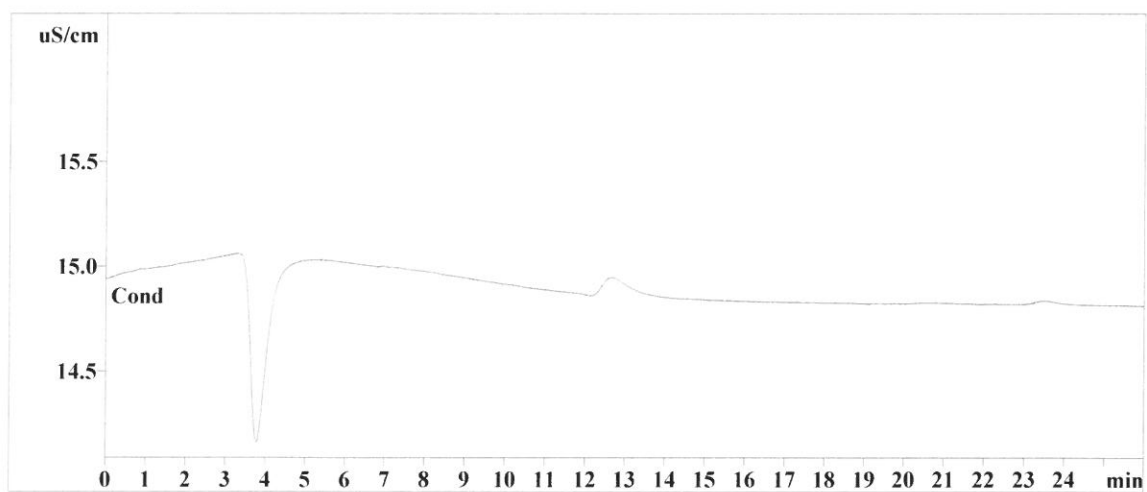

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:25 PM
Printed by: wet


Ident: STD2
Analysis from: 7/11/2017 11:10:54 AM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58338

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

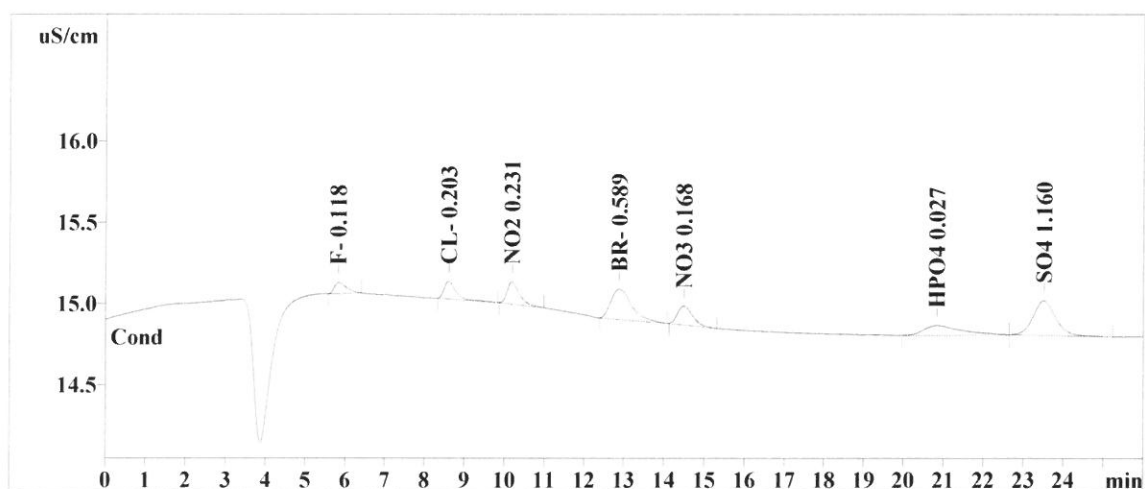

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.83	0.328	0.07	7.59	1.446	4.95	0.
2	8.59	0.298	0.11	12.10	2.297	7.86	0.
3	10.19	0.324	0.14	15.22	2.964	10.14	0.
4	12.89	0.548	0.19	20.90	6.887	23.56	0.
5	14.49	0.400	0.12	13.00	3.012	10.30	0.
6	20.82	0.957	0.06	6.73	3.957	13.54	0.
7	23.51	0.598	0.21	24.00	8.665	29.65	0.
7	26.00	0.493	0.89	99.54	29.228	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:31 PM
Printed by: wet


Ident: STD3
Analysis from: 7/11/2017 11:39:50 AM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58339

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

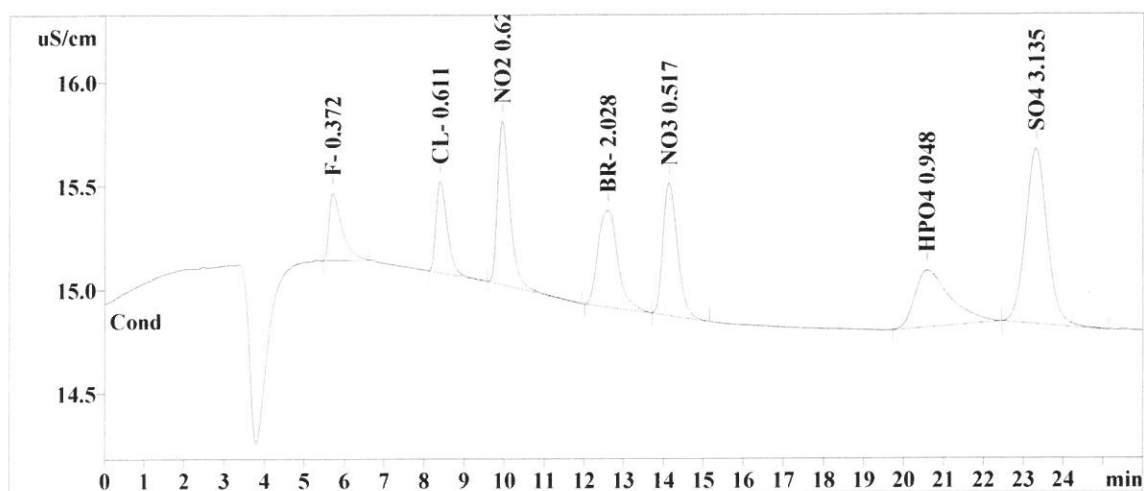

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.332	0.32	8.52	7.345	6.43	0.
2	8.40	0.288	0.44	11.62	8.457	7.40	0.
3	9.94	0.312	0.79	20.90	16.948	14.84	0.
4	12.60	0.530	0.47	12.36	16.210	14.19	0.
5	14.13	0.398	0.64	16.86	16.416	14.37	0.
6	20.58	0.901	0.27	7.28	16.866	14.76	0.
7	23.31	0.569	0.84	22.37	31.996	28.01	0.
7	26.00	0.476	3.77	99.93	114.237	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:36 PM
Printed by: wet


Ident: STD4
Analysis from: 7/11/2017 12:08:45 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58340

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

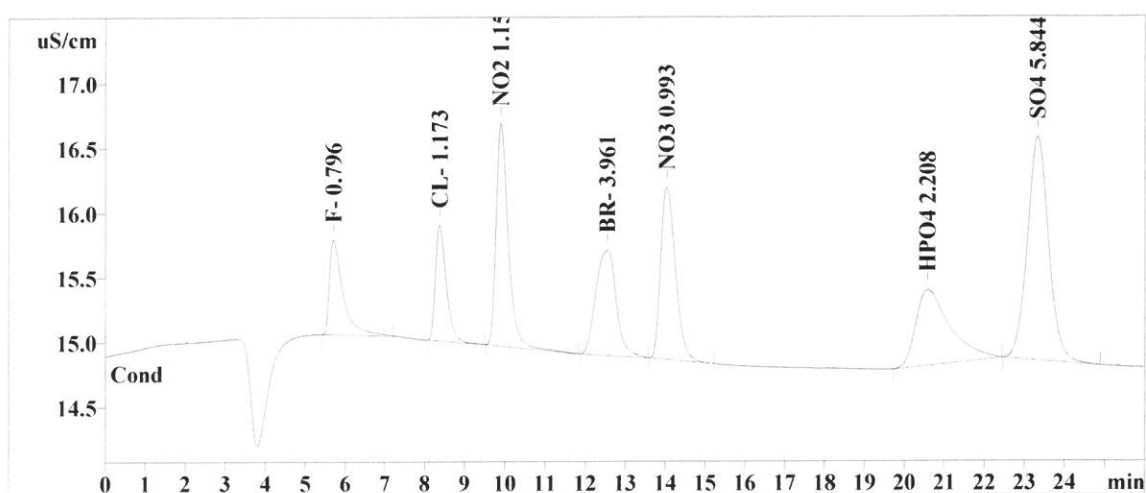

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.318	0.73	9.38	17.201	7.42	0.
2	8.38	0.283	0.90	11.46	16.942	7.30	0.
3	9.90	0.305	1.72	22.01	35.927	15.49	0.
4	12.56	0.550	0.82	10.44	28.734	12.39	0.
5	14.03	0.402	1.33	17.07	34.641	14.93	0.
6	20.59	0.852	0.59	7.49	34.514	14.88	0.
7	23.33	0.560	1.73	22.12	63.986	27.59	0.
7	26.00	0.467	7.81	99.96	231.946	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:45 PM
Printed by: wet


Ident: STD5
Analysis from: 7/11/2017 12:37:41 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58341

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

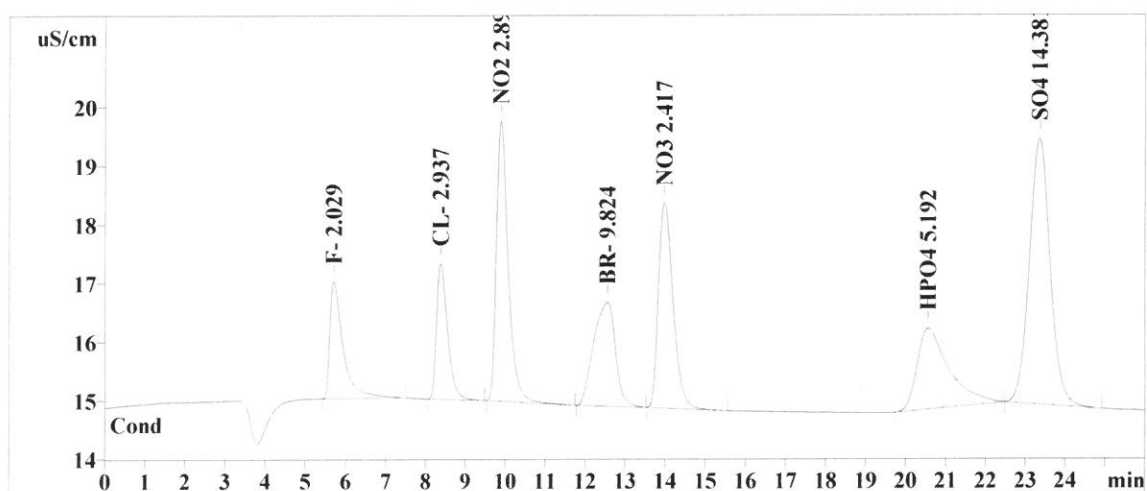

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.311	2.00	9.85	45.845	7.84	0.
2	8.38	0.281	2.31	11.41	43.598	7.46	0.
3	9.89	0.301	4.77	23.52	97.796	16.73	0.
4	12.57	0.607	1.78	8.77	66.713	11.42	0.
5	13.98	0.392	3.50	17.26	89.266	15.28	0.
6	20.56	0.782	1.38	6.83	76.335	13.06	0.
7	23.35	0.551	4.53	22.37	164.838	28.21	0.
7	26.00	0.461	20.27	99.99	584.391	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:52 PM
Printed by: wet


Ident: STD6
Analysis from: 7/11/2017 1:06:37 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58342

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

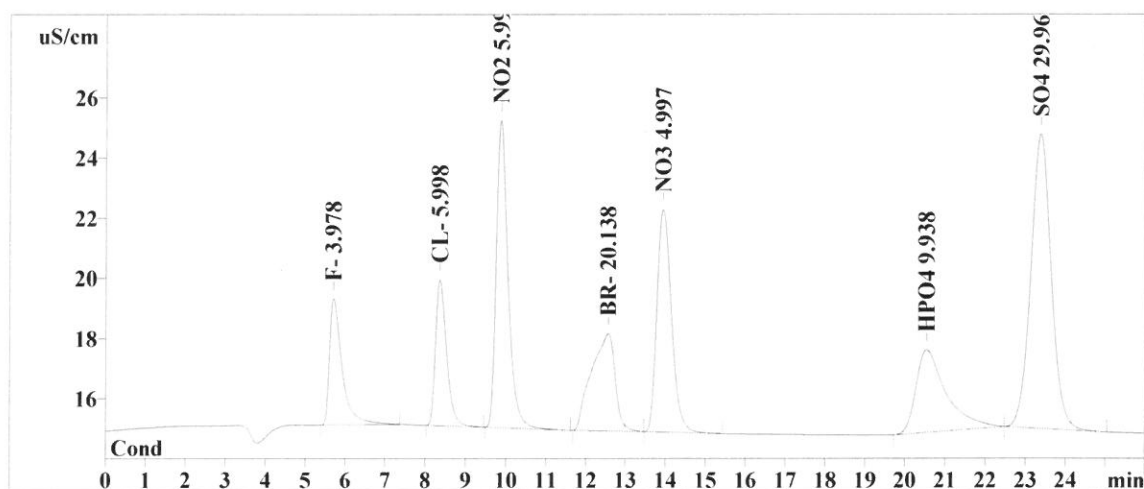

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.302	4.19	9.89	91.104	7.58	0.
2	8.36	0.277	4.83	11.40	89.840	7.47	0.
3	9.87	0.301	10.21	24.08	207.829	17.29	0.
4	12.56	0.706	3.24	7.64	133.522	11.11	0.
5	13.94	0.392	7.39	17.43	188.182	15.65	0.
6	20.53	0.726	2.75	6.48	142.827	11.88	0.
7	23.37	0.539	9.79	23.09	348.975	29.03	0.
7	26.00	0.463	42.40	100.00	1202.278	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:59 PM
Printed by: wet


Ident: STD7
Analysis from: 7/11/2017 1:35:32 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:22 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58343

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

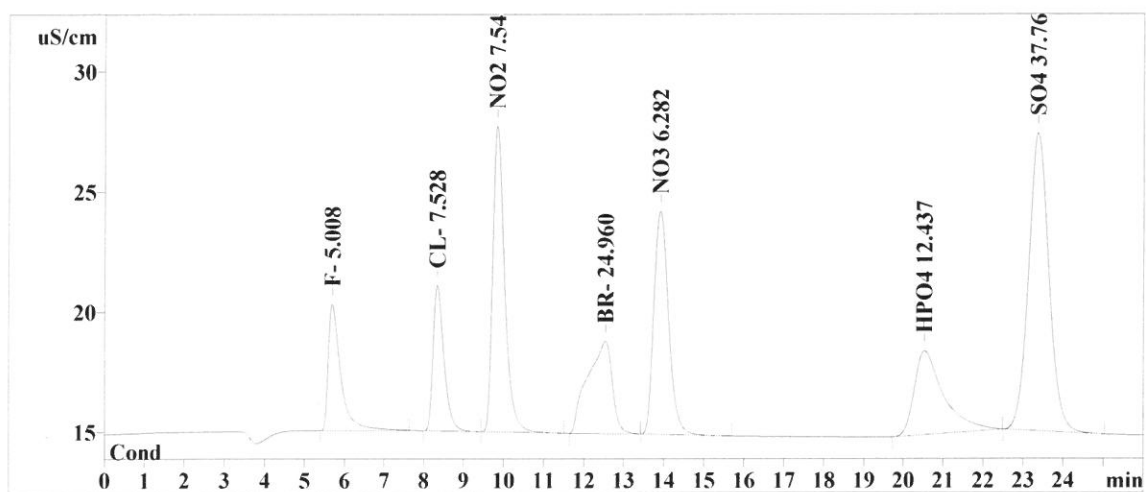

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.69	0.301	5.26	9.92	115.047	7.61	0.
2	8.34	0.278	6.06	11.41	112.966	7.47	0.
3	9.84	0.306	12.73	23.99	263.151	17.40	0.
4	12.54	0.768	3.86	7.26	164.756	10.89	0.
5	13.91	0.394	9.29	17.49	237.455	15.70	0.
6	20.53	0.708	3.49	6.58	177.848	11.76	0.
7	23.37	0.538	12.40	23.35	441.014	29.16	0.
7	26.00	0.471	53.09	100.00	1512.236	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2017 9:22:42 AM
Printed by: wet


Ident: ICV
Analysis from: 7/11/2017 3:03:18 PM
File: _2017-07-11_

Last save: 7/11/2017 3:29:08 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58346

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

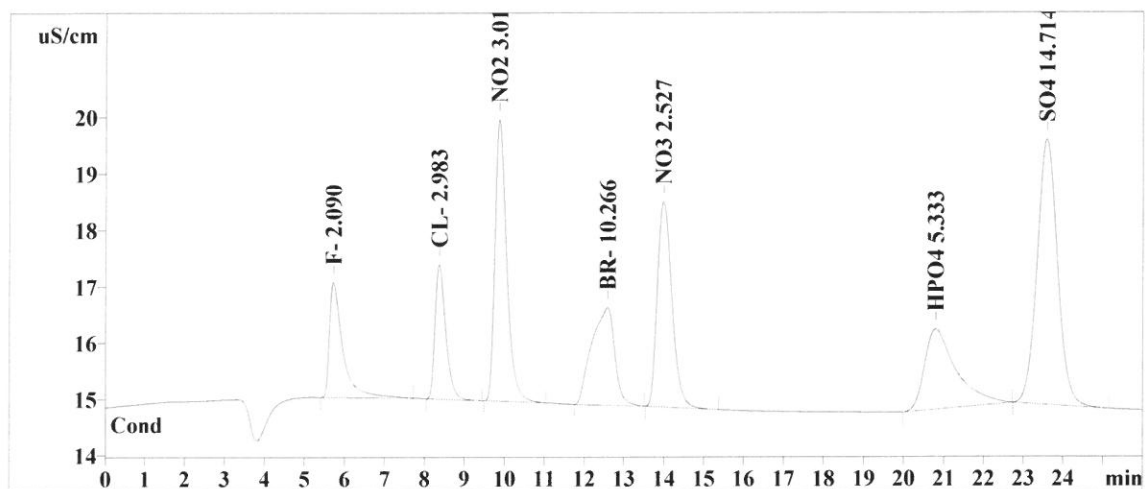

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.73	0.308	2.04	9.77	47.249	7.83	0.
2	8.37	0.278	2.39	11.39	44.295	7.34	0.
3	9.87	0.303	4.99	23.85	102.065	16.91	0.
4	12.59	0.673	1.74	8.31	69.572	11.52	0.
5	13.98	0.396	3.64	17.40	93.474	15.48	0.
6	20.79	0.774	1.43	6.83	78.312	12.97	0.
7	23.59	0.546	4.70	22.45	168.770	27.95	0.
7	26.00	0.468	20.93	99.99	603.737	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2017 9:22:48 AM
Printed by: wet


Ident: ICB
Analysis from: 7/11/2017 3:32:14 PM
File: _2017-07-11_

Last save: 7/12/2017 9:21:56 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58347

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

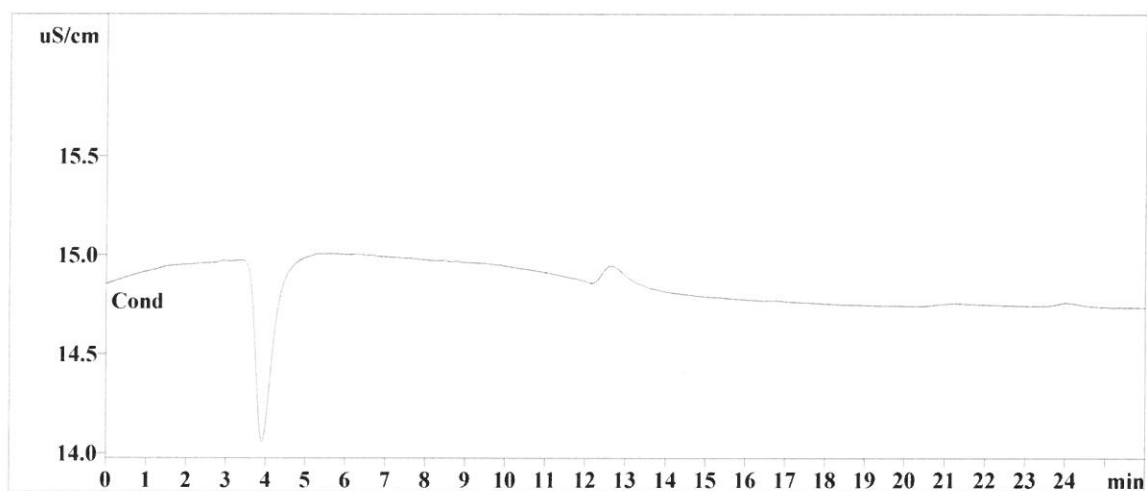

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:20:14 AM
Printed by: wet


Ident: CCV
Analysis from: 7/13/2017 10:41:22 AM
File: _2017-07-13_

Last save: 7/13/2017 11:07:12 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58371

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

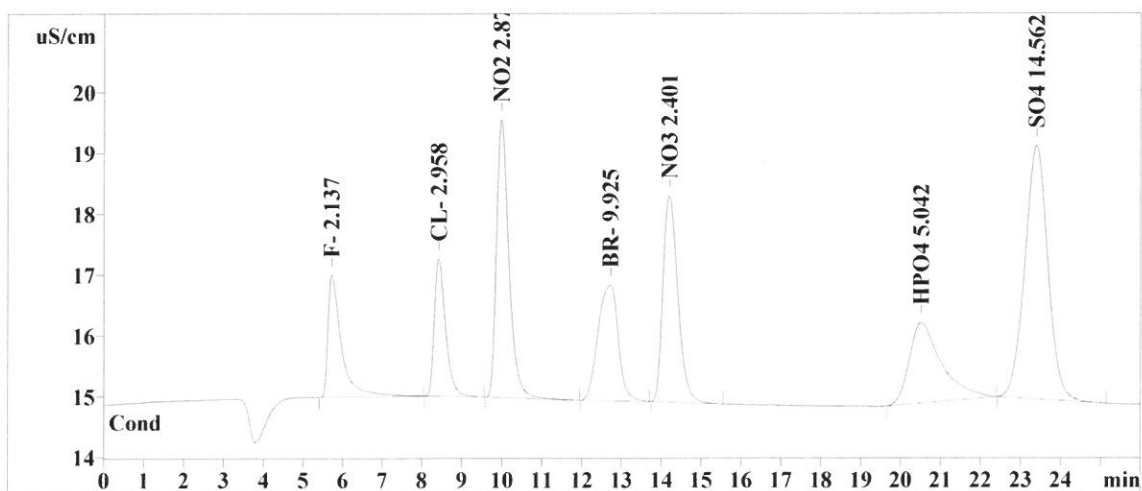

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.73	0.317	2.01	10.24	48.351	8.24	0.
2	8.42	0.290	2.26	11.50	43.912	7.49	0.
3	9.98	0.313	4.57	23.27	97.187	16.57	0.
4	12.71	0.559	1.90	9.70	67.363	11.48	0.
5	14.19	0.402	3.39	17.27	88.650	15.11	0.
6	20.51	0.794	1.33	6.76	74.227	12.65	0.
7	23.39	0.606	4.17	21.25	166.971	28.46	0.
7	26.00	0.469	19.62	100.00	586.660	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:20:46 AM
Printed by: wet


Ident: CCB
Analysis from: 7/13/2017 11:17:48 AM
File: _2017-07-13_

Last save: 7/14/2017 11:20:40 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58372

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

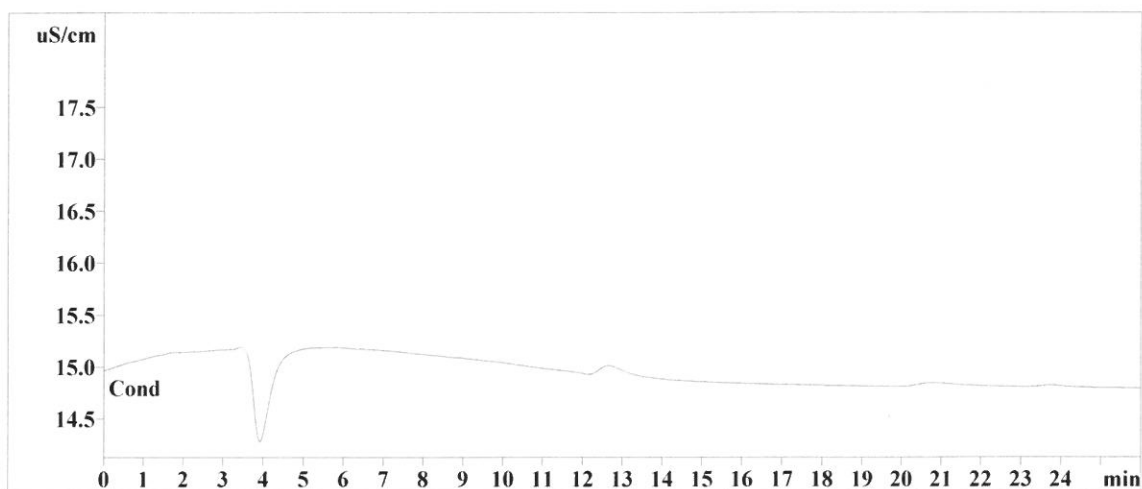

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:20:53 AM
Printed by: wet


Ident: LB88715BLW
Analysis from: 7/13/2017 11:46:44 AM
File: _2017-07-13_

Last save: 7/14/2017 11:20:40 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58373

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

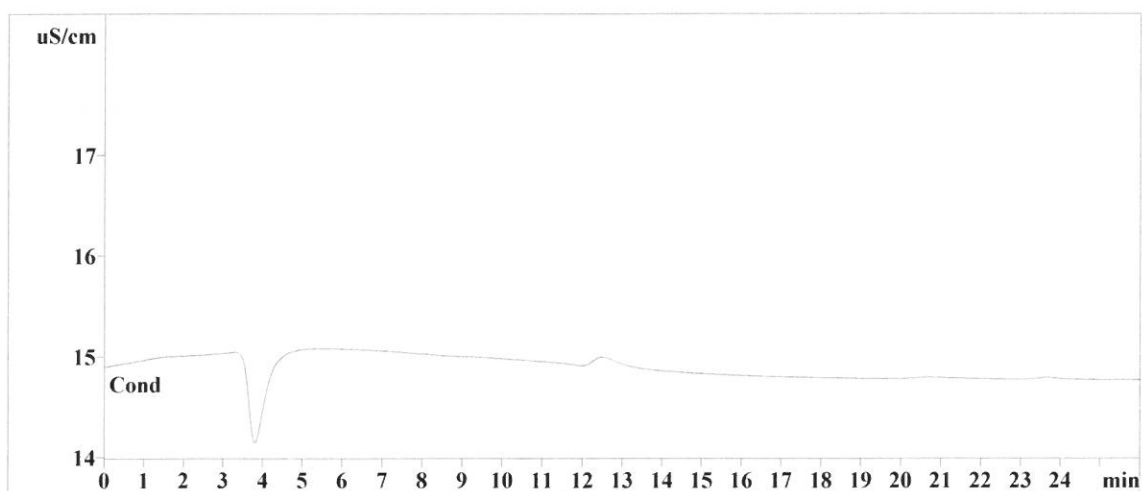

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:20:58 AM
Printed by: wet


Ident: LB88715BSW
Analysis from: 7/13/2017 12:15:39 PM
File: _2017-07-13_

Last save: 7/14/2017 11:20:08 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58374

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

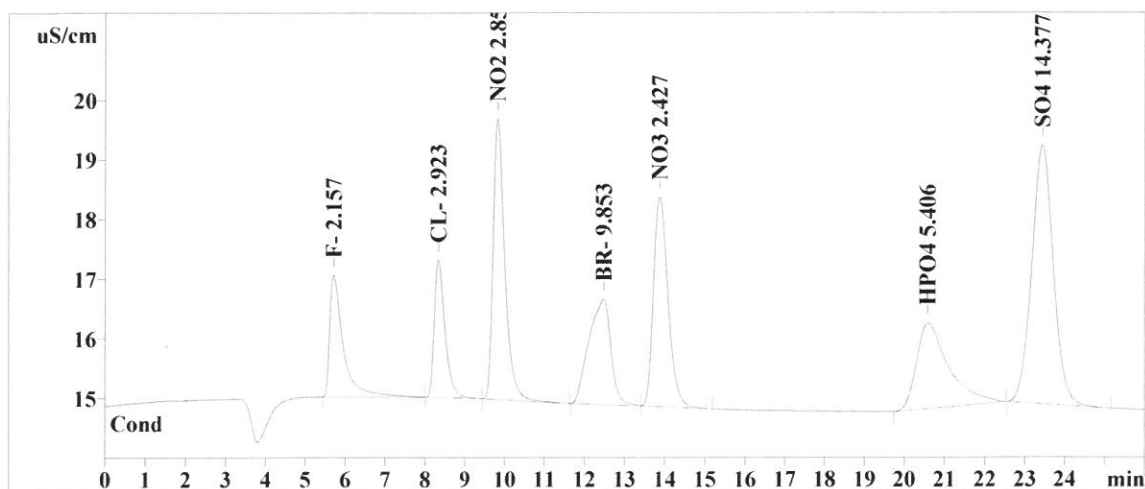

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.316	2.04	10.14	48.812	8.28	0.
2	8.33	0.280	2.31	11.46	43.381	7.36	0.
3	9.82	0.301	4.71	23.40	96.592	16.39	0.
4	12.47	0.619	1.77	8.80	66.896	11.35	0.
5	13.87	0.393	3.51	17.44	89.630	15.21	0.
6	20.59	0.779	1.44	7.15	79.322	13.46	0.
7	23.43	0.577	4.34	21.60	164.786	27.96	0.
7	26.00	0.466	20.11	99.99	589.419	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:21:56 AM
Printed by: wet


Ident: I4177-01
Analysis from: 7/13/2017 1:08:00 PM
File: _2017-07-13_

Last save: 7/14/2017 11:21:52 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58377

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

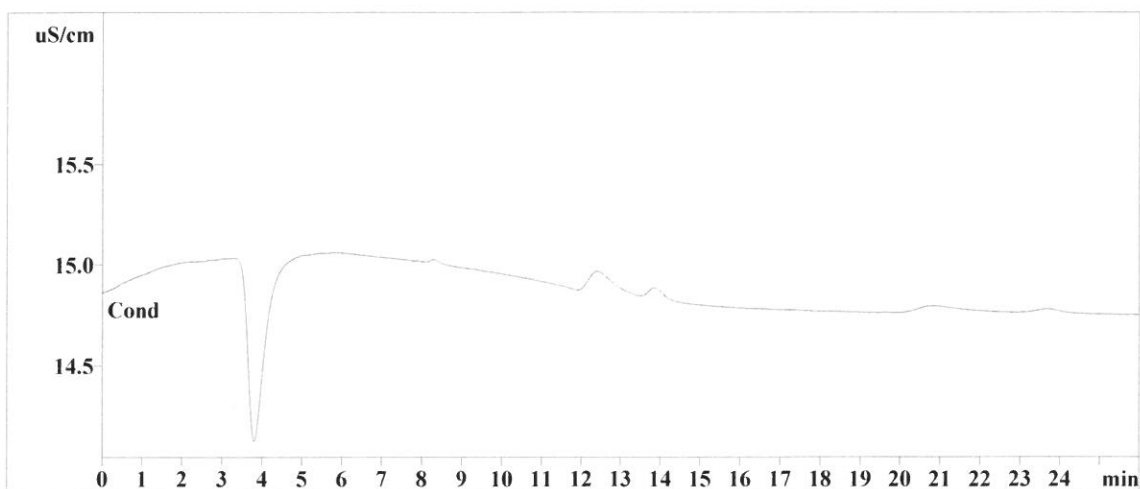

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:22:19 AM
Printed by: wet


Ident: I4178-01
Analysis from: 7/13/2017 1:36:56 PM
File: _2017-07-13_

Last save: 7/14/2017 11:22:12 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58378

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

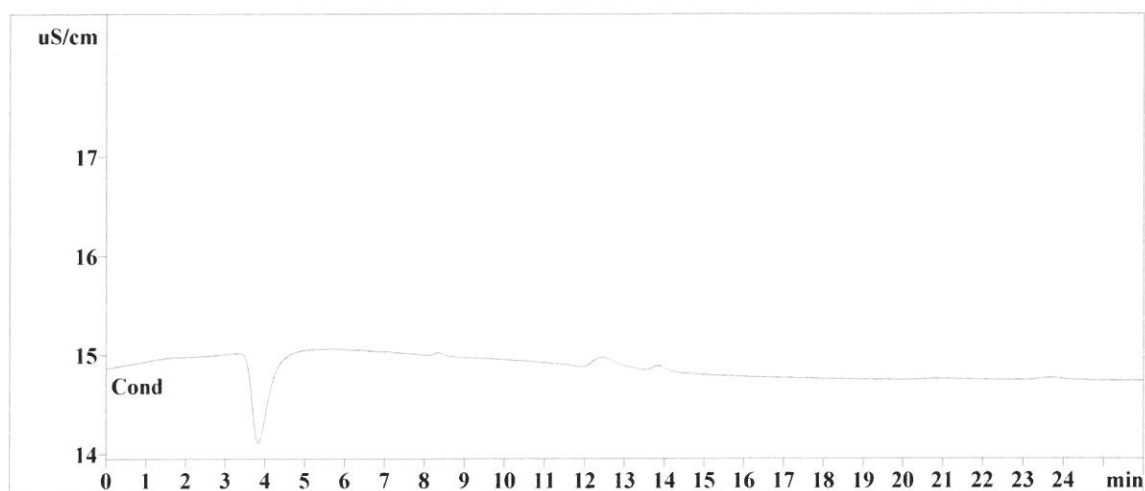

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:22:26 AM
Printed by: wet


Ident: I4179-01
Analysis from: 7/13/2017 2:05:52 PM
File: _2017-07-13_

Last save: 7/14/2017 11:22:12 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58379

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

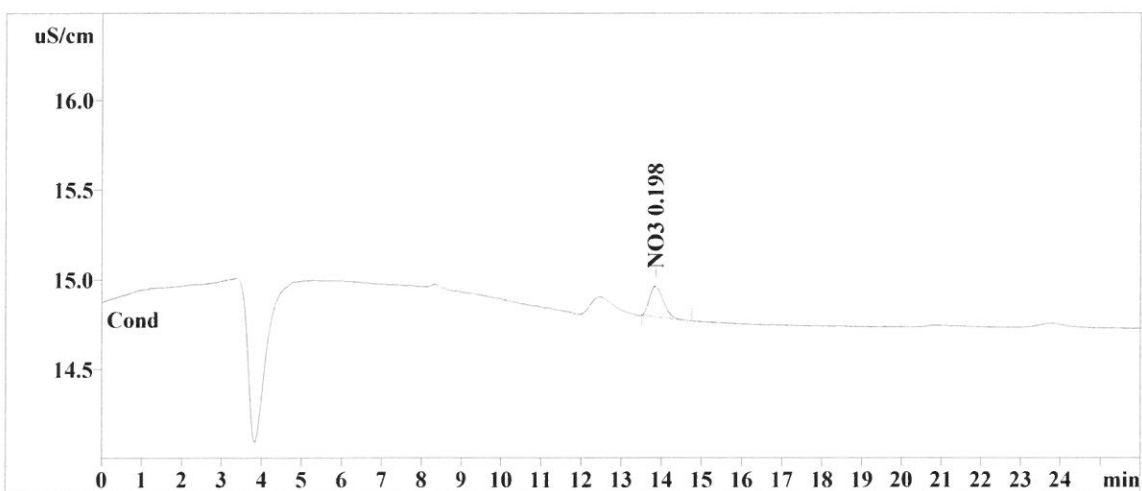

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	0.00	0.000	0.00	0.00	0.000	0.00	0.
2	0.00	0.000	0.00	0.00	0.000	0.00	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	0.00	0.000	0.00	0.00	0.000	0.00	0.
5	13.84	0.382	0.17	99.64	4.164	100.00	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	26.00	0.055	0.17	99.64	4.164	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:22:33 AM
Printed by: wet


Ident: I4179-01DUP
Analysis from: 7/13/2017 2:34:47 PM
File: _2017-07-13_

Last save: 7/14/2017 11:22:12 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58380

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

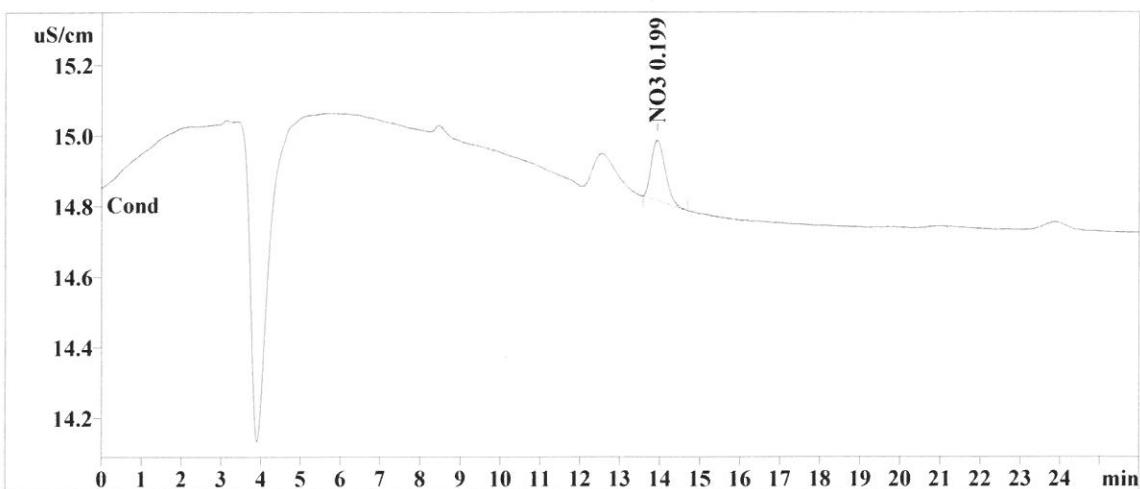

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	0.00	0.000	0.00	0.00	0.000	0.00	0.
2	0.00	0.000	0.00	0.00	0.000	0.00	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	0.00	0.000	0.00	0.00	0.000	0.00	0.
5	13.93	0.384	0.17	99.88	4.217	100.00	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	26.00	0.055	0.17	99.88	4.217	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:22:42 AM
Printed by: wet


Ident: I4179-01MS
Analysis from: 7/13/2017 3:03:43 PM
File: _2017-07-13_

Last save: 7/13/2017 3:29:32 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58381

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

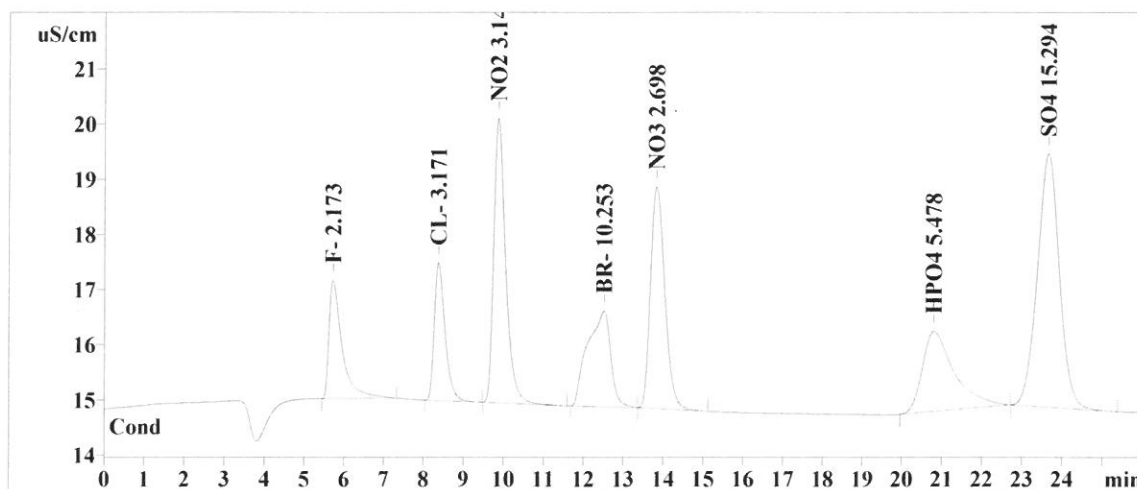

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.313	2.13	9.89	49.186	7.83	0.
2	8.37	0.282	2.50	11.57	47.139	7.50	0.
3	9.87	0.304	5.16	23.88	106.599	16.96	0.
4	12.52	0.706	1.74	8.05	69.491	11.06	0.
5	13.83	0.385	4.02	18.60	100.028	15.92	0.
6	20.80	0.782	1.45	6.73	80.336	12.78	0.
7	23.65	0.581	4.59	21.27	175.621	27.95	0.
7	26.00	0.479	21.59	99.99	628.400	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:25:45 AM
Printed by: wet


Ident: CCV
Analysis from: 7/13/2017 3:32:38 PM
File: _2017-07-13_

Last save: 7/13/2017 4:01:32 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58382

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

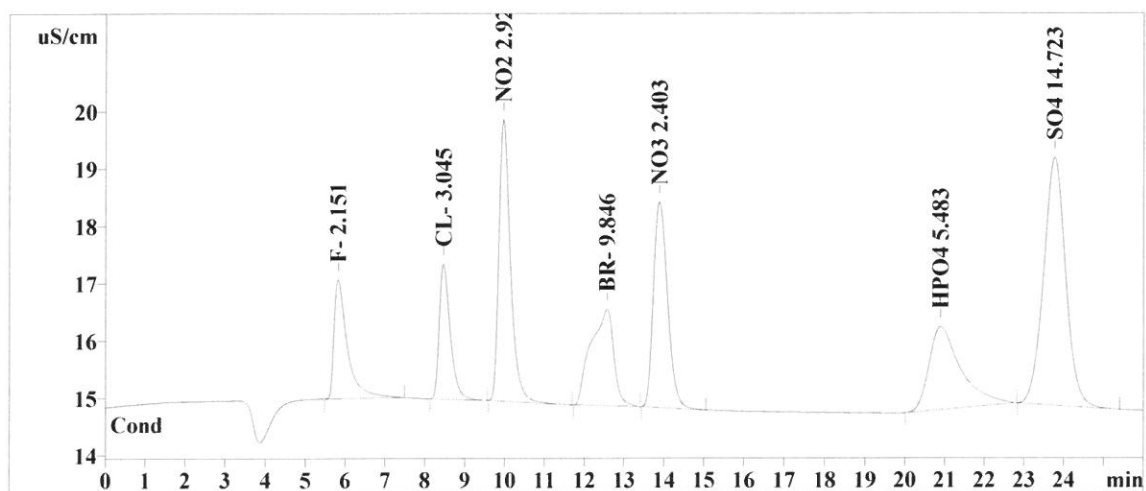

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.82	0.321	2.07	10.16	48.667	8.14	0.
2	8.46	0.285	2.36	11.56	45.224	7.56	0.
3	9.97	0.296	4.91	24.10	99.103	16.58	0.
4	12.57	0.704	1.68	8.25	66.851	11.18	0.
5	13.88	0.384	3.58	17.57	88.730	14.84	0.
6	20.89	0.783	1.45	7.11	80.414	13.45	0.
7	23.77	0.594	4.33	21.22	168.876	28.25	0.
7	26.00	0.481	20.38	99.98	597.864	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/14/2017 11:25:52 AM
Printed by: wet


Ident: CCB
Analysis from: 7/13/2017 4:01:34 PM
File: _2017-07-13_

Last save: 7/14/2017 11:20:40 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58383

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

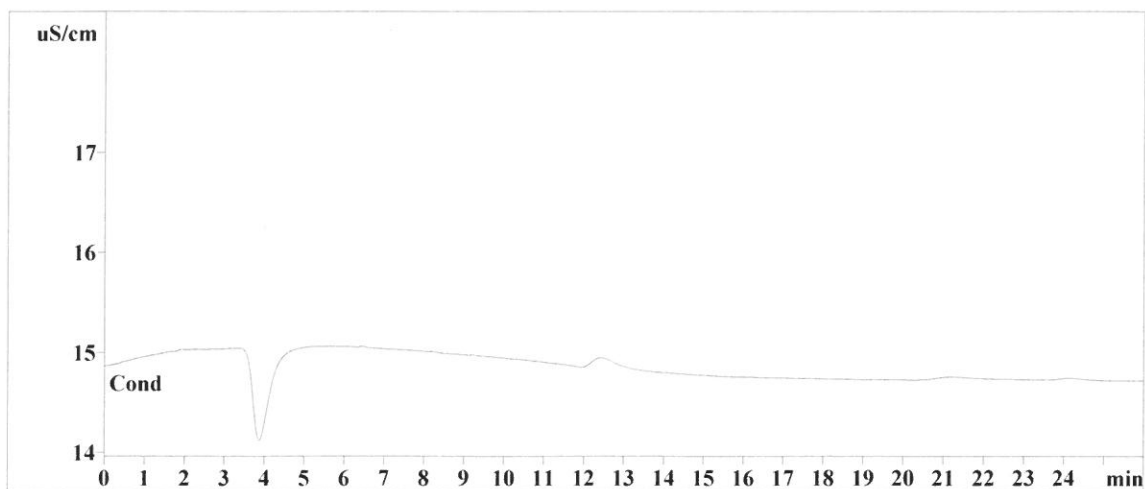

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD