

Clear table


ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2017-07-11_	7/11/17 10:41
STD2	0.1180	0.2030	0.2310	0.5890	0.1680	0.0270	1.1600	_2017-07-11_	7/11/17 11:10
STD3	0.3720	0.6110	0.6240	2.0280	0.5170	0.9480	3.1350	_2017-07-11_	7/11/17 11:39
STD4	0.7960	1.1730	1.1580	3.9610	0.9930	2.2080	5.8440	_2017-07-11_	7/11/17 12:08
STD5	2.0290	2.9370	2.8980	9.8240	2.4170	5.1920	14.3810	_2017-07-11_	7/11/17 12:37
STD6	3.9780	5.9980	5.9920	20.1380	4.9970	9.9380	29.9690	_2017-07-11_	7/11/17 13:06
STD7	5.0080	7.5280	7.5480	24.9600	6.2820	12.4370	37.7610	_2017-07-11_	7/11/17 13:35
ICV	2.0900	2.9830	3.0120	10.2660	2.5270	5.3330	14.7140	_2017-07-11_	7/11/17 15:03
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2017-07-11_	7/11/17 15:32
CCV	2.0190	2.9740	2.8890	10.1790	2.4560	5.1220	14.3850	_2017-07-17_	7/17/17 15:46
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2017-07-17_	7/17/17 16:21
LB88763BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2017-07-17_	7/17/17 16:50
LB88763BSW	2.0990	2.9480	2.8850	10.0660	2.4420	5.4860	14.4820	_2017-07-17_	7/17/17 17:19
I4234-01	0.0000	54.2650	0.0000	0.9450	0.0000	4.4810	11.7420	_2017-07-17_	7/17/17 17:48
I4234-02	0.3790	79.1500	0.0000	0.8510	0.0000	3.6730	10.6360	_2017-07-17_	7/17/17 18:17
I4234-04	0.2540	69.0920	0.0000	1.4080	0.0000	3.3340	12.4930	_2017-07-17_	7/17/17 18:46
I4234-04DUP	0.2570	69.1780	0.0000	1.3430	0.0000	3.2920	12.5480	_2017-07-17_	7/17/17 19:15
I4234-04MS	4.0850	65.4460	2.9210	11.4340	2.5450	8.7820	27.5020	_2017-07-17_	7/17/17 19:44
CCV	2.0590	2.9950	2.9210	10.0680	2.4710	5.5920	14.5130	_2017-07-17_	7/17/17 20:13
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2017-07-17_	7/17/17 20:42

7/11/17
7/15/17

IC-1
7-11-17

CALIBRATION OF COMPONENT F-

Method: ANIONS 07-11-17.mtw
Equation: $Q = 0.861053 \cdot A + 1.10647$
RSD: 1.232 %
Correlation coefficient: 0.999938

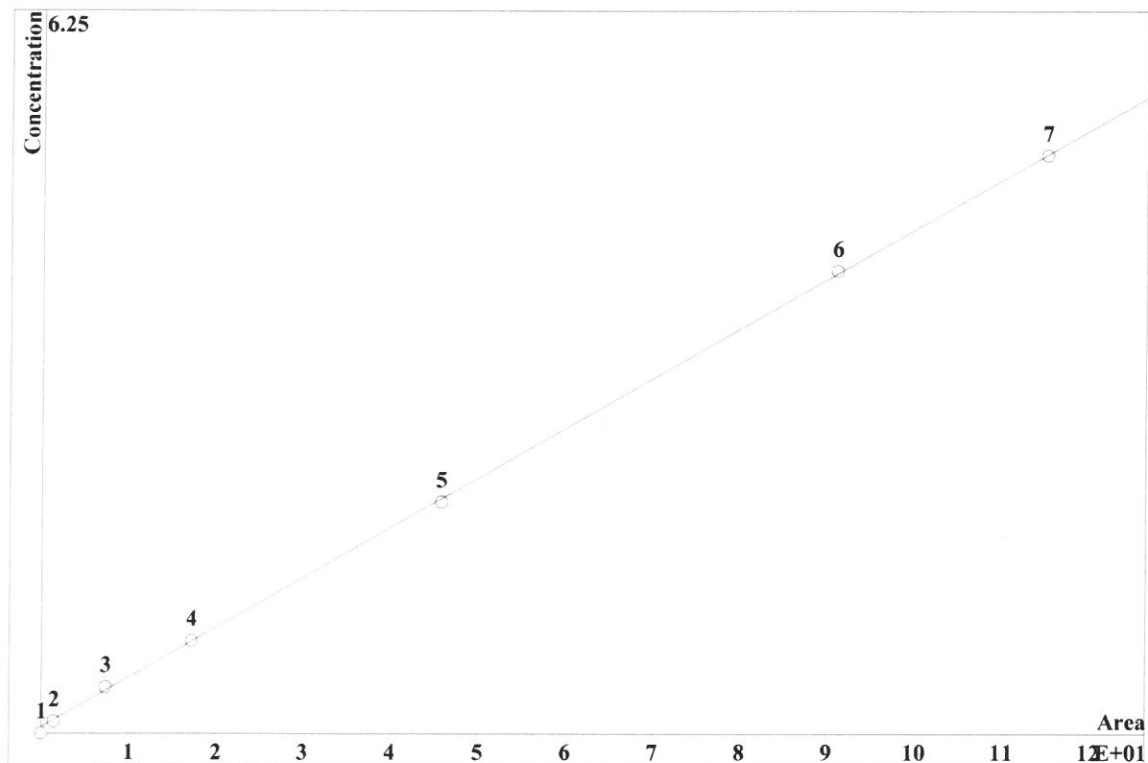


K3 = 0 K2 = 0 K1 = 0.861053 K0 = 1.10647
Base: Area
Ref.channel: Cond
ISTD:
Formula: Linear
Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.06832	1.446	0.1	20	5.72	Yes	
3	0.3217	7.345	0.4	20	5.72	Yes	
4	0.7336	17.2	0.8	20	5.72	Yes	
5	1.996	45.84	2	20	5.72	Yes	
6	4.193	91.1	4	20	5.72	Yes	
7	5.265	115	5	20	5.72	Yes	

CALIBRATION OF COMPONENT CL-

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 1.32378 \cdot A + 1.02533$
 RSD: 1.499 %
 Correlation coefficient: 0.999908

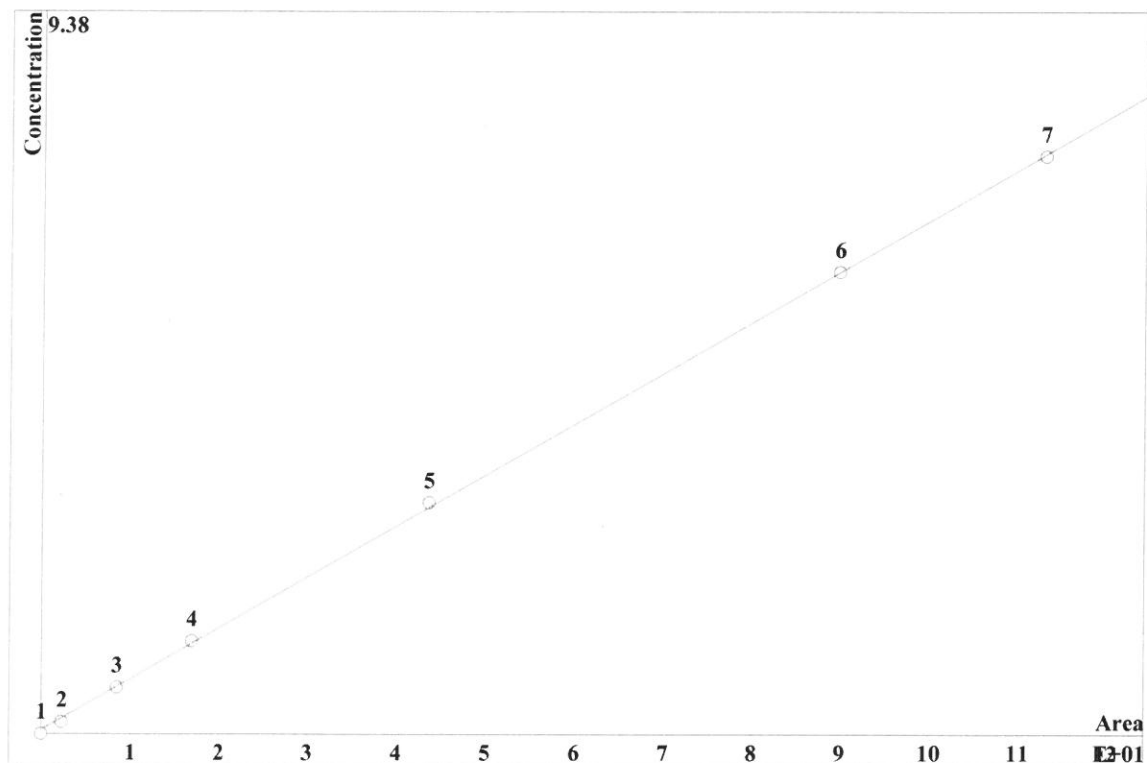


K3 = 0 K2 = 0 K1 = 1.32378 K0 = 1.02533
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1		0	0	0	0			No
2	0.1087	2.297	0.15	20	8.411	Yes		Yes
3	0.4389	8.457	0.6	20	8.411	Yes		Yes
4	0.8963	16.94	1.2	20	8.411	Yes		Yes
5	2.313	43.6	3	20	8.411	Yes		Yes
6	4.834	89.84	6	20	8.411	Yes		Yes
7	6.056	113	7.5	20	8.411	Yes		Yes

CALIBRATION OF COMPONENT NO2

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 0.562432 \cdot A + 2.94942$
 RSD: 2.396 %
 Correlation coefficient: 0.999766

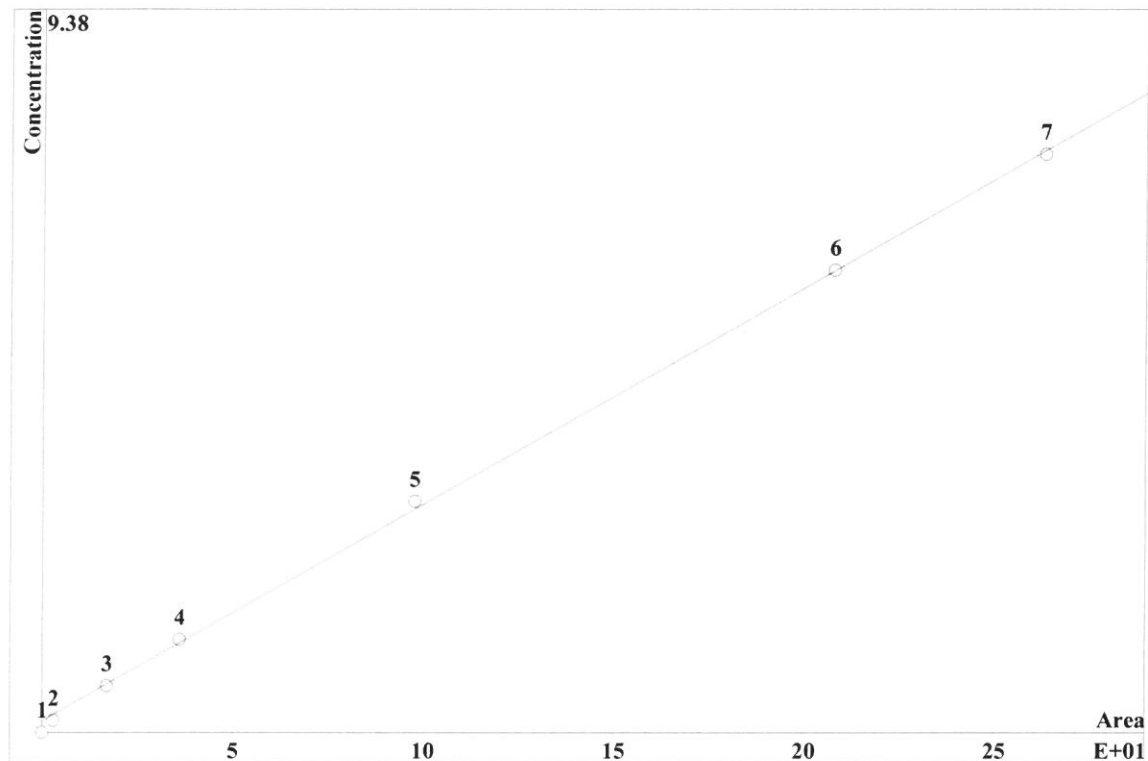


K3 = 0 K2 = 0 K1 = 0.562432 K0 = 2.94942
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.1363	2.964	0.15	20	9.95	Yes	
3	0.7893	16.95	0.6	20	9.95	Yes	
4	1.72	35.93	1.2	20	9.95	Yes	
5	4.769	97.8	3	20	9.95	Yes	
6	10.21	207.8	6	20	9.95	Yes	
7	12.73	263.2	7.5	20	9.95	Yes	

CALIBRATION OF COMPONENT BR-

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 3.08748 \cdot A - 9.48858$
 RSD: 1.211 %
 Correlation coefficient: 0.999940

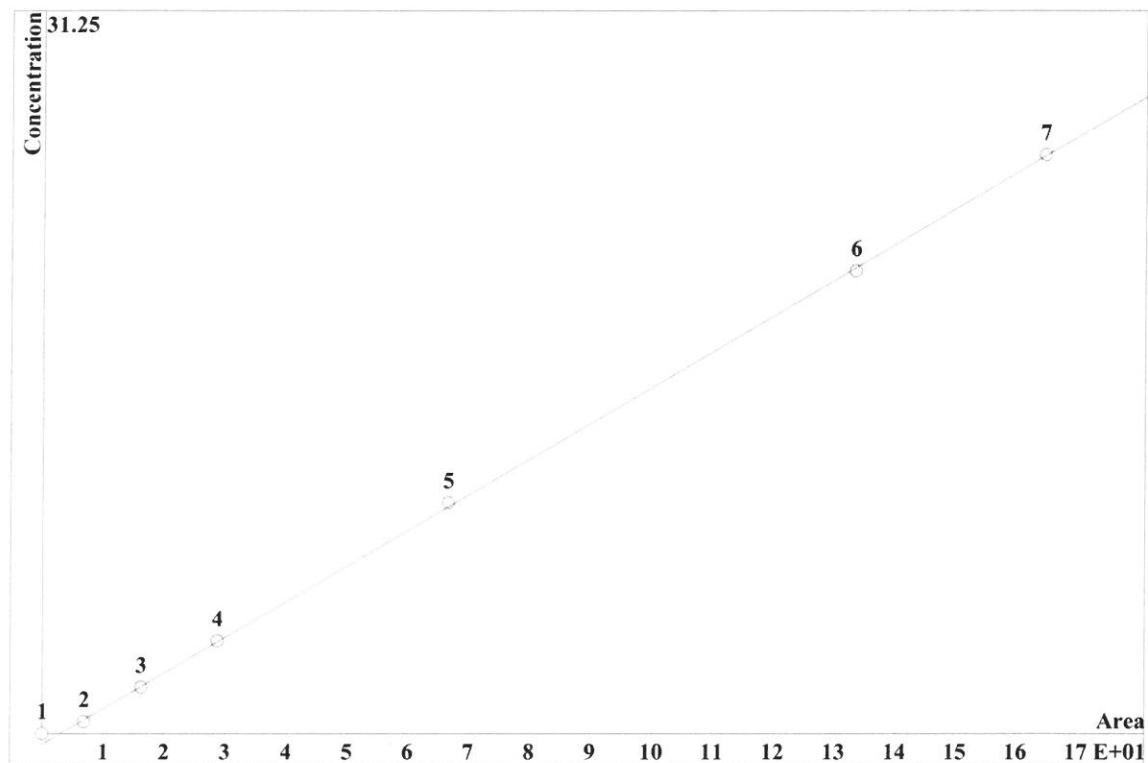


K3 = 0 K2 = 0 K1 = 3.08748 K0 = -9.48858
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.1874	6.887	0.5	20	12.61	Yes	
3	0.4669	16.21	2	20	12.61	Yes	
4	0.8161	28.73	4	20	12.61	Yes	
5	1.778	66.71	10	20	12.61	Yes	
6	3.237	133.5	20	20	12.61	Yes	
7	3.857	164.8	25	20	12.61	Yes	

CALIBRATION OF COMPONENT NO3

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 0.521641 \cdot A + 1.78354$
 RSD: 1.957 %
 Correlation coefficient: 0.999844

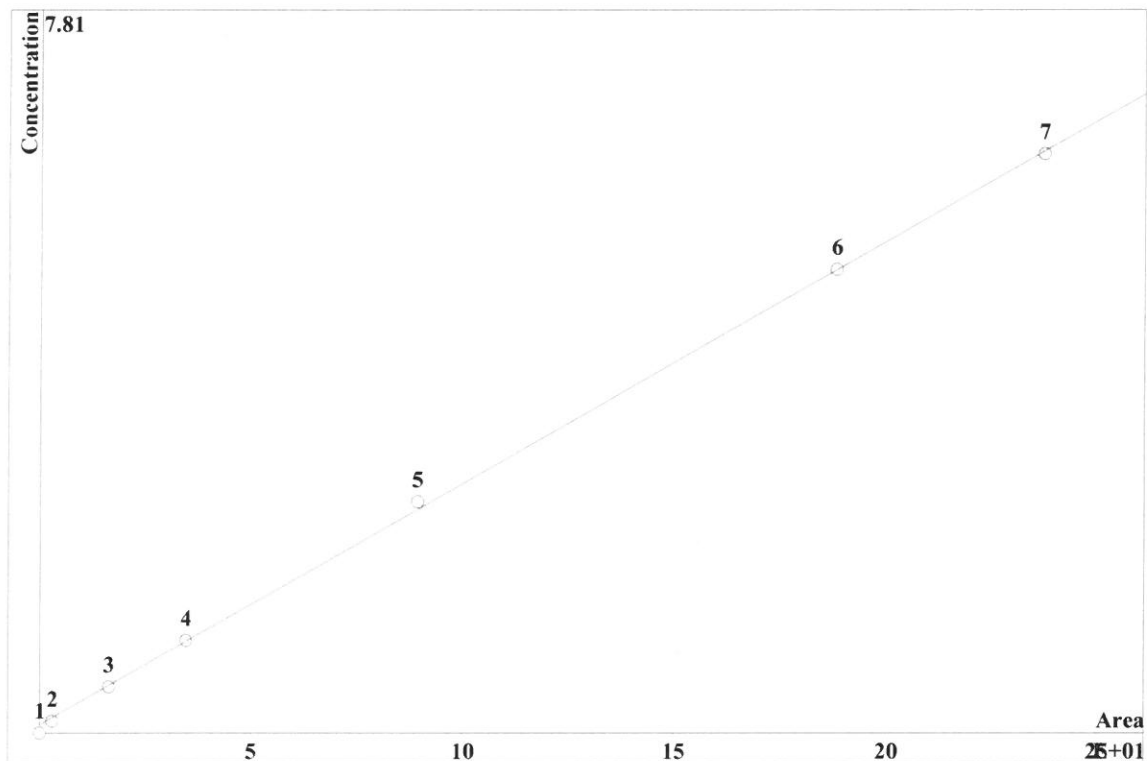


K3 = 0 K2 = 0 K1 = 0.521641 K0 = 1.78354
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.1166	3.012	0.125	20	14.11	Yes	
3	0.637	16.42	0.5	20	14.11	Yes	
4	1.334	34.64	1	20	14.11	Yes	
5	3.498	89.27	2.5	20	14.11	Yes	
6	7.391	188.2	5	20	14.11	Yes	
7	9.285	237.5	6.25	20	14.11	Yes	

±□;

CALIBRATION OF COMPONENT HPO4

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 1.42734 \cdot A - 5.10864$
 RSD: 3.656 %
 Correlation coefficient: 0.999454

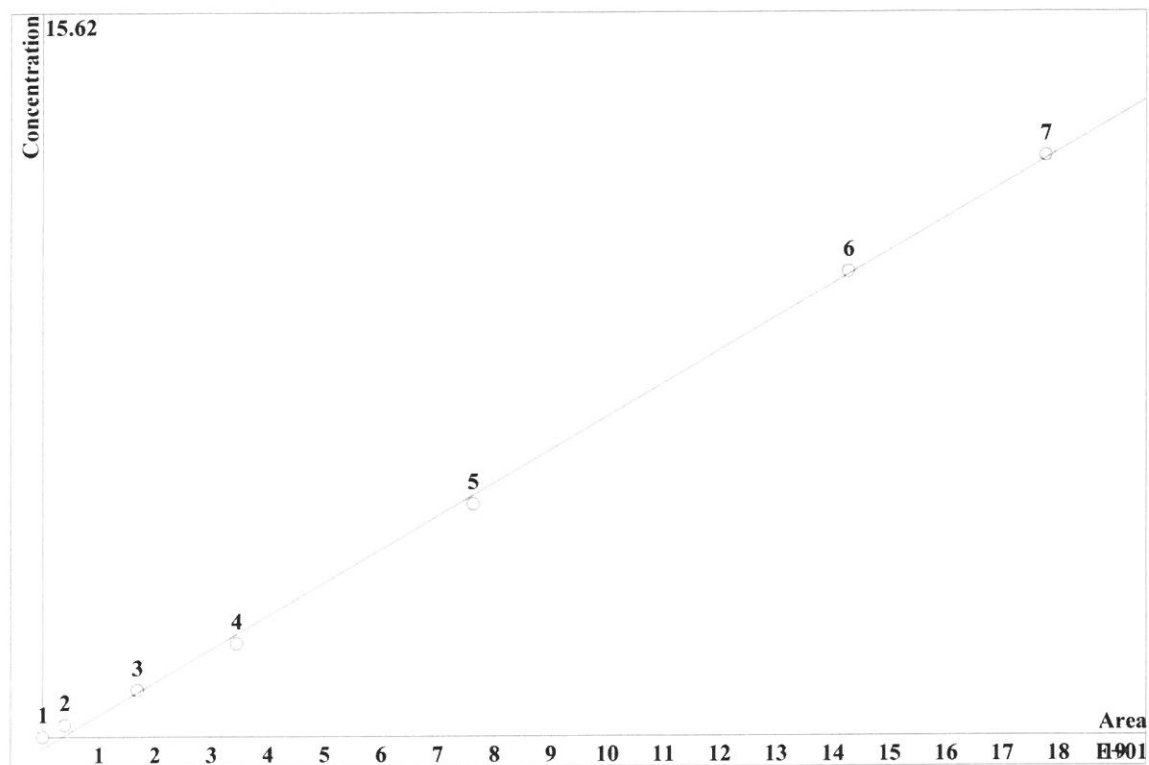


K3 = 0 K2 = 0 K1 = 1.42734 K0 = -5.10864
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0	0		No
2	0.06101	3.957	0.25	20	20.8	Yes	
3	0.2755	16.87	1	20	20.8	Yes	
4	0.5854	34.51	2	20	20.8	Yes	
5	1.384	76.34	5	20	20.8	Yes	
6	2.746	142.8	10	20	20.8	Yes	
7	3.493	177.8	12.5	20	20.8	Yes	

CALIBRATION OF COMPONENT SO4

Method: ANIONS 07-11-17.mtw
 Equation: $Q = 1.69309 \cdot A + 8.53567$
 RSD: 2.648 %
 Correlation coefficient: 0.999714

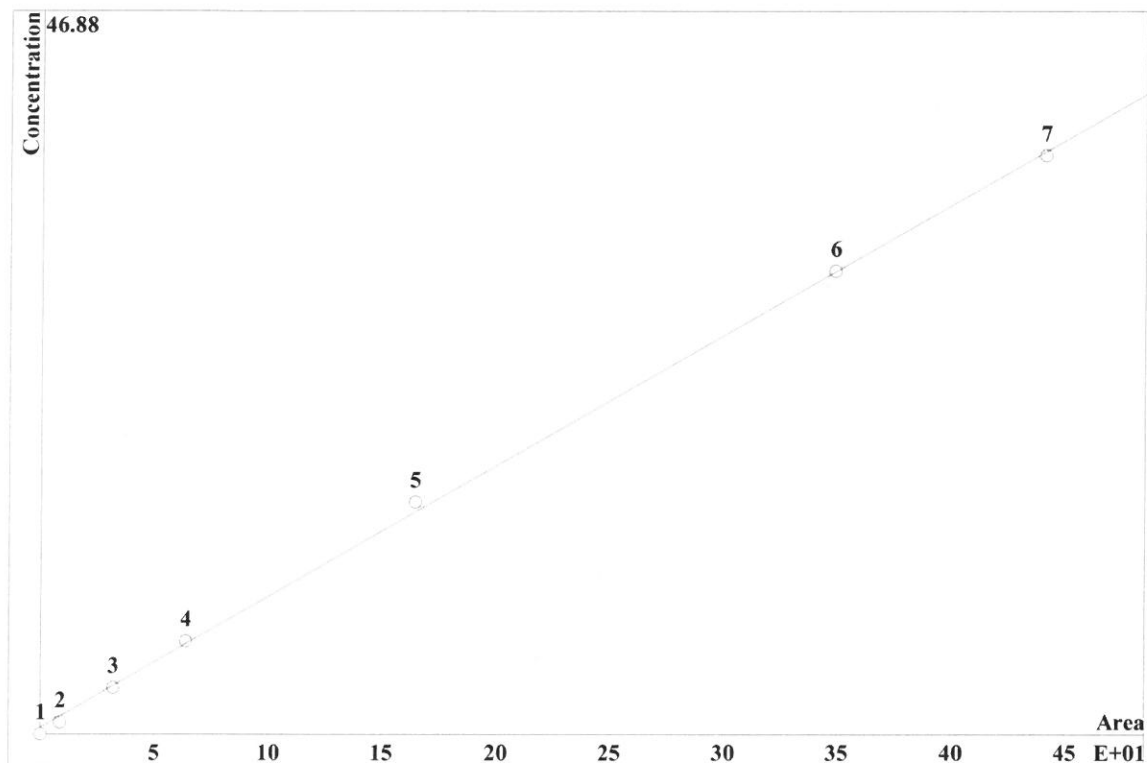

K3 = 0 K2 = 0 K1 = 1.69309 K0 = 8.53567
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		No
2	0.2149	8.665	0.75	20	23.28	Yes	
3	0.8445	32	3	20	23.28	Yes	
4	1.728	63.99	6	20	23.28	Yes	
5	4.535	164.8	15	20	23.28	Yes	
6	9.788	349	30	20	23.28	Yes	
7	12.4	441	37.5	20	23.28	Yes	

Report date: 7/11/2017 2:05:17 PM
Printed by: wet


Ident: STD1
Analysis from: 7/11/2017 10:41:58 AM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58337

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

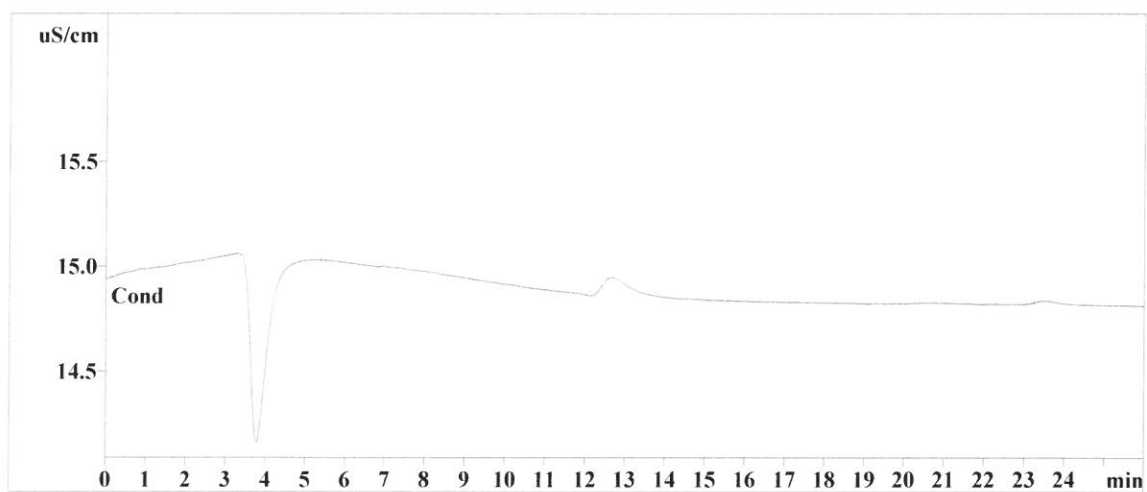

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:25 PM
Printed by: wet


Ident: STD2
Analysis from: 7/11/2017 11:10:54 AM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58338

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

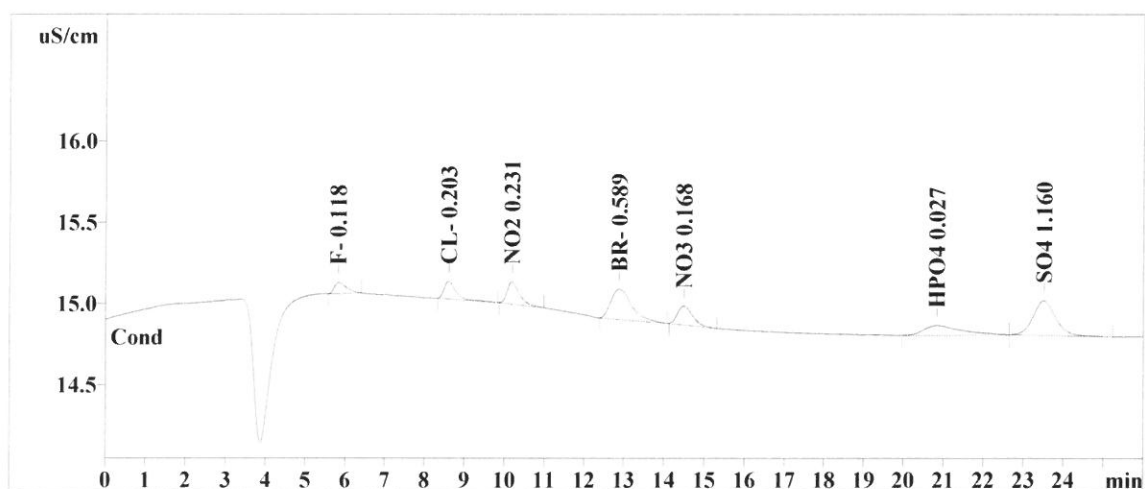

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.83	0.328	0.07	7.59	1.446	4.95	0.
2	8.59	0.298	0.11	12.10	2.297	7.86	0.
3	10.19	0.324	0.14	15.22	2.964	10.14	0.
4	12.89	0.548	0.19	20.90	6.887	23.56	0.
5	14.49	0.400	0.12	13.00	3.012	10.30	0.
6	20.82	0.957	0.06	6.73	3.957	13.54	0.
7	23.51	0.598	0.21	24.00	8.665	29.65	0.
7	26.00	0.493	0.89	99.54	29.228	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:31 PM
Printed by: wet


Ident: STD3
Analysis from: 7/11/2017 11:39:50 AM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58339

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

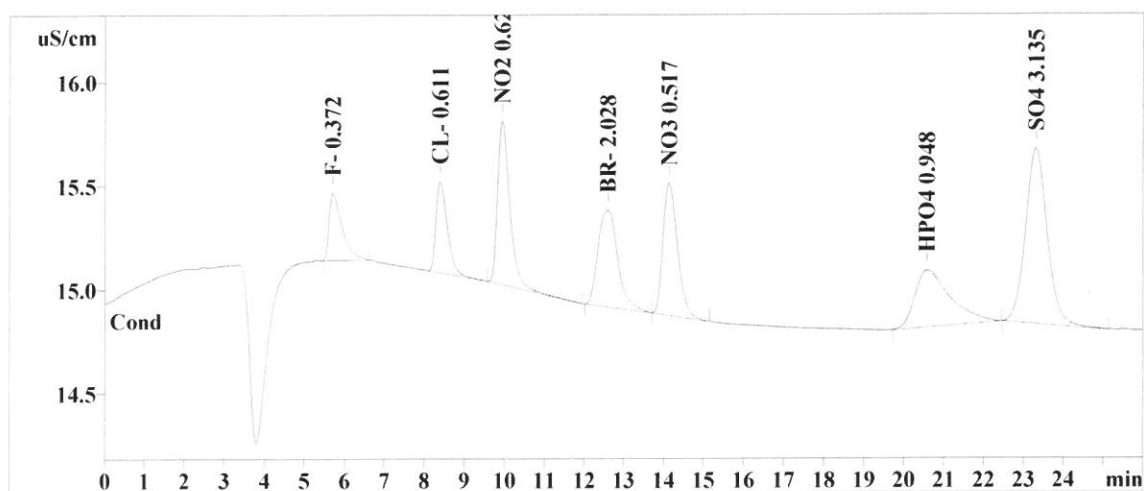

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.332	0.32	8.52	7.345	6.43	0.
2	8.40	0.288	0.44	11.62	8.457	7.40	0.
3	9.94	0.312	0.79	20.90	16.948	14.84	0.
4	12.60	0.530	0.47	12.36	16.210	14.19	0.
5	14.13	0.398	0.64	16.86	16.416	14.37	0.
6	20.58	0.901	0.27	7.28	16.866	14.76	0.
7	23.31	0.569	0.84	22.37	31.996	28.01	0.
7	26.00	0.476	3.77	99.93	114.237	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:36 PM
Printed by: wet


Ident: STD4
Analysis from: 7/11/2017 12:08:45 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58340

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

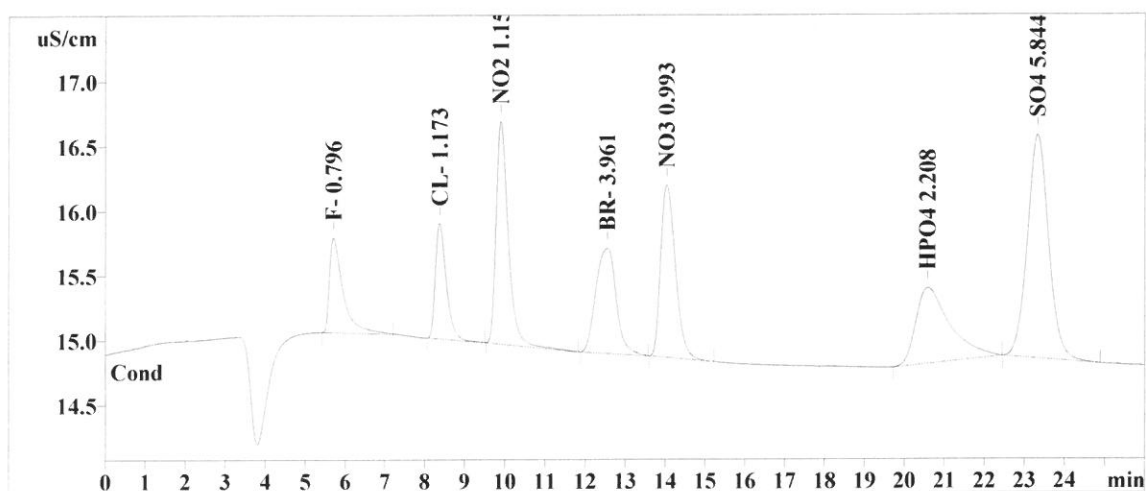

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.318	0.73	9.38	17.201	7.42	0.
2	8.38	0.283	0.90	11.46	16.942	7.30	0.
3	9.90	0.305	1.72	22.01	35.927	15.49	0.
4	12.56	0.550	0.82	10.44	28.734	12.39	0.
5	14.03	0.402	1.33	17.07	34.641	14.93	0.
6	20.59	0.852	0.59	7.49	34.514	14.88	0.
7	23.33	0.560	1.73	22.12	63.986	27.59	0.
7	26.00	0.467	7.81	99.96	231.946	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:45 PM
Printed by: wet


Ident: STD5
Analysis from: 7/11/2017 12:37:41 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58341

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

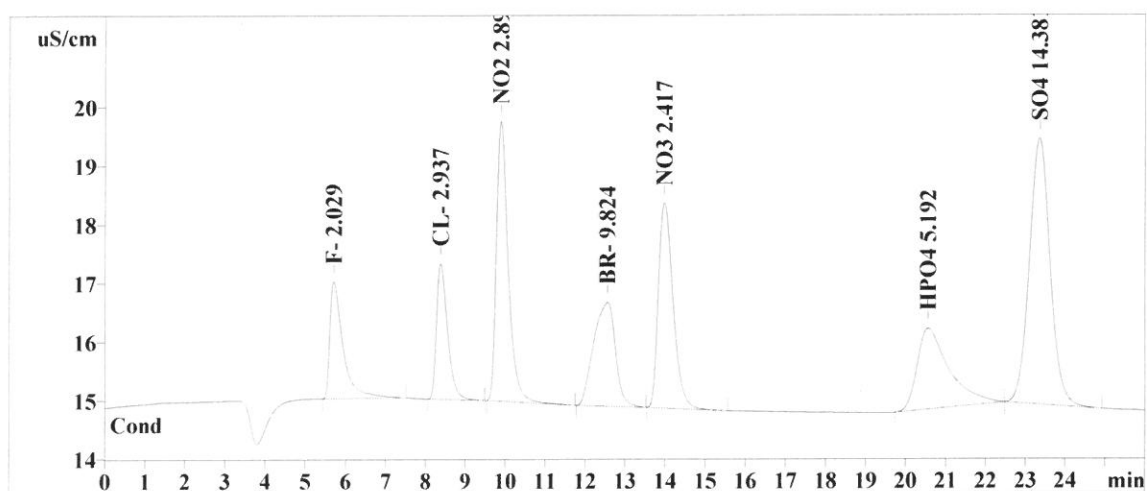

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.311	2.00	9.85	45.845	7.84	0.
2	8.38	0.281	2.31	11.41	43.598	7.46	0.
3	9.89	0.301	4.77	23.52	97.796	16.73	0.
4	12.57	0.607	1.78	8.77	66.713	11.42	0.
5	13.98	0.392	3.50	17.26	89.266	15.28	0.
6	20.56	0.782	1.38	6.83	76.335	13.06	0.
7	23.35	0.551	4.53	22.37	164.838	28.21	0.
7	26.00	0.461	20.27	99.99	584.391	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:52 PM
Printed by: wet


Ident: STD6
Analysis from: 7/11/2017 1:06:37 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:14 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58342

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AP/AK
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

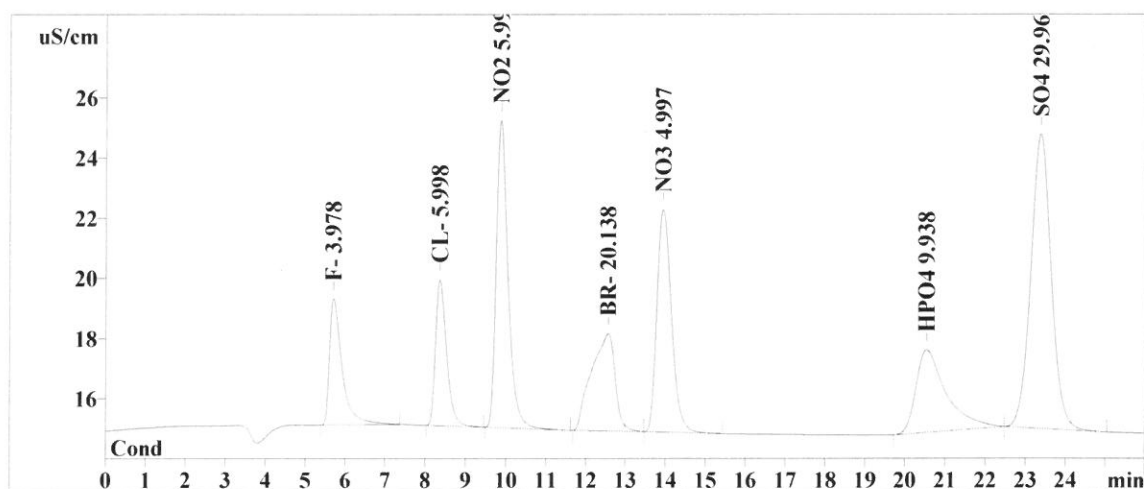

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.302	4.19	9.89	91.104	7.58	0.
2	8.36	0.277	4.83	11.40	89.840	7.47	0.
3	9.87	0.301	10.21	24.08	207.829	17.29	0.
4	12.56	0.706	3.24	7.64	133.522	11.11	0.
5	13.94	0.392	7.39	17.43	188.182	15.65	0.
6	20.53	0.726	2.75	6.48	142.827	11.88	0.
7	23.37	0.539	9.79	23.09	348.975	29.03	0.
7	26.00	0.463	42.40	100.00	1202.278	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/11/2017 2:05:59 PM
Printed by: wet


Ident: STD7
Analysis from: 7/11/2017 1:35:32 PM
File: _2017-07-11_

Last save: 7/11/2017 2:04:22 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58343

Last save: 7/11/2017 9:41:46 AM

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

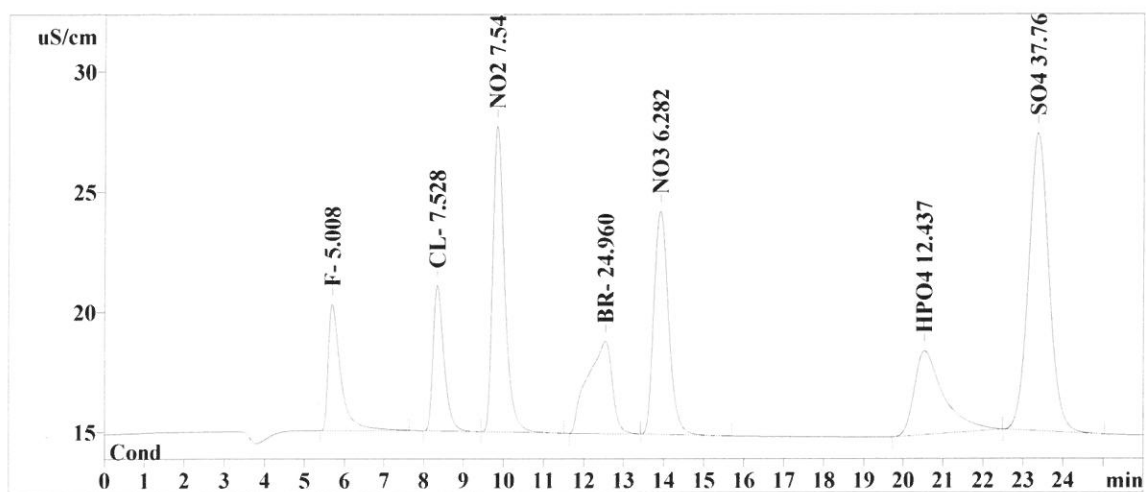

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.69	0.301	5.26	9.92	115.047	7.61	0.
2	8.34	0.278	6.06	11.41	112.966	7.47	0.
3	9.84	0.306	12.73	23.99	263.151	17.40	0.
4	12.54	0.768	3.86	7.26	164.756	10.89	0.
5	13.91	0.394	9.29	17.49	237.455	15.70	0.
6	20.53	0.708	3.49	6.58	177.848	11.76	0.
7	23.37	0.538	12.40	23.35	441.014	29.16	0.
7	26.00	0.471	53.09	100.00	1512.236	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2017 9:22:42 AM
Printed by: wet


Ident: ICV
Analysis from: 7/11/2017 3:03:18 PM
File: _2017-07-11_

Last save: 7/11/2017 3:29:08 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58346

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

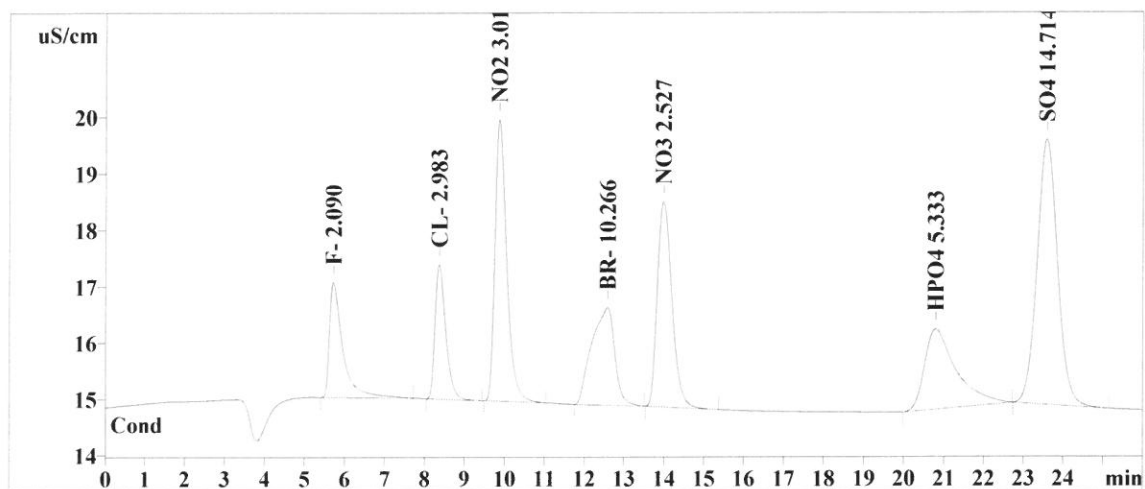

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.73	0.308	2.04	9.77	47.249	7.83	0.
2	8.37	0.278	2.39	11.39	44.295	7.34	0.
3	9.87	0.303	4.99	23.85	102.065	16.91	0.
4	12.59	0.673	1.74	8.31	69.572	11.52	0.
5	13.98	0.396	3.64	17.40	93.474	15.48	0.
6	20.79	0.774	1.43	6.83	78.312	12.97	0.
7	23.59	0.546	4.70	22.45	168.770	27.95	0.
7	26.00	0.468	20.93	99.99	603.737	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/12/2017 9:22:48 AM
Printed by: wet


Ident: ICB
Analysis from: 7/11/2017 3:32:14 PM
File: _2017-07-11_

Last save: 7/12/2017 9:21:56 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58347

Last save: 7/11/2017 2:01:22 PM

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

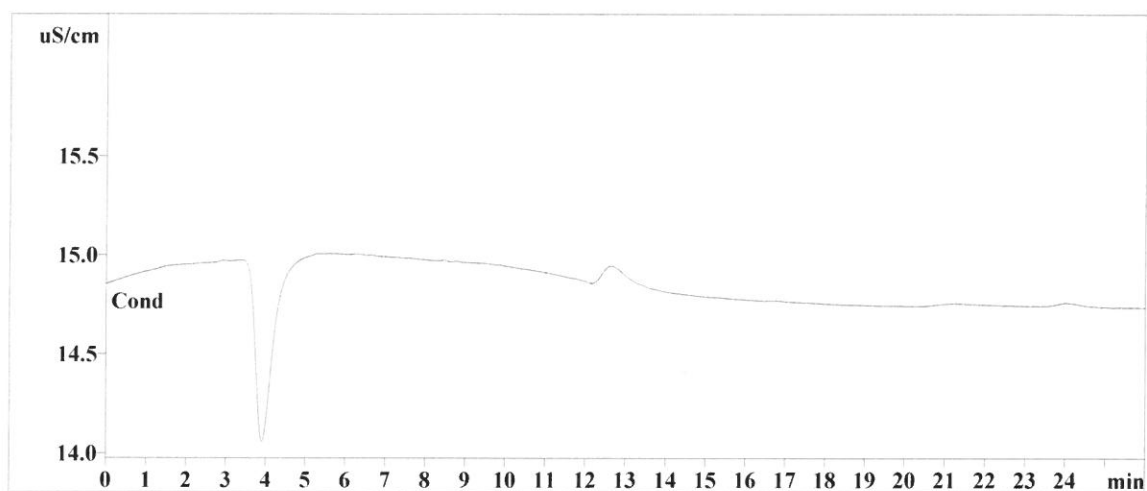

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 11:59:12 AM
Printed by: wet


Ident: CCV
Analysis from: 7/17/2017 3:46:11 PM
File: _2017-07-17_

Last save: 7/17/2017 4:12:02 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58392

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

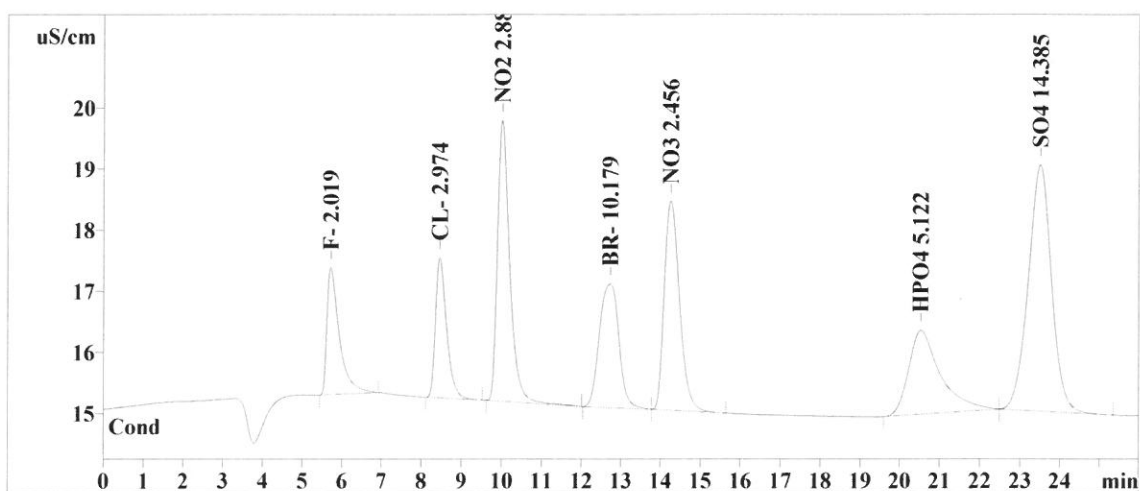

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.311	2.07	10.48	45.608	7.76	0.
2	8.46	0.288	2.29	11.57	44.155	7.52	0.
3	10.01	0.311	4.59	23.20	97.675	16.63	0.
4	12.73	0.537	2.03	10.23	69.008	11.75	0.
5	14.25	0.409	3.42	17.26	90.743	15.45	0.
6	20.52	0.772	1.37	6.93	75.356	12.83	0.
7	23.50	0.621	4.02	20.32	164.886	28.07	0.
7	26.00	0.464	19.79	99.99	587.432	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 11:59:39 AM
Printed by: wet


Ident: CCB
Analysis from: 7/17/2017 4:21:52 PM
File: _2017-07-17_

Last save: 7/18/2017 11:59:30 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58393

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

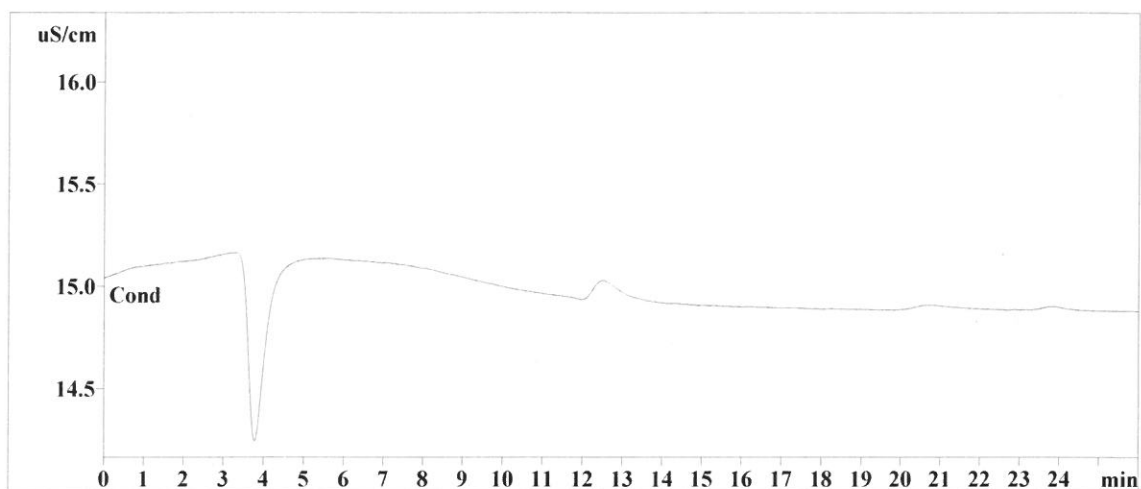

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 11:59:46 AM
Printed by: wet


Ident: LB88763BLW
Analysis from: 7/17/2017 4:50:48 PM
File: _2017-07-17_

Last save: 7/18/2017 11:59:32 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58394

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

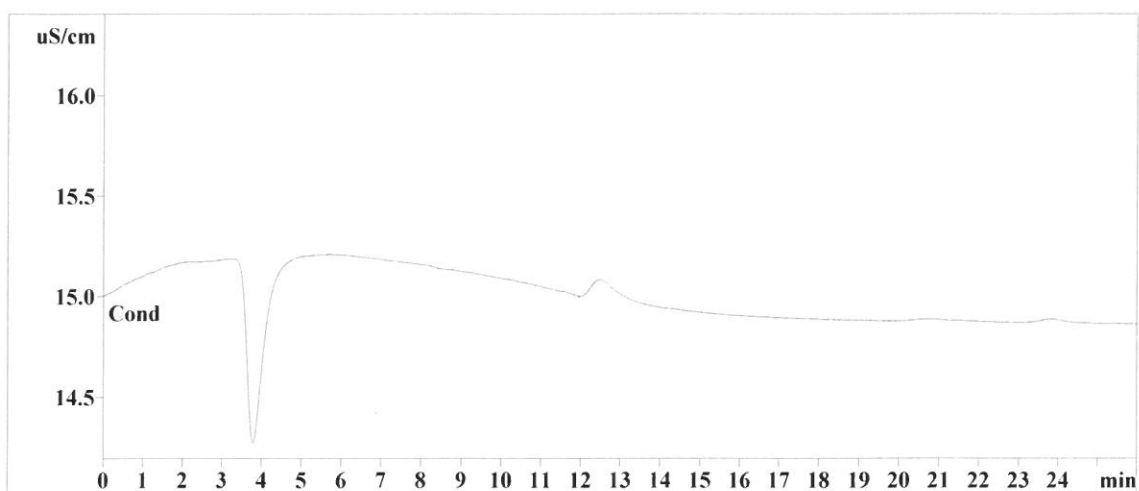

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:00:19 PM
Printed by: wet


Ident: LB88763BSW
Analysis from: 7/17/2017 5:19:43 PM
File: _2017-07-17_

Last save: 7/18/2017 11:59:02 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58395

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

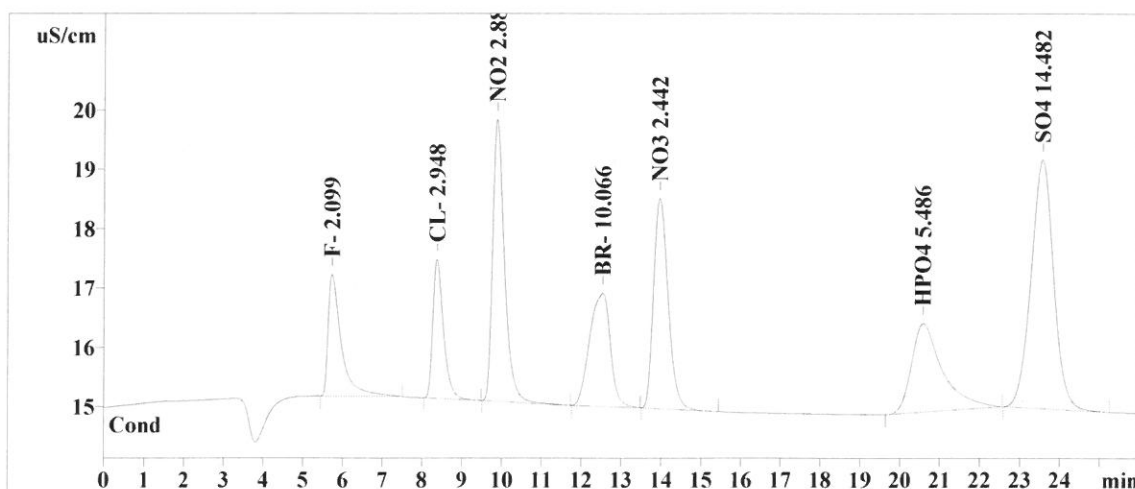

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.73	0.312	2.05	10.10	47.479	8.00	0.
2	8.37	0.279	2.34	11.55	43.764	7.37	0.
3	9.88	0.301	4.75	23.43	97.541	16.43	0.
4	12.54	0.570	1.91	9.41	68.280	11.50	0.
5	13.95	0.393	3.54	17.46	90.212	15.19	0.
6	20.58	0.754	1.49	7.35	80.450	13.55	0.
7	23.55	0.601	4.19	20.68	166.029	27.96	0.
7	26.00	0.459	20.26	99.99	593.755	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:00:36 PM
Printed by: wet


Ident: I4234-01
Analysis from: 7/17/2017 5:48:39 PM
File: _2017-07-17_

Last save: 7/17/2017 6:14:28 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58396

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

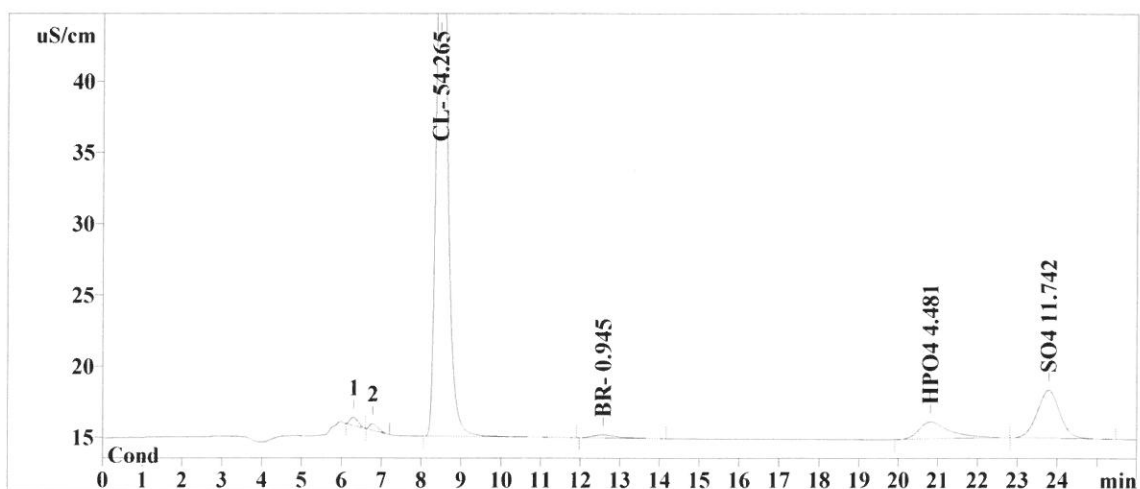

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	0.00	0.000	0.00	0.00	0.000	0.00	0.
2	8.47	0.269	44.86	88.49	819.069	78.44	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	12.58	0.602	0.22	0.43	9.194	0.88	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	20.81	0.767	1.21	2.38	66.371	6.36	0.
7	23.78	0.603	3.37	6.66	133.659	12.80	0.
7	26.00	0.320	49.65	97.95	1028.292	98.47	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:00:46 PM
Printed by: wet


Ident: I4234-02
Analysis from: 7/17/2017 6:17:35 PM
File: _2017-07-17_

Last save: 7/17/2017 6:43:24 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58397

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

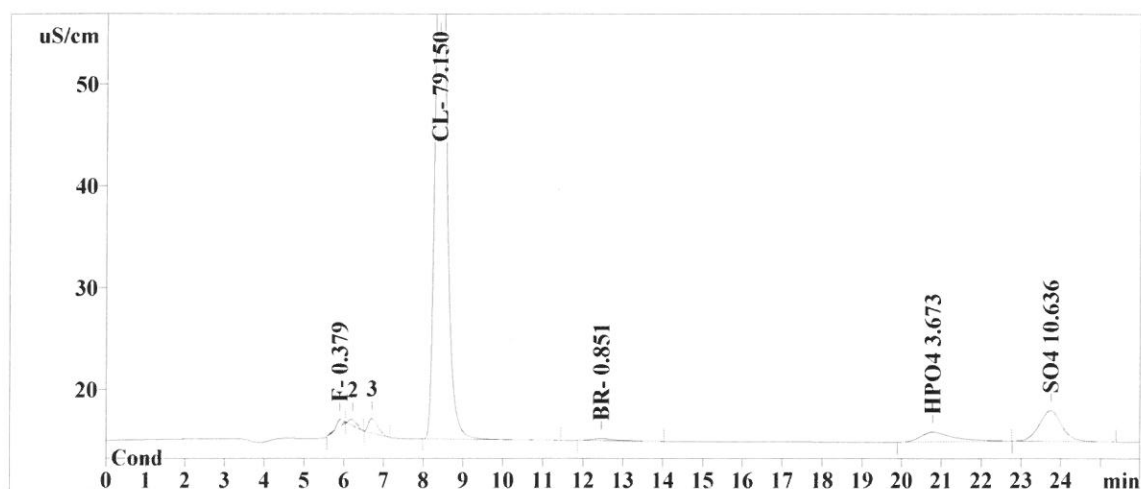

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.158	0.71	1.02	7.514	0.53	0.
2	8.40	0.284	63.01	90.09	1195.042	84.24	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	12.46	0.603	0.20	0.29	8.585	0.61	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	20.78	0.807	0.96	1.37	55.052	3.88	0.
7	23.74	0.604	3.02	4.31	120.593	8.50	0.
7	26.00	0.351	67.90	97.08	1386.786	97.75	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:00:57 PM
Printed by: wet


Ident: I4234-04
Analysis from: 7/17/2017 6:46:30 PM
File: _2017-07-17_

Last save: 7/17/2017 7:12:20 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58398

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

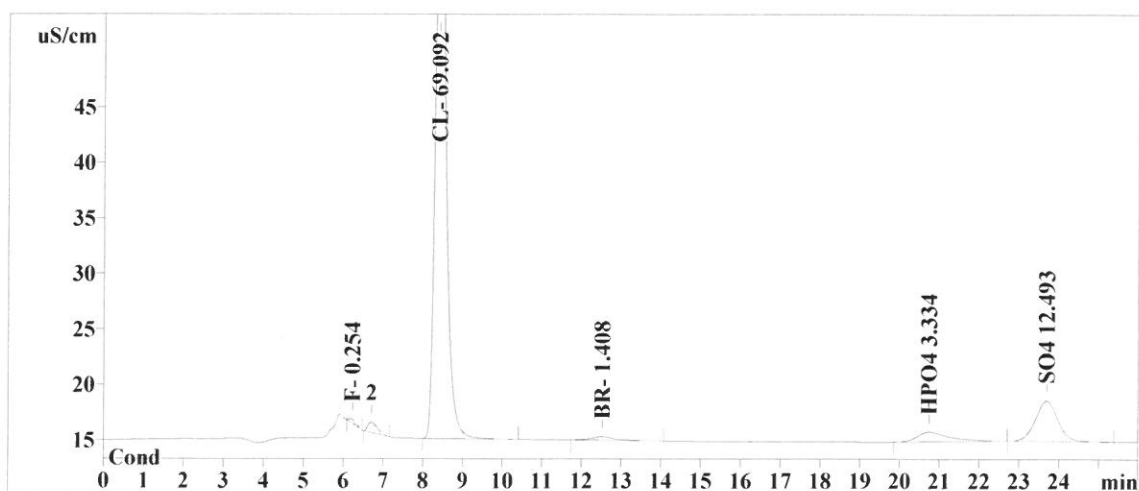

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	6.22	0.215	0.36	0.57	4.622	0.36	0.
2	8.40	0.269	57.74	90.38	1043.089	82.24	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	12.52	0.540	0.32	0.50	12.195	0.96	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	20.74	0.802	0.88	1.38	50.294	3.97	0.
7	23.69	0.594	3.63	5.69	142.532	11.24	0.
7	26.00	0.346	62.93	98.51	1252.732	98.76	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:01:07 PM
Printed by: wet


Ident: I4234-04DUP
Analysis from: 7/17/2017 7:15:26 PM
File: _2017-07-17_

Last save: 7/17/2017 7:41:16 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58399

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

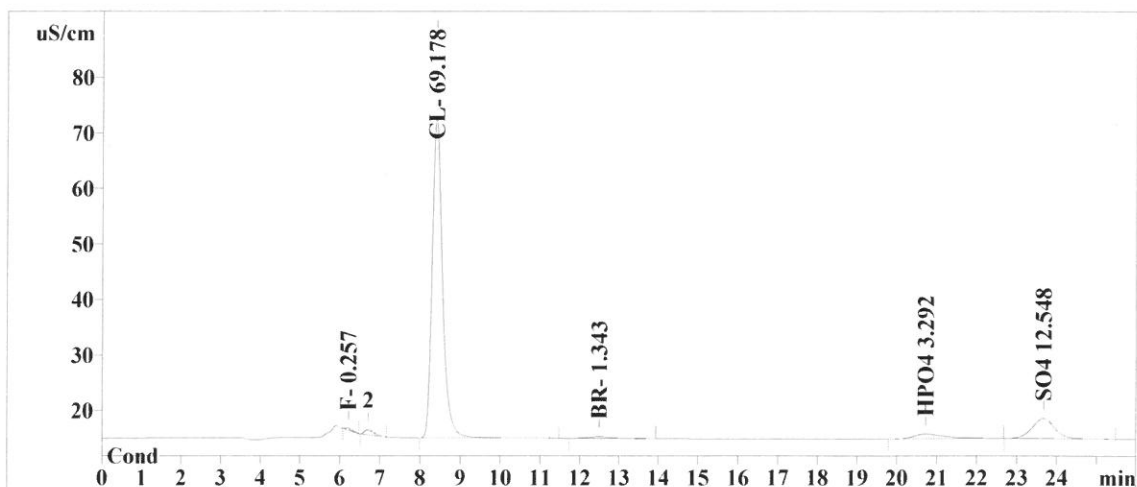

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	6.22	0.215	0.37	0.57	4.694	0.37	0.
2	8.40	0.268	57.73	90.42	1044.379	82.30	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	12.49	0.530	0.32	0.50	11.771	0.93	0.
5	0.00	0.000	0.00	0.00	0.000	0.00	0.
6	20.73	0.799	0.87	1.37	49.711	3.92	0.
7	23.67	0.600	3.62	5.67	143.183	11.28	0.
7	26.00	0.345	62.91	98.53	1253.738	98.79	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:01:20 PM
Printed by: wet


Ident: I4234-04MS
Analysis from: 7/17/2017 7:44:21 PM
File: _2017-07-17_

Last save: 7/17/2017 8:10:10 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58400

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

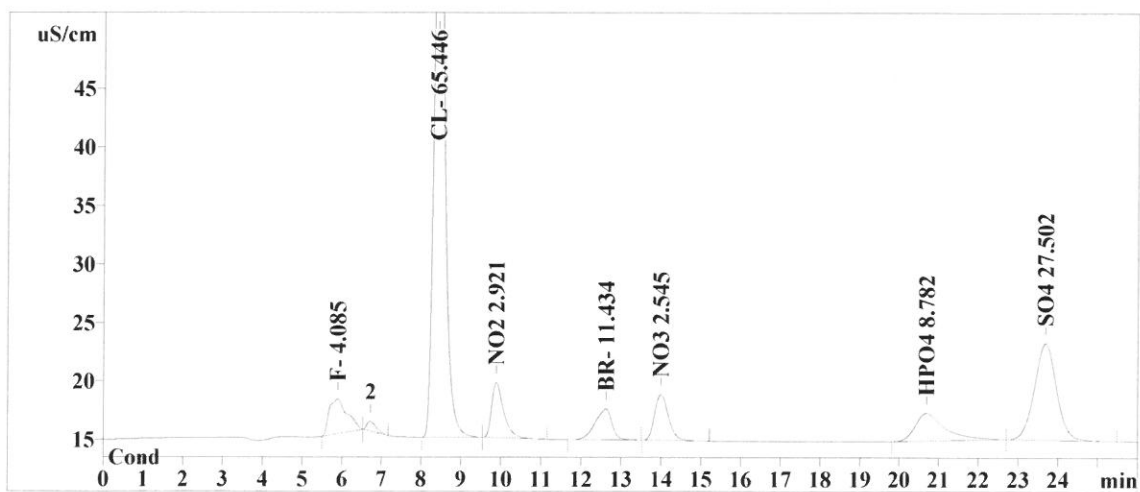

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.89	0.520	2.97	3.69	93.608	5.17	0.
2	8.41	0.269	54.83	68.06	988.002	54.53	0.
3	9.89	0.308	4.71	5.85	98.819	5.45	0.
4	12.62	0.451	2.66	3.30	77.141	4.26	0.
5	13.99	0.371	3.91	4.86	94.157	5.20	0.
6	20.68	0.736	2.38	2.95	126.639	6.99	0.
7	23.68	0.588	8.25	10.25	319.833	17.65	0.
7	26.00	0.463	79.72	98.95	1798.200	99.24	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:01:30 PM
Printed by: wet


Ident: CCV
Analysis from: 7/17/2017 8:13:17 PM
File: _2017-07-17_

Last save: 7/17/2017 8:39:06 PM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58401

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

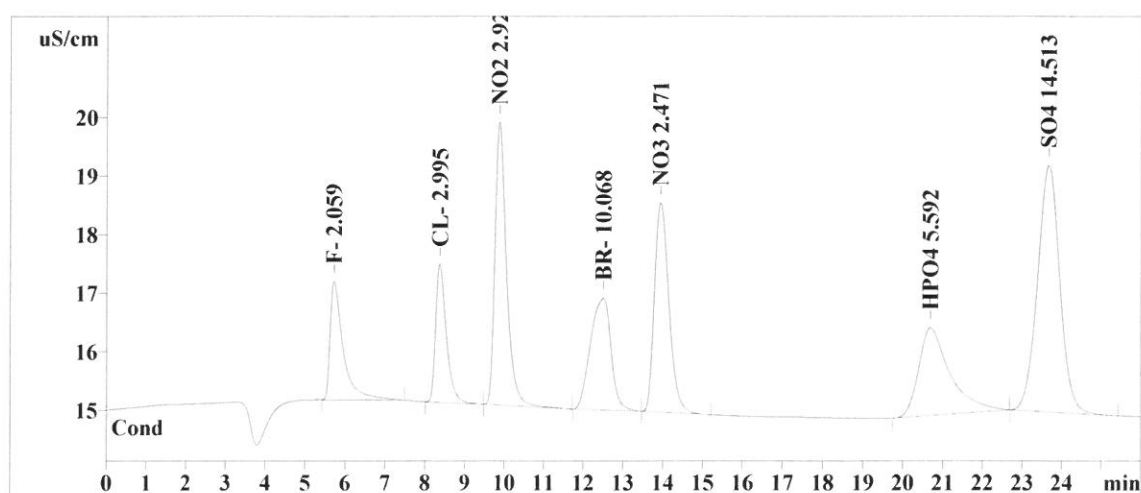

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.309	2.02	9.90	46.529	7.78	0.
2	8.36	0.279	2.36	11.57	44.481	7.44	0.
3	9.87	0.300	4.83	23.67	98.825	16.53	0.
4	12.50	0.568	1.91	9.36	68.289	11.42	0.
5	13.93	0.394	3.57	17.49	91.317	15.28	0.
6	20.68	0.761	1.50	7.36	81.933	13.71	0.
7	23.66	0.600	4.21	20.65	166.397	27.84	0.
7	26.00	0.459	20.41	99.99	597.771	100.00	0.

This report has been created by IC Net
METROHM LTD

Report date: 7/18/2017 12:01:38 PM
Printed by: wet


Ident: CCB
Analysis from: 7/17/2017 8:42:12 PM
File: _2017-07-17_

Last save: 7/18/2017 11:59:32 AM

Method: ANIONS 07-11-17.mtw
Run operator: wet
Analysis number: 58402

Last save: 7/14/2017 10:59:46 AM

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

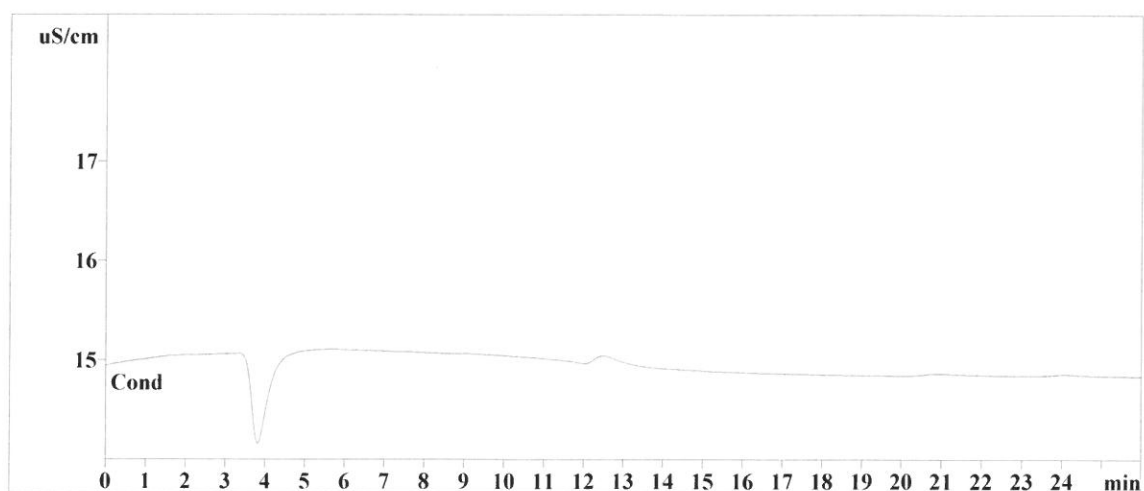

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD