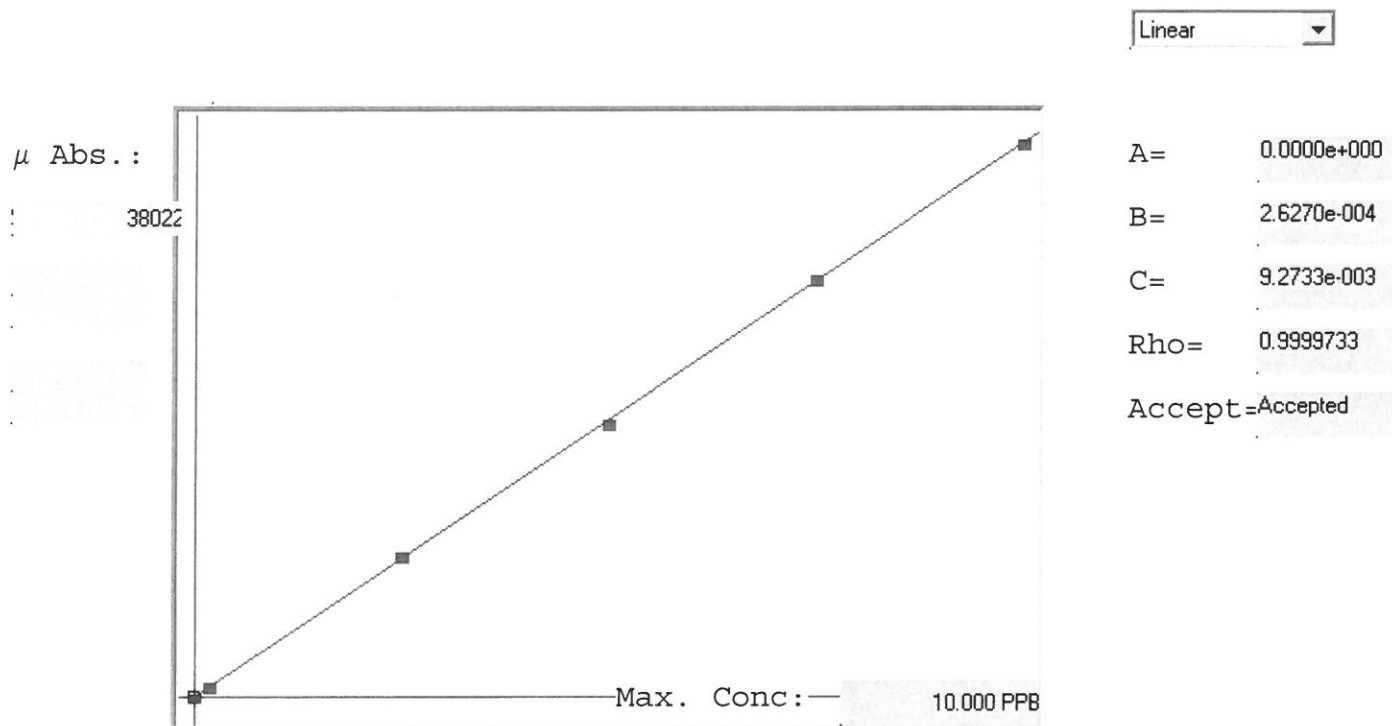


7471A

LB88836
INSTRUMENT 10: CV2

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.000	0.000	-34	0.000	-34				
0.2	0.200	0.193	-0.007	698	0.0 %	698				
2.5	2.500	2.535	0.035	9614	0.0 %	9614				
5.0	5.000	4.950	-0.050	18808	0.0 %	18808				
7.5	7.500	7.525	0.025	28608	0.0 %	28608	0			
10.0	10.000	9.998	-0.002	38022	0.0 %	38022				

LB88836 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 20 Jul 2017 14:46:25

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-34	-	0.00007471A	PPB		20 Jul 2017 14:48:43	S	Std
0.2 - 1	50.2	698	-	0.20007471A	PPB		20 Jul 2017 14:51:01	S	Std
2.5 - 1	52.5	9614	-	2.50007471A	PPB		20 Jul 2017 14:53:18	S	Std
5.0 - 1	55	18808	-	5.00007471A	PPB		20 Jul 2017 14:55:36	S	Std
7.5 - 1	57.5	28608	-	7.50007471A	PPB		20 Jul 2017 14:57:53	S	Std
10.0 - 1	510	38022	-	10.00007471A	PPB		20 Jul 2017 15:00:09	S	Std
ICV68 - 1	ICV68	14789	3.8943	-7471A	PPB		20 Jul 2017 15:02:55	U	SMPL
ICB68 - 1	ICB68	-184	-0.0391	-7471A	PPB		20 Jul 2017 15:05:10	U	SMPL
CCV57 - 1	CCV57	19277	5.0733	-7471A	PPB		20 Jul 2017 15:07:26	U	SMPL
CCB57 - 1	CCB57	-181	-0.0383	-7471A	PPB		20 Jul 2017 15:09:42	U	SMPL
CRA - 1	CRA	725	0.1997	-7471A	PPB		20 Jul 2017 15:11:58	U	SMPL
HighStd - 1	HighStd	38369	10.0887	-7471A	PPB		20 Jul 2017 15:14:14	U	SMPL
ChkStd - 1	ChkStd	27240	7.1652	-7471A	PPB		20 Jul 2017 15:16:30	U	SMPL
PB100782BL - 1	PBS	-230	-0.0511	-7471A	PPB		20 Jul 2017 15:18:48	U	SMPL
PB100782BS - 1	LCSS	13354	3.5173	-7471A	PPB		20 Jul 2017 15:21:07	U	SMPL
I4282-01 - 1	FK-GF-02-007-A	1978	0.5289	-7471A	PPB		20 Jul 2017 15:23:24	U	SMPL
I4282-01DUP - 1	FK-GF-02-007-ADUP	1767	0.4735	-7471A	PPB		20 Jul 2017 15:28:22	U	SMPL
I4282-01MS - 1	FK-GF-02-007-AMS	16494	4.3422	-7471A	PPB		20 Jul 2017 15:30:39	U	SMPL
I4282-01MSD - 1	FK-GF-02-007-AMSD	16297	4.2905	-7471A	PPB		20 Jul 2017 15:32:57	U	SMPL
I4282-03 - 1	FK-GF-02-007-B	1528	0.4107	-7471A	PPB		20 Jul 2017 15:35:13	U	SMPL
CCV58 - 1	CCV58	19494	5.1303	-7471A	PPB		20 Jul 2017 15:37:29	U	SMPL
CCB58 - 1	CCB58	-168	-0.0349	-7471A	PPB		20 Jul 2017 15:39:45	U	SMPL
I4290-01 - 1	S-1	3017	0.8018	-7471A	PPB		20 Jul 2017 15:42:01	U	SMPL
I4290-02 - 1	S-2	523	0.1467	-7471A	PPB		20 Jul 2017 15:44:17	U	SMPL
I4290-03 - 1	S-3	1079	0.2927	-7471A	PPB		20 Jul 2017 15:46:33	U	SMPL
I4290-04 - 1	S-4	851	0.2328	-7471A	PPB		20 Jul 2017 15:48:50	U	SMPL
I4290-05 - 1	S-5	977	0.2659	-7471A	PPB		20 Jul 2017 15:51:06	U	SMPL
I4305-02 - 1	E2-N5-WSW	36481	9.5927	-7471A	PPB		20 Jul 2017 15:53:23	U	SMPL
I4305-03 - 1	E2-N5-BASE	50388	13.2461	-7471A	PPB		20 Jul 2017 15:55:41	U	SMPL
I4305-04 - 1	E2-M5-BASE	102541	26.9465	-7471A	PPB		20 Jul 2017 15:58:00	U	SMPL
I4305-05 - 1	E2-M5-WSW	121116	31.8262	-7471A	PPB		20 Jul 2017 16:00:20	U	SMPL
I4308-01 - 1	NB-08-071917	3858	1.0228	-7471A	PPB		20 Jul 2017 16:02:39	U	SMPL
CCV59 - 1	CCV59	19319	5.0843	-7471A	PPB		20 Jul 2017 16:04:58	U	SMPL
CCB59 - 1	CCB59	-182	-0.0385	-7471A	PPB		20 Jul 2017 16:07:15	U	SMPL
I4312-01 - 1	VNJ-209	464	0.1312	-7471A	PPB		20 Jul 2017 16:09:31	U	SMPL
I4312-05 - 1	72-11987	464	0.1312	-7471A	PPB		20 Jul 2017 16:11:47	U	SMPL
I4312-09 - 1	72-11978	551	0.1540	-7471A	PPB		20 Jul 2017 16:14:03	U	SMPL
I4312-13 - 1	VNJ-237	595	0.1656	-7471A	PPB		20 Jul 2017 16:16:19	U	SMPL
I4312-17 - 1	156	1458	0.3923	-7471A	PPB		20 Jul 2017 16:18:36	U	SMPL
I4316-01 - 1	OR-02-071917	3970	1.0522	-7471A	PPB		20 Jul 2017 16:20:53	U	SMPL
I4317-01 - 1	SP-1-TP-1-2-3-COMP	379	0.1088	-7471A	PPB		20 Jul 2017 16:23:10	U	SMPL
I4319-01 - 1	B-2(0-6)COMP	2359	0.6290	-7471A	PPB		20 Jul 2017 16:25:28	U	SMPL
I4282-01LX5 - 1		298	0.0876	-7471A	PPB		20 Jul 2017 16:27:45	U	SMPL
I4282-01A - 1		17276	4.5476	-7471A	PPB		20 Jul 2017 16:30:02	U	SMPL
CCV60 - 1	CCV60	19550	5.1450	-7471A	PPB		20 Jul 2017 16:32:18	U	SMPL
CCB60 - 1	CCB60	-145	-0.0288	-7471A	PPB		20 Jul 2017 16:34:34	U	SMPL
I4305-03DLX2 - 1		25653	6.7483	-7471A	PPB		20 Jul 2017 16:39:25	U	SMPL
I4305-04DLX5 - 1		20640	5.4314	-7471A	PPB		20 Jul 2017 16:41:41	U	SMPL
I4305-05DLX5 - 1		24296	6.3918	-7471A	PPB		20 Jul 2017 16:43:58	U	SMPL
CCV61 - 1	CCV61	19153	5.0407	-7471A	PPB		20 Jul 2017 16:46:15	U	SMPL
CCB61 - 1	CCB61	-176	-0.0370	-7471A	PPB		20 Jul 2017 16:48:33	U	SMPL