

245.1


L988863

INSTRUMENT ID: CV1

Linear

 $\mu$  Abs.:

29256

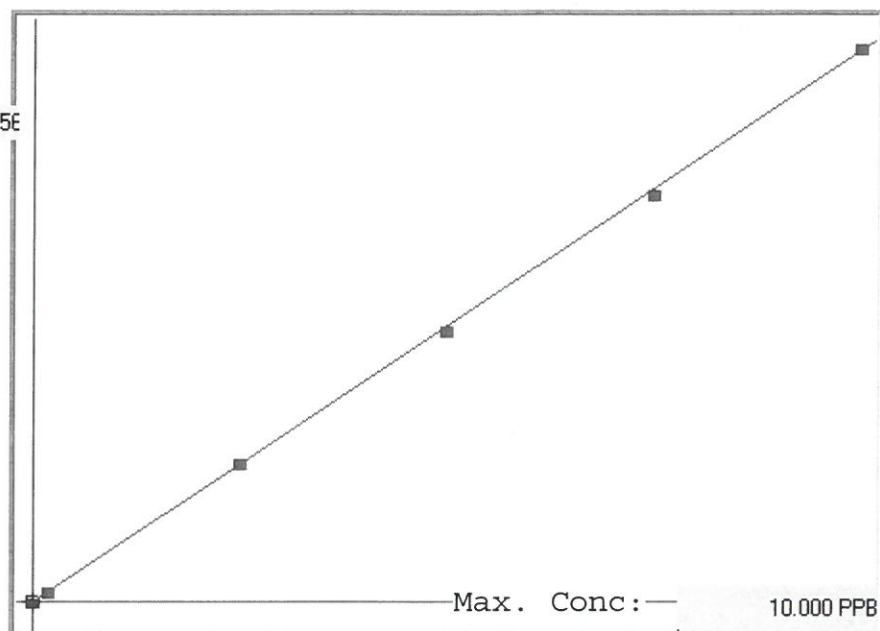

A= 0.0000e+000

B= 3.4372e-004

C= 1.8988e-002

Rho= 0.9999046

Accept=Accepted

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|
| 0.0    | 0.000  | 0.014  | 0.014  | -15   | 0.000      | -15   |       |       |       |       |
| 0.2    | 0.200  | 0.209  | 0.009  | 554   | 0.0 %      | 554   |       |       |       |       |
| 2.5    | 2.500  | 2.531  | 0.031  | 7309  | 0.0 %      | 7309  |       |       |       |       |
| 5.0    | 5.000  | 4.950  | -0.050 | 14345 | 0.0 %      | 14345 |       |       |       |       |
| 7.5    | 7.500  | 7.421  | -0.079 | 21536 | 0.0 %      | 21536 |       |       |       |       |
| 10.0   | 10.000 | 10.075 | 0.075  | 29256 | 0.0 %      | 29256 |       |       |       |       |

## LB88863 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 21 Jul 2017 10:16:47

| Sample ID       | Extended ID | $\mu$ Abs. | Conc.   | Std Conc | Method | Units | Date                 | Type | Type |
|-----------------|-------------|------------|---------|----------|--------|-------|----------------------|------|------|
| 0.0 - 1         | 50          | -15        | -       | 0.0000   | 245.1  | PPB   | 21 Jul 2017 10:21:34 | S    | Std  |
| 0.2 - 1         | 50.2        | 554        | -       | 0.2000   | 245.1  | PPB   | 21 Jul 2017 10:23:42 | S    | Std  |
| 2.5 - 1         | 52.5        | 7309       | -       | 2.5000   | 245.1  | PPB   | 21 Jul 2017 10:25:51 | S    | Std  |
| 5.0 - 1         | 55          | 14345      | -       | 5.0000   | 245.1  | PPB   | 21 Jul 2017 10:27:59 | S    | Std  |
| 7.5 - 1         | 57.5        | 21536      | -       | 7.5000   | 245.1  | PPB   | 21 Jul 2017 10:30:07 | S    | Std  |
| 10.0 - 1        | 510         | 29256      | -       | 10.0000  | 245.1  | PPB   | 21 Jul 2017 10:32:15 | S    | Std  |
| ICV69 - 1       | ICV69       | 11333      | 3.9143  | -245.1   |        | PPB   | 21 Jul 2017 10:34:47 | U    | SMPL |
| ICB69 - 1       | ICB69       | -161       | -0.0363 | -245.1   |        | PPB   | 21 Jul 2017 10:36:54 | U    | SMPL |
| CCV62 - 1       | CCV62       | 14424      | 4.9767  | -245.1   |        | PPB   | 21 Jul 2017 10:39:01 | U    | SMPL |
| CCB62 - 1       | CCB62       | -152       | -0.0333 | -245.1   |        | PPB   | 21 Jul 2017 10:41:07 | U    | SMPL |
| CRA - 1         | CRA         | 530        | 0.2012  | -245.1   |        | PPB   | 21 Jul 2017 10:43:15 | U    | SMPL |
| HighStd - 1     | HighStd     | 29317      | 10.0957 | -245.1   |        | PPB   | 21 Jul 2017 10:45:22 | U    | SMPL |
| ChkStd - 1      | ChkStd      | 20366      | 7.0191  | -245.1   |        | PPB   | 21 Jul 2017 10:47:29 | U    | SMPL |
| PB100806BL - 1  | PBW         | -190       | -0.0463 | -245.1   |        | PPB   | 21 Jul 2017 10:49:37 | U    | SMPL |
| PB100806BS - 1  | LCSW        | 11372      | 3.9277  | -245.1   |        | PPB   | 21 Jul 2017 10:54:08 | U    | SMPL |
| I4313-01 - 1    | M-COMB-8    | 45         | 0.0345  | -245.1   |        | PPB   | 21 Jul 2017 10:56:15 | U    | SMPL |
| I4313-01DUP - 1 | M-COMB-8DUP | 139        | 0.0668  | -245.1   |        | PPB   | 21 Jul 2017 10:58:24 | U    | SMPL |
| I4313-01MS - 1  | M-COMB-8MS  | 11550      | 3.9889  | -245.1   |        | PPB   | 21 Jul 2017 11:00:32 | U    | SMPL |
| I4313-01MSD - 1 | M-COMB-8MSD | 11378      | 3.9298  | -245.1   |        | PPB   | 21 Jul 2017 11:02:40 | U    | SMPL |
| I4313-02 - 1    | M-COMB-9    | -75        | -0.0068 | -245.1   |        | PPB   | 21 Jul 2017 11:04:48 | U    | SMPL |
| CCV63 - 1       | CCV63       | 14139      | 4.8788  | -245.1   |        | PPB   | 21 Jul 2017 11:06:54 | U    | SMPL |
| CCB63 - 1       | CCB63       | -134       | -0.0271 | -245.1   |        | PPB   | 21 Jul 2017 11:09:00 | U    | SMPL |
| I4313-03 - 1    | B-COMB-1    | 63         | 0.0406  | -245.1   |        | PPB   | 21 Jul 2017 11:11:08 | U    | SMPL |
| I4313-01LX5 - 1 |             | 0          | 0.0190  | -245.1   |        | PPB   | 21 Jul 2017 11:13:15 | U    | SMPL |
| I4313-01A - 1   |             | 13011      | 4.4911  | -245.1   |        | PPB   | 21 Jul 2017 11:15:22 | U    | SMPL |
| CCV64 - 1       | CCV64       | 14293      | 4.9317  | -245.1   |        | PPB   | 21 Jul 2017 11:17:30 | U    | SMPL |
| CCB64 - 1       | CCB64       | -114       | -0.0202 | -245.1   |        | PPB   | 21 Jul 2017 11:19:37 | U    | SMPL |