


ISM02.4

LB88872
INSTRUMENT ID: CV2

Linear

 μ Abs.:

41343

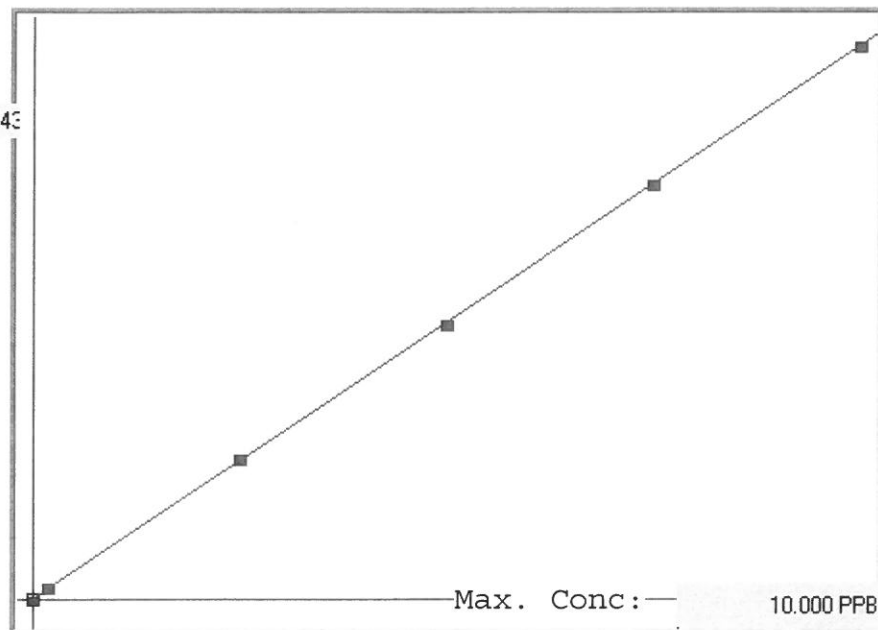

A= 0.0000e+000

B= 2.4228e-004

C= -5.9406e-003

Rho= 0.9999805

Accept=Accepted

slope
Y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	-0.015	-0.015	-37	0.000	-37					-
0.2	0.200	0.209	0.009	889	0.0 %	889					4
2.5	2.500	2.534	0.034	10485	0.0 %	10485					1
5.0	5.000	4.960	-0.040	20498	0.0 %	20498					-1
7.5	7.500	7.500	0.000	30981	0.0 %	30981					0
10.0	10.000	10.011	0.011	41343	0.0 %	41343					0

NB
7/12/17

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	-37	-		0 ISM02.4	PPB	7/21/2017 14:09	Std
	0.2 S0.2	889	-		0.2 ISM02.4	PPB	7/21/2017 14:11	Std
	2.5 S2.5	10485	-		2.5 ISM02.4	PPB	7/21/2017 14:14	Std
	5 S5	20498	-		5 ISM02.4	PPB	7/21/2017 14:16	Std
	7.5 S7.5	30981	-		7.5 ISM02.4	PPB	7/21/2017 14:18	Std
	10 S10	41343	-		10 ISM02.4	PPB	7/21/2017 14:21	Std
ICV	ICV	16011	3.8732 -		ISM02.4	PPB	7/21/2017 14:23	SMPL
ICB	ICB	-182	-0.05 -		ISM02.4	PPB	7/21/2017 14:26	SMPL
CCV069	CCV069	20645	4.9959 -		ISM02.4	PPB	7/21/2017 14:28	SMPL
CCB069	CCB069	-170	-0.0471 -		ISM02.4	PPB	7/21/2017 14:30	SMPL
PB100819BL	PBS004	-40	-0.0156 -		ISM02.4	PPB	7/21/2017 14:32	SMPL
I4260-01	MBDX22	318	0.0711 -		ISM02.4	PPB	7/21/2017 14:40	SMPL
I4260-02	MBDX22D	284	0.0629 -		ISM02.4	PPB	7/21/2017 14:42	SMPL
I4260-03	MBDX22S	10629	2.5693 -		ISM02.4	PPB	7/21/2017 14:45	SMPL
I4260-04	MBDX23	77	0.0127 -		ISM02.4	PPB	7/21/2017 14:47	SMPL
I4260-05	MBDX25	426	0.0973 -		ISM02.4	PPB	7/21/2017 14:49	SMPL
I4260-06	MBDX26	304	0.0677 -		ISM02.4	PPB	7/21/2017 14:51	SMPL
I4260-07	MBDX27	163	0.0336 -		ISM02.4	PPB	7/21/2017 14:54	SMPL
I4260-08	MBDX28	232	0.0503 -		ISM02.4	PPB	7/21/2017 14:56	SMPL
I4260-09	MBDX32	258	0.0566 -		ISM02.4	PPB	7/21/2017 14:58	SMPL
I4260-10	MBDX33	198	0.042 -		ISM02.4	PPB	7/21/2017 15:00	SMPL
I4260-12	MBDX21	696	0.1627 -		ISM02.4	PPB	7/21/2017 15:03	SMPL
I4260-13	MBDX24	13961	3.3765 -		ISM02.4	PPB	7/21/2017 15:05	SMPL
I4260-14	MBDX29	1099	0.2603 -		ISM02.4	PPB	7/21/2017 15:07	SMPL
I4260-15	MBDX30	984	0.2325 -		ISM02.4	PPB	7/21/2017 15:10	SMPL
I4260-16	MBDX31	5268	1.2704 -		ISM02.4	PPB	7/21/2017 15:12	SMPL
CCV070	CCV070	20840	5.0432 -		ISM02.4	PPB	7/21/2017 15:14	SMPL
CCB070	CCB070	-134	-0.0384 -		ISM02.4	PPB	7/21/2017 15:16	SMPL