


7470A

LB88928
INSTRUMENT ID: CV1

Linear

 μ Abs.:

3364E

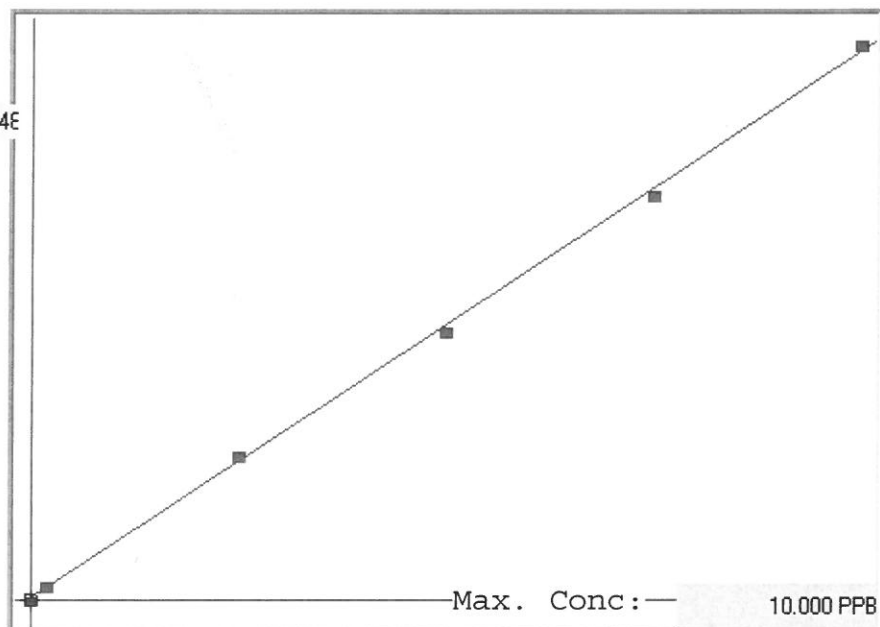

A= 0.0000e+000

B= 3.0154e-004

C= -3.7796e-002

Rho= 0.9996996

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.025	-0.025	44	0.000	44				
0.2	0.200	0.228	0.028	881	0.0 %	881				
2.5	2.500	2.607	0.107	8771	0.0 %	8771				
5.0	5.000	4.906	-0.094	16396	0.0 %	16396				
7.5	7.500	7.375	-0.125	24582	0.0 %	24582				
10.0	10.000	10.109	0.109	33648	0.0 %	33648				

LB88928 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 24 Jul 2017 10:01:18

Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	44	-	0.00007470A	PPB	24 Jul 2017 11:31:28	S	Std
0.2 - 1	50.2	881	-	0.20007470A	PPB	24 Jul 2017 11:33:37	S	Std
2.5 - 1	52.5	8771	-	2.50007470A	PPB	24 Jul 2017 11:35:45	S	Std
5.0 - 1	55	16396	-	5.00007470A	PPB	24 Jul 2017 11:37:53	S	Std
7.5 - 1	57.5	24582	-	7.50007470A	PPB	24 Jul 2017 11:40:00	S	Std
10.0 - 1	510	33648	-	10.00007470A	PPB	24 Jul 2017 11:42:08	S	Std
ICV72 - 1	ICV72	12772	3.8135	-7470A	PPB	24 Jul 2017 11:44:48	U	SMPL
ICB72 - 1	ICB72	36	-0.0269	-7470A	PPB	24 Jul 2017 11:46:54	U	SMPL
CCV78 - 1	CCV78	15536	4.6470	-7470A	PPB	24 Jul 2017 11:49:02	U	SMPL
CCB78 - 1	CCB78	66	-0.0179	-7470A	PPB	24 Jul 2017 11:51:08	U	SMPL
CRA - 1	CRA	887	0.2297	-7470A	PPB	24 Jul 2017 11:53:16	U	SMPL
HighStd - 1	HighStd	34190	10.2720	-7470A	PPB	24 Jul 2017 11:55:22	U	SMPL
ChkStd - 1	ChkStd	23377	7.0114	-7470A	PPB	24 Jul 2017 11:57:29	U	SMPL
PB100853BL - 1	PBW	-75	-0.0604	-7470A	PPB	24 Jul 2017 11:59:38	U	SMPL
PB100853BS - 1	LCSW	12402	3.7020	-7470A	PPB	24 Jul 2017 12:01:48	U	SMPL
PB100853TB - 1	PB100808TB	6	-0.0360	-7470A	PPB	24 Jul 2017 12:03:55	U	SMPL
I4319-02 - 1	B-2(0-6)COMP	87	-0.0116	-7470A	PPB	24 Jul 2017 12:06:03	U	SMPL
I4319-02DUP - 1	B-2(0-6)COMPDUP	93	-0.0098	-7470A	PPB	24 Jul 2017 12:08:12	U	SMPL
I4319-02MS - 1	B-2(0-6)COMPMS	13536	4.0439	-7470A	PPB	24 Jul 2017 12:10:20	U	SMPL
I4319-02MSD - 1	B-2(0-6)COMPMSD	11979	3.5744	-7470A	PPB	24 Jul 2017 12:12:27	U	SMPL
CCV79 - 1	CCV79	15540	4.6482	-7470A	PPB	24 Jul 2017 12:14:34	U	SMPL
CCB79 - 1	CCB79	21	-0.0315	-7470A	PPB	24 Jul 2017 12:16:40	U	SMPL
I4347-03 - 1	B-2(6-10)COMP	211	0.0258	-7470A	PPB	24 Jul 2017 12:18:48	U	SMPL
I4354-04 - 1	265434-265578-COMP	626	0.1510	-7470A	PPB	24 Jul 2017 12:20:54	U	SMPL
I4358-03 - 1	TR-05-072017	103	-0.0067	-7470A	PPB	24 Jul 2017 12:23:01	U	SMPL
I4363-03 - 1	B-COMB-4	89	-0.0110	-7470A	PPB	24 Jul 2017 12:25:08	U	SMPL
PB100854BL - 1	PBW	4	-0.0366	-7470A	PPB	24 Jul 2017 12:27:15	U	SMPL
PB100854BS - 1	LCSW	12132	3.6205	-7470A	PPB	24 Jul 2017 12:29:23	U	SMPL
I4354-03 - 1	265434-265578-COMP	4576	1.3421	-7470A	PPB	24 Jul 2017 12:31:31	U	SMPL
I4362-01 - 1	FRAC-TANK	2134	0.6057	-7470A	PPB	24 Jul 2017 12:33:39	U	SMPL
I4362-01DUP - 1	FRAC-TANKDUP	2174	0.6178	-7470A	PPB	24 Jul 2017 12:35:48	U	SMPL
I4362-01MS - 1	FRAC-TANKMS	14966	4.4751	-7470A	PPB	24 Jul 2017 12:37:55	U	SMPL
CCV80 - 1	CCV80	15516	4.6410	-7470A	PPB	24 Jul 2017 12:40:02	U	SMPL
CCB80 - 1	CCB80	53	-0.0218	-7470A	PPB	24 Jul 2017 12:42:09	U	SMPL
I4362-01MSD - 1	FRAC-TANKMSD	15884	4.7519	-7470A	PPB	24 Jul 2017 12:44:17	U	SMPL
I4369-01 - 1	MW-1-20170720	47	-0.0236	-7470A	PPB	24 Jul 2017 12:46:24	U	SMPL
I4369-02 - 1	MW-2-20170720	171	0.0138	-7470A	PPB	24 Jul 2017 12:48:32	U	SMPL
I4369-03 - 1	MW-3-20170720	149	0.0071	-7470A	PPB	24 Jul 2017 12:50:39	U	SMPL
I4369-04 - 1	MW-4-20170720	147	0.0065	-7470A	PPB	24 Jul 2017 12:52:46	U	SMPL
I4369-05 - 1	MW-5-20170720	153	0.0083	-7470A	PPB	24 Jul 2017 12:54:54	U	SMPL
I4369-06 - 1	MW-6-20170720	159	0.0101	-7470A	PPB	24 Jul 2017 12:57:02	U	SMPL
I4369-07 - 1	DUP-1-20170720	112	-0.0040	-7470A	PPB	24 Jul 2017 12:59:10	U	SMPL
I4369-09 - 1	MW-1-20170720	168	0.0129	-7470A	PPB	24 Jul 2017 13:01:19	U	SMPL
I4369-10 - 1	MW-2-20170720	158	0.0098	-7470A	PPB	24 Jul 2017 13:03:26	U	SMPL
CCV81 - 1	CCV81	16408	4.9099	-7470A	PPB	24 Jul 2017 13:05:33	U	SMPL
CCB81 - 1	CCB81	57	-0.0206	-7470A	PPB	24 Jul 2017 13:07:40	U	SMPL
I4369-11 - 1	MW-3-20170720	172	0.0141	-7470A	PPB	24 Jul 2017 13:09:48	U	SMPL
I4369-12 - 1	MW-4-20170720	78	-0.0143	-7470A	PPB	24 Jul 2017 13:11:56	U	SMPL
I4369-13 - 1	MW-5-20170720	104	-0.0064	-7470A	PPB	24 Jul 2017 13:14:03	U	SMPL
I4369-14 - 1	MW-6-20170720	70	-0.0167	-7470A	PPB	24 Jul 2017 13:16:10	U	SMPL
I4369-15 - 1	DUP-1-20170720	102	-0.0070	-7470A	PPB	24 Jul 2017 13:18:18	U	SMPL
I4395-01 - 1	VL-WWTP-004	671	0.1645	-7470A	PPB	24 Jul 2017 13:20:25	U	SMPL
I4398-02 - 1	RINSEBLANK-SEDIMENT	28	-0.0294	-7470A	PPB	24 Jul 2017 13:22:33	U	SMPL
CCV82 - 1	CCV82	16301	4.8777	-7470A	PPB	24 Jul 2017 13:24:42	U	SMPL
CCB82 - 1	CCB82	49	-0.0230	-7470A	PPB	24 Jul 2017 13:26:50	U	SMPL
I4319-02LX5 - 1		117	-0.0025	-7470A	PPB	24 Jul 2017 13:28:58	U	SMPL
I4319-02A - 1		13363	3.9917	-7470A	PPB	24 Jul 2017 13:31:05	U	SMPL
I4362-01LX5 - 1		460	0.1009	-7470A	PPB	24 Jul 2017 13:33:12	U	SMPL
I4362-01A - 1		15655	4.6829	-7470A	PPB	24 Jul 2017 13:35:19	U	SMPL
CCV83 - 1	CCV83	16213	4.8511	-7470A	PPB	24 Jul 2017 13:37:26	U	SMPL
CCB83 - 1	CCB83	31	-0.0284	-7470A	PPB	24 Jul 2017 13:39:34	U	SMPL