


7470A

LB88985
INSTRUMENT ID: CV1

Linear

 μ Abs.:

32905

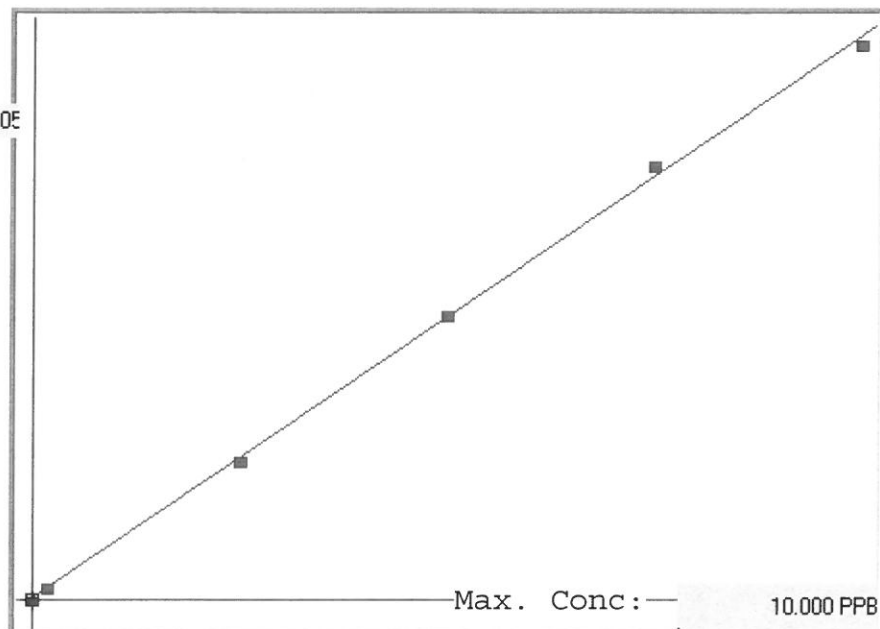

A= 0.0000e+000

B= 2.9987e-004

C= -2.6448e-002

Rho= 0.9995783

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.016	-0.016	34	0.000	34				
0.2	0.200	0.199	-0.001	751	0.0 %	751				
2.5	2.500	2.436	-0.064	8212	0.0 %	8212				
5.0	5.000	5.049	0.049	16924	0.0 %	16924				
7.5	7.500	7.692	0.192	25739	0.0 %	25739				
10.0	10.000	9.841	-0.159	32905	0.0 %	32905				

LB88985 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 25 Jul 2017 13:57:50

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	34	-	0.0000	7470A	PPB	25 Jul 2017 14:00:22	S	Std
0.2 - 1	50.2	751	-	0.2000	7470A	PPB	25 Jul 2017 14:02:30	S	Std
2.5 - 1	52.5	8212	-	2.5000	7470A	PPB	25 Jul 2017 14:04:39	S	Std
5.0 - 1	55	16924	-	5.0000	7470A	PPB	25 Jul 2017 14:06:47	S	Std
7.5 - 1	57.5	25739	-	7.5000	7470A	PPB	25 Jul 2017 14:08:55	S	Std
10.0 - 1	510	32905	-	10.0000	7470A	PPB	25 Jul 2017 14:11:02	S	Std
ICV76 - 1	ICV76	12503	3.7229	-7470A	PPB	PPB	25 Jul 2017 14:13:42	U	SMPL
ICB76 - 1	ICB76	-120	-0.0624	-7470A	PPB	PPB	25 Jul 2017 14:15:48	U	SMPL
CCV93 - 1	CCV93	16870	5.0324	-7470A	PPB	PPB	25 Jul 2017 14:17:56	U	SMPL
CCB93 - 1	CCB93	-119	-0.0621	-7470A	PPB	PPB	25 Jul 2017 14:20:02	U	SMPL
CRA - 1	CRA	710	0.1865	-7470A	PPB	PPB	25 Jul 2017 14:22:10	U	SMPL
HighStd - 1	HighStd	33519	10.0250	-7470A	PPB	PPB	25 Jul 2017 14:24:16	U	SMPL
ChkStd - 1	ChkStd	22361	6.6790	-7470A	PPB	PPB	25 Jul 2017 14:26:23	U	SMPL
PB100917BL - 1	PBW	-16	-0.0312	-7470A	PPB	PPB	25 Jul 2017 14:31:24	U	SMPL
PB100917BS - 1	LCSW	12602	3.7525	-7470A	PPB	PPB	25 Jul 2017 14:33:31	U	SMPL
I4302-01 - 1	RINSEBLANK-SOIL	-90	-0.0534	-7470A	PPB	PPB	25 Jul 2017 14:35:39	U	SMPL
I4402-07 - 1	FRAC-TANK-260783	-5	-0.0279	-7470A	PPB	PPB	25 Jul 2017 14:37:47	U	SMPL
I4402-07DUP - 1	FRAC-TANK-260783DUP	-8	-0.0288	-7470A	PPB	PPB	25 Jul 2017 14:39:56	U	SMPL
I4402-07MS - 1	FRAC-TANK-260783MS	13533	4.0317	-7470A	PPB	PPB	25 Jul 2017 14:42:04	U	SMPL
I4402-07MSD - 1	FRAC-TANK-260783MSD	12884	3.8371	-7470A	PPB	PPB	25 Jul 2017 14:44:11	U	SMPL
CCV94 - 1	CCV94	16849	5.0261	-7470A	PPB	PPB	25 Jul 2017 14:49:33	U	SMPL
CCB94 - 1	CCB94	-124	-0.0636	-7470A	PPB	PPB	25 Jul 2017 14:51:40	U	SMPL
I4402-07LX5 - 1		14	-0.0223	-7470A	PPB	PPB	25 Jul 2017 14:53:47	U	SMPL
I4402-07A - 1		13594	4.0500	-7470A	PPB	PPB	25 Jul 2017 14:55:54	U	SMPL
CCV95 - 1	CCV95	16351	4.8768	-7470A	PPB	PPB	25 Jul 2017 14:58:01	U	SMPL
CCB95 - 1	CCB95	-108	-0.0588	-7470A	PPB	PPB	25 Jul 2017 15:00:08	U	SMPL