


ISM02.4

LB 89037
INSTRUMENT ID: C14

Linear

 μ Abs.:

41135

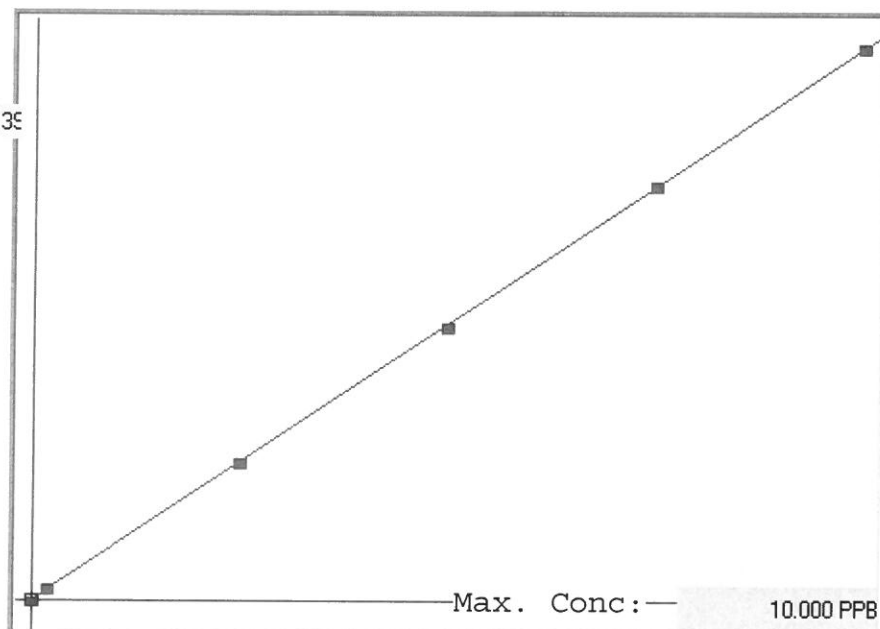

A= 0.0000e+000

B= 2.4355e-004

C= -1.0060e-002

Rho= 0.9999801

Accept=Accepted

slope
x-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.002	0.002	48	0.000	48					-
0.2	0.200	0.205	0.005	883	0.0 %	883					2
2.5	2.500	2.521	0.021	10391	0.0 %	10391					4
5.0	5.000	4.950	-0.050	20365	0.0 %	20365					-1
7.5	7.500	7.514	0.014	30892	0.0 %	30892					0
10.0	10.000	10.009	0.009	41139	0.0 %	41139					0

LB
7/26/12

LB89037

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	48	-		0 ISM02.4	PPB	7/26/2017 18:29	Std
	0.2 S0.2	883	-		0.2 ISM02.4	PPB	7/26/2017 18:31	Std
	2.5 S2.5	10391	-		2.5 ISM02.4	PPB	7/26/2017 18:33	Std
	5 S5	20365	-		5 ISM02.4	PPB	7/26/2017 18:35	Std
	7.5 S7.5	30892	-		7.5 ISM02.4	PPB	7/26/2017 18:38	Std
	10 S10	41139	-		10 ISM02.4	PPB	7/26/2017 18:40	Std
ICV	ICV	15639	3.7988 -		ISM02.4	PPB	7/26/2017 18:43	SMPL
ICB	ICB	-120	-0.0393 -		ISM02.4	PPB	7/26/2017 18:45	SMPL
CCV020	CCV020	20233	4.9177 -		ISM02.4	PPB	7/26/2017 18:47	SMPL
CCB020	CCB020	-123	-0.04 -		ISM02.4	PPB	7/26/2017 18:50	SMPL
PB100988BL	PBW003	-14	-0.0135 -		ISM02.4	PPB	7/26/2017 18:52	SMPL
I4260-11	MBDX34	18	-0.0057 -		ISM02.4	PPB	7/26/2017 18:54	SMPL
CCV021	CCV021	19945	4.8475 -		ISM02.4	PPB	7/26/2017 18:56	SMPL
CCB021	CCB021	-97	-0.0337 -		ISM02.4	PPB	7/26/2017 18:59	SMPL