

7470A


LB89139

INSTRUMENT ID: CV1

Linear

 μ Abs.:

33827

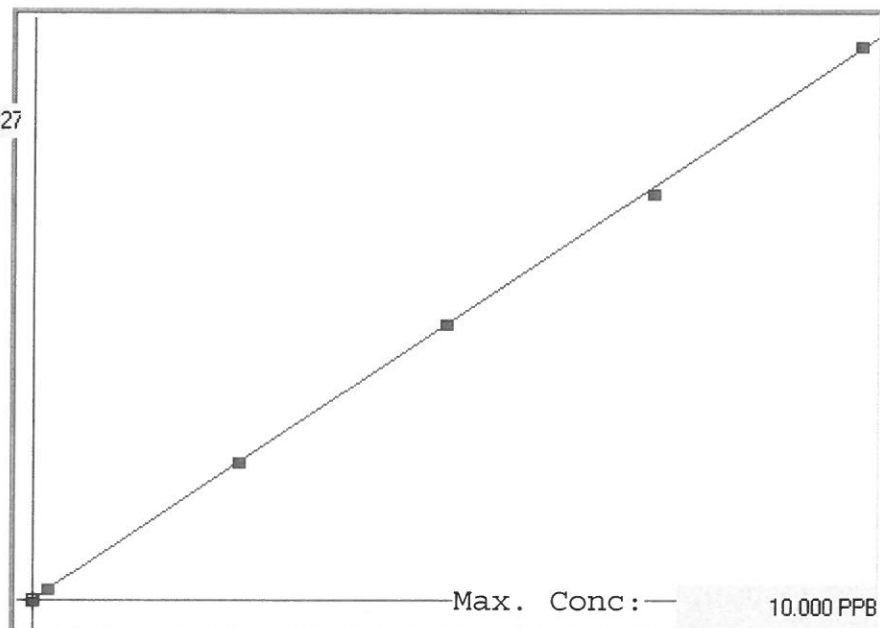

A= 0.0000e+000

B= 2.9767e-004

C= -1.4605e-003

Rho= 0.9998952

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	21	0.000	21				
0.2	0.200	0.208	0.008	703	0.0 %	703				
2.5	2.500	2.509	0.009	8433	0.0 %	8433				
5.0	5.000	5.020	0.020	16869	0.0 %	16869				
7.5	7.500	7.391	-0.109	24833	0.0 %	24833				
10.0	10.000	10.068	0.068	33827	0.0 %	33827				

LB89139 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Jul 2017 11:20:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	21	-	0.00007470A	PPB		31 Jul 2017 11:31:55	S	Std
0.2 - 1	50.2	703	-	0.20007470A	PPB		31 Jul 2017 11:34:04	S	Std
2.5 - 1	52.5	8433	-	2.50007470A	PPB		31 Jul 2017 11:36:12	S	Std
5.0 - 1	55	16869	-	5.00007470A	PPB		31 Jul 2017 11:38:20	S	Std
7.5 - 1	57.5	24833	-	7.50007470A	PPB		31 Jul 2017 11:40:28	S	Std
10.0 - 1	510	33827	-	10.00007470A	PPB		31 Jul 2017 11:46:41	S	Std
ICV85 - 1	ICV85	13293	3.9555	-7470A	PPB		31 Jul 2017 11:49:15	U	SMPL
ICB85 - 1	ICB85	-120	-0.0372	-7470A	PPB		31 Jul 2017 11:51:21	U	SMPL
CCV42 - 1	CCV42	16897	5.0283	-7470A	PPB		31 Jul 2017 11:53:28	U	SMPL
CCB42 - 1	CCB42	-110	-0.0342	-7470A	PPB		31 Jul 2017 11:55:34	U	SMPL
CRA - 1	CRA	656	0.1938	-7470A	PPB		31 Jul 2017 11:57:41	U	SMPL
HighStd - 1	HighStd	33867	10.0798	-7470A	PPB		31 Jul 2017 11:59:47	U	SMPL
ChkStd - 1	ChkStd	23878	7.1064	-7470A	PPB		31 Jul 2017 12:01:54	U	SMPL
PB101066BL - 1	PBW	-150	-0.0461	-7470A	PPB		31 Jul 2017 12:04:03	U	SMPL
PB101066BS - 1	LCSW	13139	3.9097	-7470A	PPB		31 Jul 2017 12:06:11	U	SMPL
PB101066TB - 1	PB101024TB	-63	-0.0202	-7470A	PPB		31 Jul 2017 12:08:19	U	SMPL
I4436-02 - 1	FLOOR-SWEEPINGS	27	0.0066	-7470A	PPB		31 Jul 2017 12:10:27	U	SMPL
I4475-01 - 1	A0C1	25	0.0060	-7470A	PPB		31 Jul 2017 12:12:35	U	SMPL
I4475-02 - 1	A0C2	23	0.0054	-7470A	PPB		31 Jul 2017 12:14:44	U	SMPL
I4475-03 - 1	A0C3	59	0.0161	-7470A	PPB		31 Jul 2017 12:16:50	U	SMPL
CCV43 - 1	CCV43	17120	5.0947	-7470A	PPB		31 Jul 2017 12:18:57	U	SMPL
CCB43 - 1	CCB43	-95	-0.0297	-7470A	PPB		31 Jul 2017 12:21:04	U	SMPL
I4475-04 - 1	A0C4	43	0.0113	-7470A	PPB		31 Jul 2017 12:23:11	U	SMPL
I4476-04 - 1	TP-8-LENOX-AVE	10	0.0015	-7470A	PPB		31 Jul 2017 12:25:18	U	SMPL
I4476-08 - 1	TP-7-LENOX-AVE	18	0.0039	-7470A	PPB		31 Jul 2017 12:27:24	U	SMPL
I4488-03 - 1	CL-02-072717-A	26	0.0063	-7470A	PPB		31 Jul 2017 12:29:31	U	SMPL
I4488-06 - 1	CL-02-072717-B	32	0.0081	-7470A	PPB		31 Jul 2017 12:31:39	U	SMPL
I4488-09 - 1	CL-02-072717-C	19	0.0042	-7470A	PPB		31 Jul 2017 12:33:46	U	SMPL
I4488-12 - 1	CL-02-072717-D	35	0.0090	-7470A	PPB		31 Jul 2017 12:35:54	U	SMPL
I4488-15 - 1	CL-02-072717-E	30	0.0075	-7470A	PPB		31 Jul 2017 12:38:03	U	SMPL
I4488-15DUP - 1	CL-02-072717-EDUP	26	0.0063	-7470A	PPB		31 Jul 2017 12:40:12	U	SMPL
I4488-15MS - 1	CL-02-072717-EMS	12958	3.8558	-7470A	PPB		31 Jul 2017 12:42:19	U	SMPL
CCV44 - 1	CCV44	16893	5.0271	-7470A	PPB		31 Jul 2017 12:44:25	U	SMPL
CCB44 - 1	CCB44	-98	-0.0306	-7470A	PPB		31 Jul 2017 12:46:32	U	SMPL
I4488-15MSD - 1	CL-02-072717-EMSD	13096	3.8969	-7470A	PPB		31 Jul 2017 12:48:39	U	SMPL
I4488-15LX5 - 1		-62	-0.0199	-7470A	PPB		31 Jul 2017 12:50:46	U	SMPL
I4488-15A - 1		14036	4.1767	-7470A	PPB		31 Jul 2017 12:52:53	U	SMPL
CCV45 - 1	CCV45	16913	5.0331	-7470A	PPB		31 Jul 2017 12:55:00	U	SMPL
CCB45 - 1	CCB45	-72	-0.0229	-7470A	PPB		31 Jul 2017 12:57:07	U	SMPL