


7471A

LB 89148
INSTRUMENT ID: CV 2

Linear

 μ Abs.:

40176

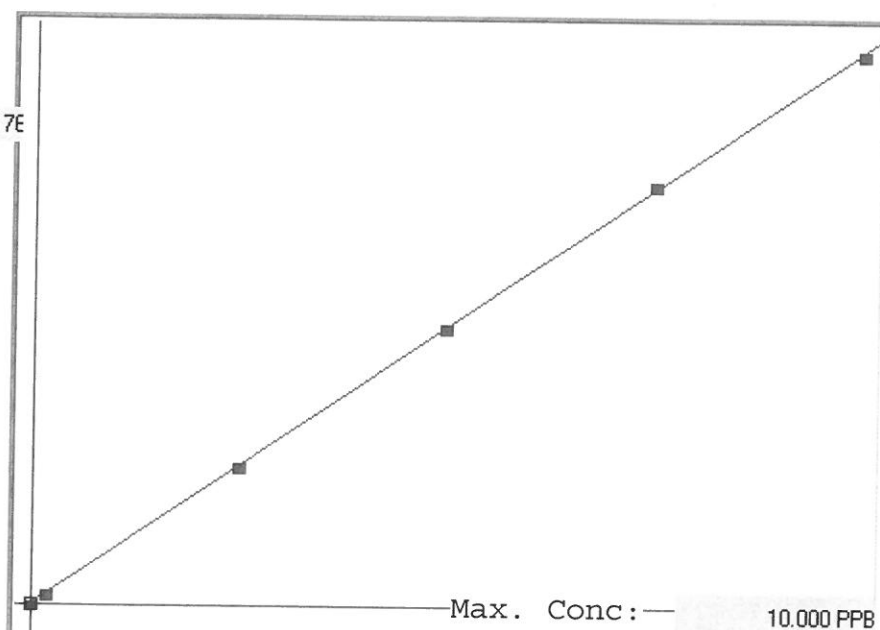

A= 0.0000e+000

B= 2.4780e-004

C= -1.3314e-002

Rho= 0.9999313

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.005	-0.005	34	0.000	34				
0.2	0.200	0.193	-0.007	832	0.0 %	832				
2.5	2.500	2.499	-0.001	10139	0.0 %	10139				
5.0	5.000	4.984	-0.016	20167	0.0 %	20167				
7.5	7.500	7.587	0.087	30671	0.0 %	30671	0			
10.0	10.000	9.942	-0.058	40176	0.0 %	40176				

LB89148 INSTRUMENT ID : CV1

Method: 7471A		Operator: Admin		Date of Analysis: 31 Jul 2017 14:18:53					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	34	-	0.0000	7471A	PPB	31 Jul 2017 14:22:47	S	Std
0.2 - 1	50.2	832	-	0.2000	7471A	PPB	31 Jul 2017 14:25:05	S	Std
2.5 - 1	52.5	10139	-	2.5000	7471A	PPB	31 Jul 2017 14:27:23	S	Std
5.0 - 1	55	20167	-	5.0000	7471A	PPB	31 Jul 2017 14:29:40	S	Std
7.5 - 1	57.5	30671	-	7.5000	7471A	PPB	31 Jul 2017 14:31:57	S	Std
10.0 - 1	510	40176	-	10.0000	7471A	PPB	31 Jul 2017 14:34:14	S	Std
ICV86 - 1	ICV86	15924	3.9326	-	7471A	PPB	31 Jul 2017 14:37:03	U	SMPL
ICB86 - 1	ICB86	-88	-0.0351	-	7471A	PPB	31 Jul 2017 14:39:18	U	SMPL
CCV46 - 1	CCV46	19776	4.8871	-	7471A	PPB	31 Jul 2017 14:41:34	U	SMPL
CCB46 - 1	CCB46	-73	-0.0314	-	7471A	PPB	31 Jul 2017 14:43:50	U	SMPL
CRA - 1	CRA	805	0.1862	-	7471A	PPB	31 Jul 2017 14:46:06	U	SMPL
HighStd - 1	HighStd	40159	9.9379	-	7471A	PPB	31 Jul 2017 14:48:22	U	SMPL
ChkStd - 1	ChkStd	27865	6.8915	-	7471A	PPB	31 Jul 2017 14:50:38	U	SMPL
PB101067BL - 1	PBS	-171	-0.0557	-	7471A	PPB	31 Jul 2017 14:52:56	U	SMPL
PB101067BS - 1	LCSS	15288	3.7750	-	7471A	PPB	31 Jul 2017 14:55:13	U	SMPL
I4511-02 - 1	TEC-PLATT-COMP	78	0.0060	-	7471A	PPB	31 Jul 2017 14:57:30	U	SMPL
I4512-01 - 1	HDD-PILWC4	65	0.0028	-	7471A	PPB	31 Jul 2017 14:59:47	U	SMPL
I4522-01 - 1	TP-2-SS1	12177	3.0041	-	7471A	PPB	31 Jul 2017 15:02:05	U	SMPL
I4522-02 - 1	TP-3D68	4075	0.9965	-	7471A	PPB	31 Jul 2017 15:04:22	U	SMPL
I4522-03 - 1	TP-5-SS2	20168	4.9842	-	7471A	PPB	31 Jul 2017 15:06:38	U	SMPL
CCV47 - 1	CCV47	19837	4.9022	-	7471A	PPB	31 Jul 2017 15:08:54	U	SMPL
CCB47 - 1	CCB47	-79	-0.0329	-	7471A	PPB	31 Jul 2017 15:11:10	U	SMPL
I4524-01 - 1	SU-04-072817	47221	11.6879	-	7471A	PPB	31 Jul 2017 15:13:26	U	SMPL
I4524-01DUP - 1	SU-04-072817DUP	43555	10.7794	-	7471A	PPB	31 Jul 2017 15:15:42	U	SMPL
I4524-01MS - 1	SU-04-072817MS	55191	13.6628	-	7471A	PPB	31 Jul 2017 15:17:59	U	SMPL
I4524-01MSD - 1	SU-04-072817MSD	56805	14.0627	-	7471A	PPB	31 Jul 2017 15:20:17	U	SMPL
I4527-01 - 1	E2-HS7-BASE	1315	0.3125	-	7471A	PPB	31 Jul 2017 15:22:36	U	SMPL
I4527-02 - 1	E2-HS7-NSW	20733	5.1242	-	7471A	PPB	31 Jul 2017 15:24:55	U	SMPL
I4527-03 - 1	E2-HS7-ESW	18103	4.4725	-	7471A	PPB	31 Jul 2017 15:27:12	U	SMPL
I4527-04 - 1	E2-HS7-SSW	36183	8.9527	-	7471A	PPB	31 Jul 2017 15:29:30	U	SMPL
I4527-05 - 1	E2-HS7-WSW	17803	4.3982	-	7471A	PPB	31 Jul 2017 15:31:47	U	SMPL
I4527-06 - 1	E2-N8-BASE	391092	HIGH	-	7471A	PPB	31 Jul 2017 15:34:05	X	
CCV48 - 1	CCV48	19171	4.7372	-	7471A	PPB	31 Jul 2017 15:35:56	U	SMPL
CCB48 - 1	CCB48	-74	-0.0317	-	7471A	PPB	31 Jul 2017 15:41:04	U	SMPL
I4527-07 - 1	E2-N8-NSW	221104	54.7753	-	7471A	PPB	31 Jul 2017 15:43:20	U	SMPL
I4527-09 - 1	E2-O8-BASE	235839	58.4266	-	7471A	PPB	31 Jul 2017 15:45:36	U	SMPL
I4527-10 - 1	E2-N8-WSW	-118	-0.0426	-	7471A	PPB	31 Jul 2017 15:50:56	U	SMPL
I4524-01LX5 - 1		8549	2.1051	-	7471A	PPB	31 Jul 2017 15:53:12	U	SMPL
I4524-01A - 1		61479	15.2209	-	7471A	PPB	31 Jul 2017 15:55:29	U	SMPL
I4527-06DLX10 - 1		56025	13.8694	-	7471A	PPB	31 Jul 2017 15:57:45	U	SMPL
I4527-07DLX10 - 1		22350	5.5249	-	7471A	PPB	31 Jul 2017 16:00:05	U	SMPL
I4527-09DLX10 - 1		23355	5.7740	-	7471A	PPB	31 Jul 2017 16:02:24	U	SMPL
CCV49 - 1	CCV49	19898	4.9173	-	7471A	PPB	31 Jul 2017 16:04:43	U	SMPL
CCB49 - 1	CCB49	-89	-0.0354	-	7471A	PPB	31 Jul 2017 16:06:59	U	SMPL
I4524-01DLX2 - 1		23616	5.8386	-	7471A	PPB	31 Jul 2017 16:09:16	U	SMPL
I4524-01DUPDLX2 - 1		21917	5.4176	-	7471A	PPB	31 Jul 2017 16:11:33	U	SMPL
I4524-01MSDLX2 - 1		27477	6.7954	-	7471A	PPB	31 Jul 2017 16:13:50	U	SMPL
I4524-01MSDDLX2 - 1		28462	7.0395	-	7471A	PPB	31 Jul 2017 16:16:08	U	SMPL
I4524-01LDLX10 - 1		4573	1.1199	-	7471A	PPB	31 Jul 2017 16:18:25	U	SMPL
I4524-01ADLX2 - 1		30620	7.5742	-	7471A	PPB	31 Jul 2017 16:23:20	U	SMPL
I4527-06DL2X50 - 1		10904	2.6887	-	7471A	PPB	31 Jul 2017 16:25:36	U	SMPL
CCV50 - 1	CCV50	19323	4.7748	-	7471A	PPB	31 Jul 2017 16:27:54	U	SMPL
CCB50 - 1	CCB50	-88	-0.0351	-	7471A	PPB	31 Jul 2017 16:30:11	U	SMPL