

Clear table

LC-2
300.0
8/1/19 AT


ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-06-08	6/8/17 10:57
STD2	0.1300	0.2280	0.2430	0.6830	0.1990	0.1330	1.2860	2017-06-08	6/8/17 11:28
STD3	0.4180	0.6310	0.6350	2.0810	0.5240	1.0660	3.2030	2017-06-08	6/8/17 11:59
STD4	0.8040	1.1660	1.1560	3.8980	0.9740	2.0580	5.8490	2017-06-08	6/8/17 12:30
STD5	1.9330	2.8390	2.8230	9.5130	2.3720	4.7630	14.1600	2017-06-08	6/8/17 13:01
STD6	3.8830	5.8840	5.9620	19.6130	4.9110	10.0520	29.5180	2017-06-08	6/8/17 13:32
STD7	5.0950	7.6330	7.6040	25.4210	6.3610	12.7380	38.2680	2017-06-08	6/8/17 14:03
ICV	2.0250	2.9610	2.9530	9.8990	2.4660	5.1220	14.6460	2017-06-08	6/8/17 15:47
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-06-08	6/8/17 17:26
CCV	2.0230	3.0850	2.9590	9.9520	2.4790	5.0210	14.4890	2017-07-07	7/7/17 16:48
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-07	7/7/17 17:19
LB89167BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-07	7/7/17 17:50
LB89167BSW	2.0260	3.0360	2.9600	9.9540	2.4750	5.0380	14.4680	2017-07-07	7/7/17 18:21
I4047-01	0.0900	0.1610	0.2040	0.6040	0.1600	0.0590	1.0650	2017-07-07	7/7/17 18:52
I4047-02	0.0950	0.1590	0.2030	0.6090	0.1620	0.1020	1.0670	2017-07-07	7/7/17 19:23
I4047-03	0.0930	0.1620	0.2050	0.6110	0.1610	0.0940	1.0590	2017-07-07	7/7/17 19:54
I4047-04	0.0940	0.1600	0.2040	0.6050	0.1620	0.0990	1.0660	2017-07-07	7/7/17 20:25
I4047-05	0.0940	0.1600	0.2030	0.6110	0.1620	0.0950	1.0670	2017-07-07	7/7/17 20:56
I4047-06	0.0920	0.1600	0.2050	0.6080	0.1620	0.0930	1.0660	2017-07-07	7/7/17 21:27
I4047-07	0.0940	0.1620	0.2040	0.6080	0.1610	0.0960	1.0690	2017-07-07	7/7/17 21:58
I4047-07	0.0950	0.1600	0.2030	0.6110	0.1620	0.0950	1.0670	2017-07-07	7/7/17 22:29
CCV	1.9440	2.9230	2.8970	9.7550	2.4200	4.7710	14.1450	2017-07-07	7/7/17 23:00
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-07-07	7/7/17 23:31

IC 2 Cat.

6-8-17

CALIBRATION OF COMPONENT F-

Method: AnionIC2-060817.mtw
 Equation: $Q = 0.0174627 \cdot A + 1.01419$
 RSD: 3.795 %
 Correlation coefficient: 0.999412

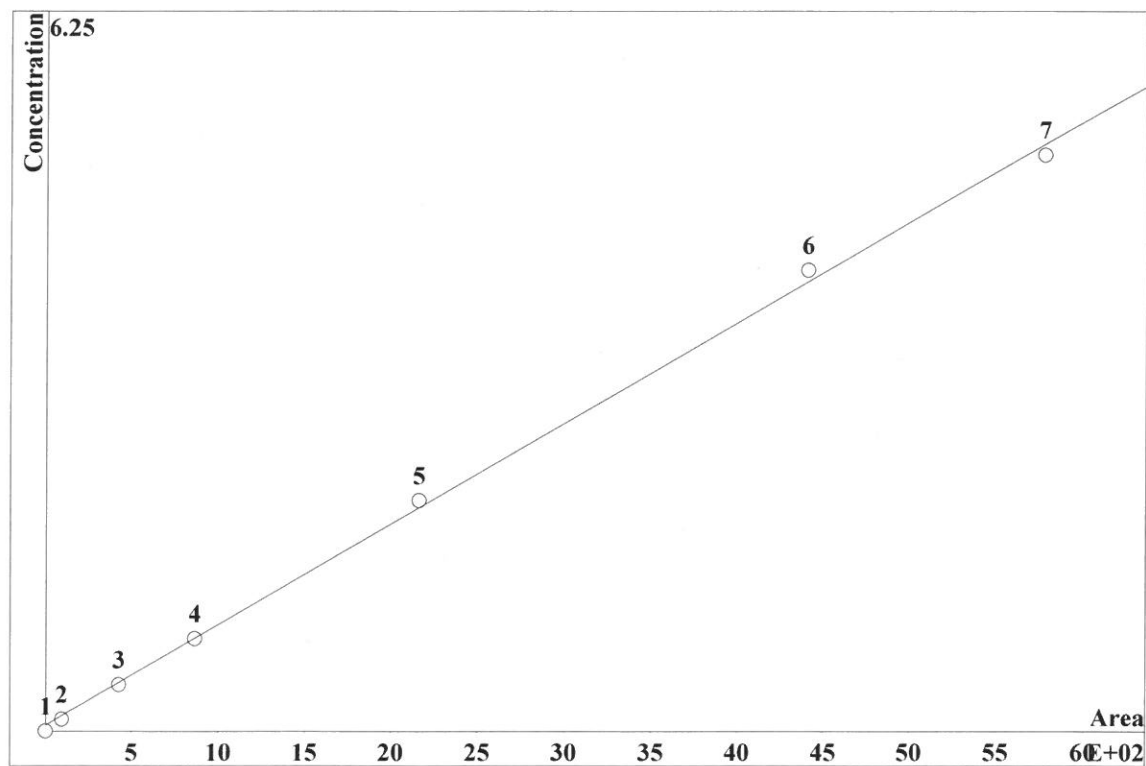


K3 = 0 K2 = 0 K1 = 0.0174627 K0 = 1.01419
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.097	96.77	0.1	20	5.175		
3	16.82	425.8	0.4	20	5.175		
4	35.31	865.9	0.8	20	5.175		
5	86.96	2163	2	20	5.175		
6	176.6	4410	4	20	5.175		
7	242.2	5777	5	20	5.175		

CALIBRATION OF COMPONENT CL-

Method: AnionIC2-060817.mtw
 Equation: $Q = 0.0259527 \cdot A + 1.8564$
 RSD: 4.057 %
 Correlation coefficient: 0.999328

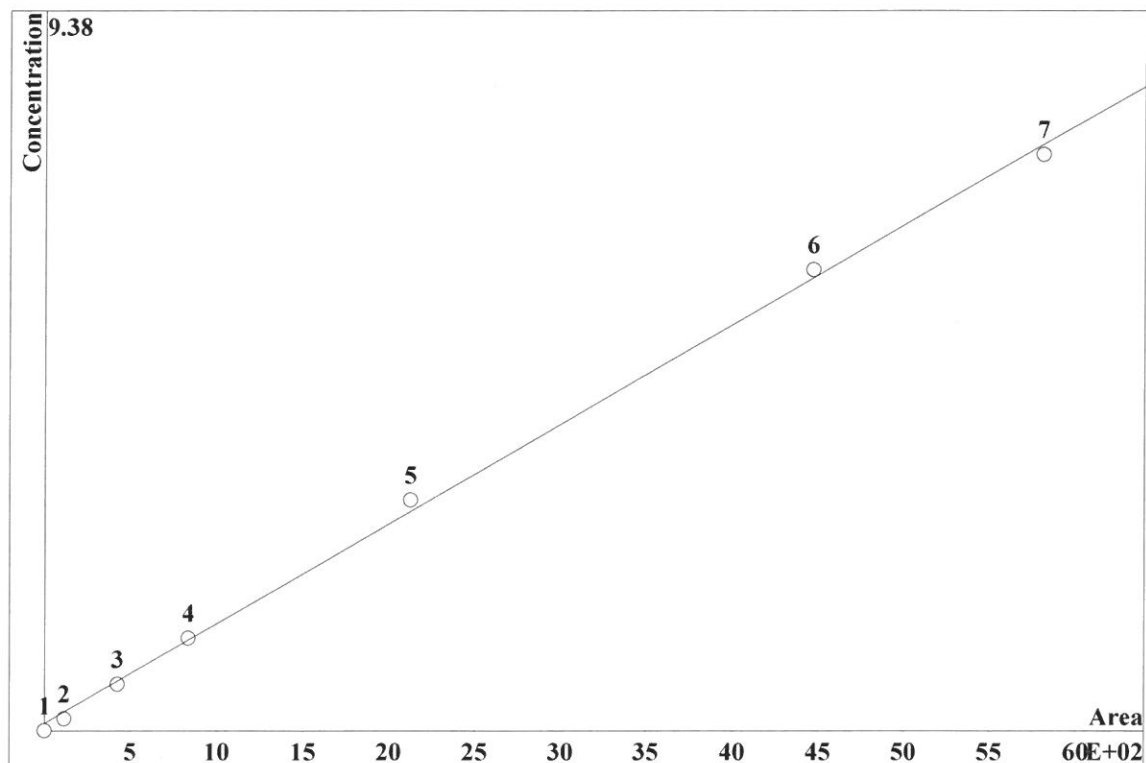

K3 = 0 K2 = 0 K1 = 0.0259527 K0 = 1.8564

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.818	118	0.15	20	9.032		
3	27.41	426	0.6	20	9.032		
4	55.39	836.6	1.2	20	9.032		
5	145.2	2127	3	20	9.032		
6	310.2	4471	6	20	9.032		
7	405.9	5811	7.5	20	9.032		

CALIBRATION OF COMPONENT NO2

Method: AnionIC2-060817.mtw
 Equation: $Q = 0.0109583 \cdot A + 2.83736$
 RSD: 4.065 %
 Correlation coefficient: 0.999325

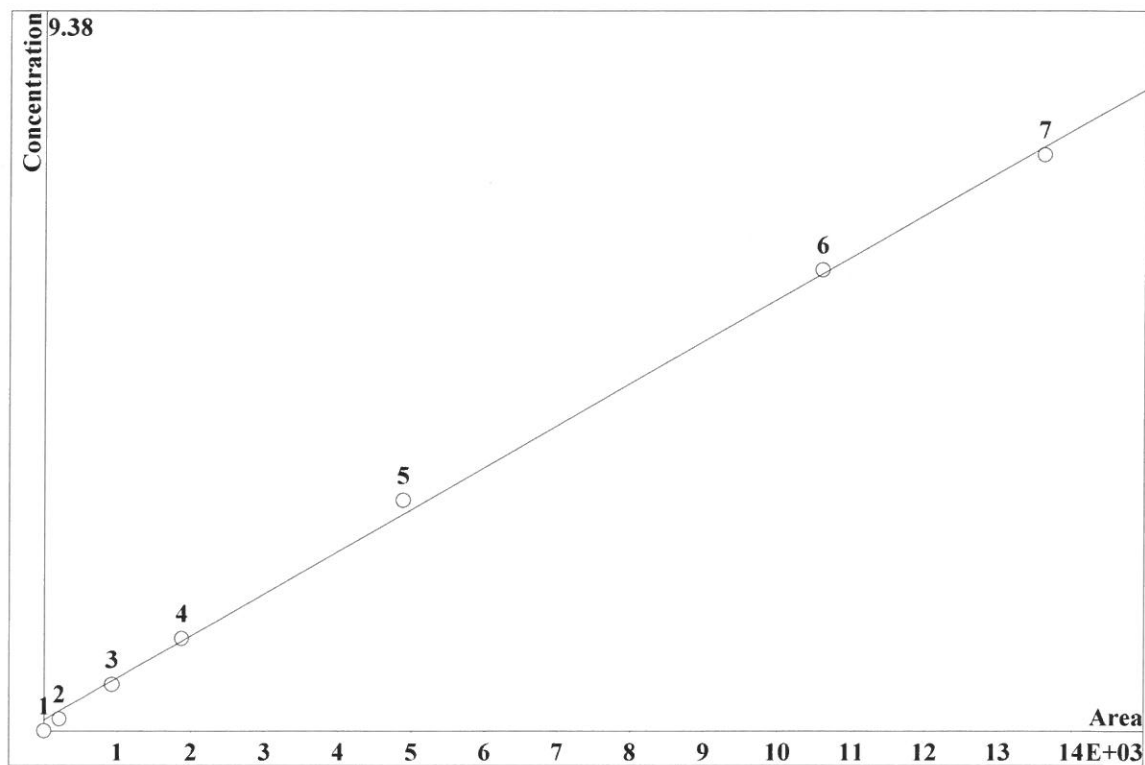

K3 = 0 K2 = 0 K1 = 0.0109583 K0 = 2.83736

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.54	217.3	0.15	20	11.72		
3	53.22	928	0.6	20	11.72		
4	106.9	1872	1.2	20	11.72		
5	283.9	4884	3	20	11.72		
6	616.3	1.06e+04	6	20	11.72		
7	779.7	1.362e+04	7.5	20	11.72		

CALIBRATION OF COMPONENT BR-

Method: AnionIC2-060817.mtw
 Equation: $Q = 0.0578527 \cdot A + 7.66262$
 RSD: 3.793 %
 Correlation coefficient: 0.999413

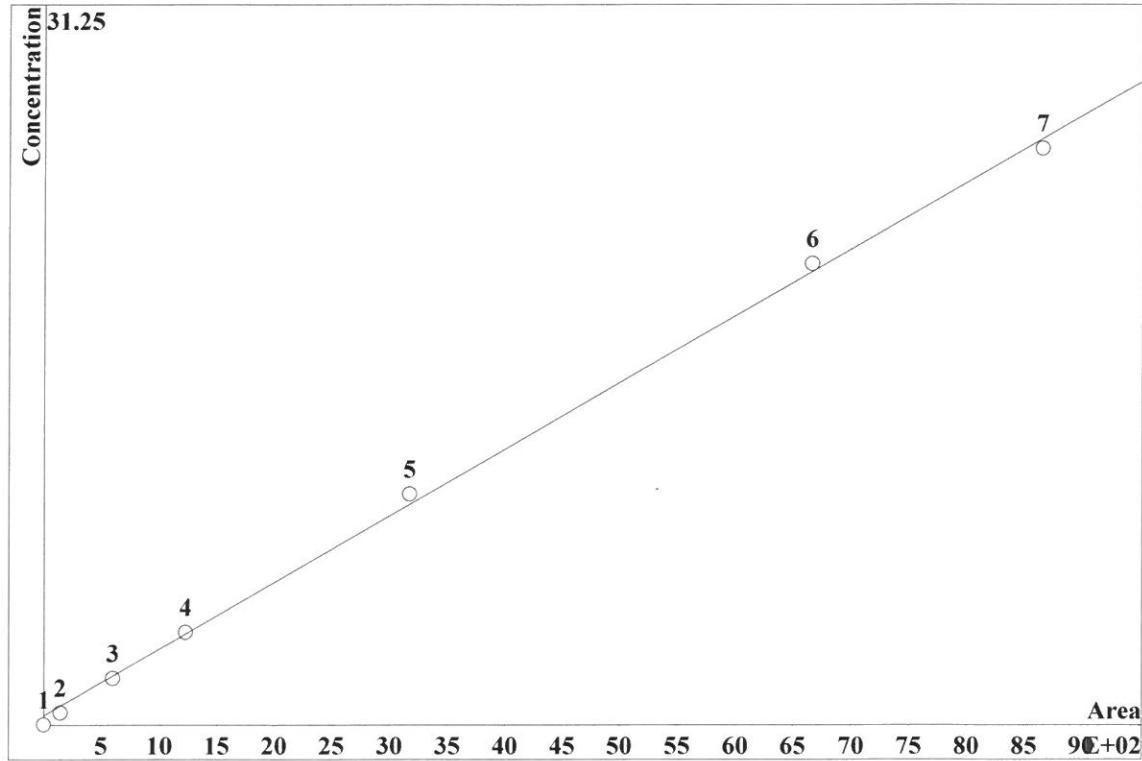

K3 = 0 K2 = 0 K1 = 0.0578527 K0 = 7.66262

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.632	147.3	0.5	20	15.11		
3	27.36	600.7	2	20	15.11		
4	55.9	1227	4	20	15.11		
5	145.6	3172	10	20	15.11		
6	307.5	6663	20	20	15.11		
7	400.6	8656	25	20	15.11		

CALIBRATION OF COMPONENT NO3

Method: AnionIC2-060817.mtw
 Equation: $Q = 0.0102392 \cdot A + 2.16037$
 RSD: 4.092 %
 Correlation coefficient: 0.999316

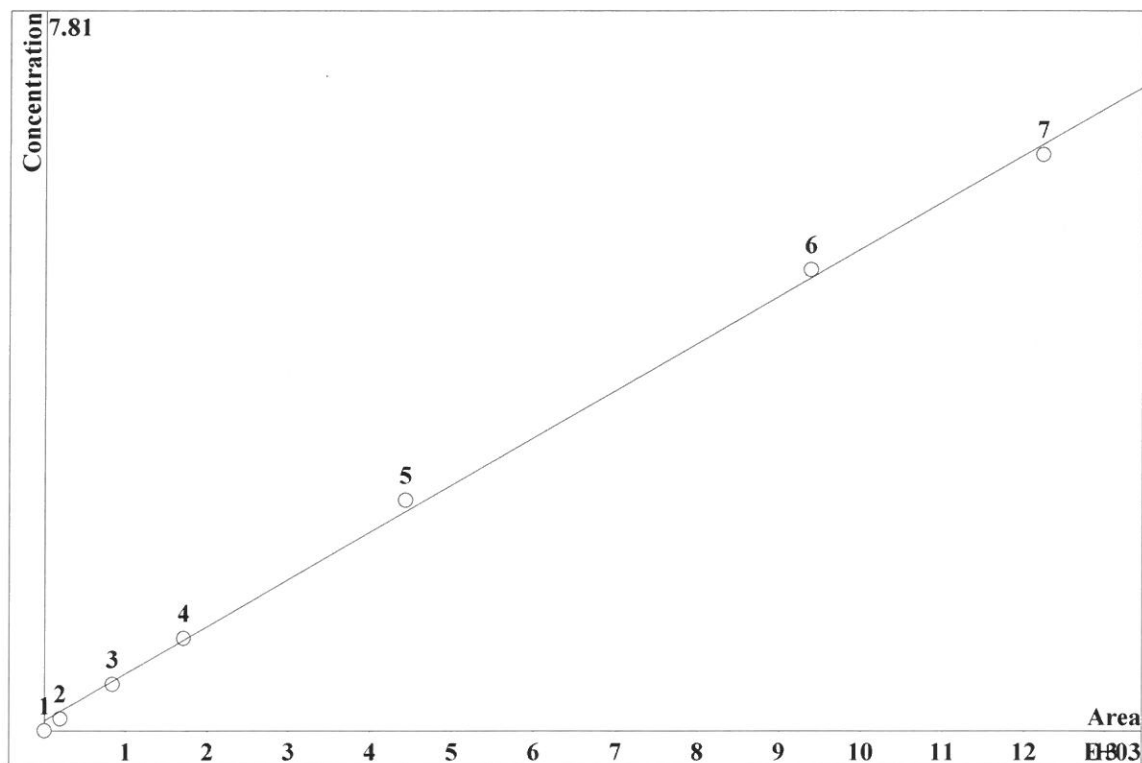

K3 = 0 K2 = 0 K1 = 0.0102392 K0 = 2.16037

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.867	198.1	0.125	20	17.96		
3	33.01	832.6	0.5	20	17.96		
4	67.19	1706	1	20	17.96		
5	172.9	4432	2.5	20	17.96		
6	358.7	9383	5	20	17.96		
7	462.1	1.221e+04	6.25	20	17.96		

CALIBRATION OF COMPONENT HPO4

Method: AnionIC2-060817.mtw
 Equation: $Q = 0.0277933 \cdot A - 4.40358$
 RSD: 4.810 %
 Correlation coefficient: 0.999055

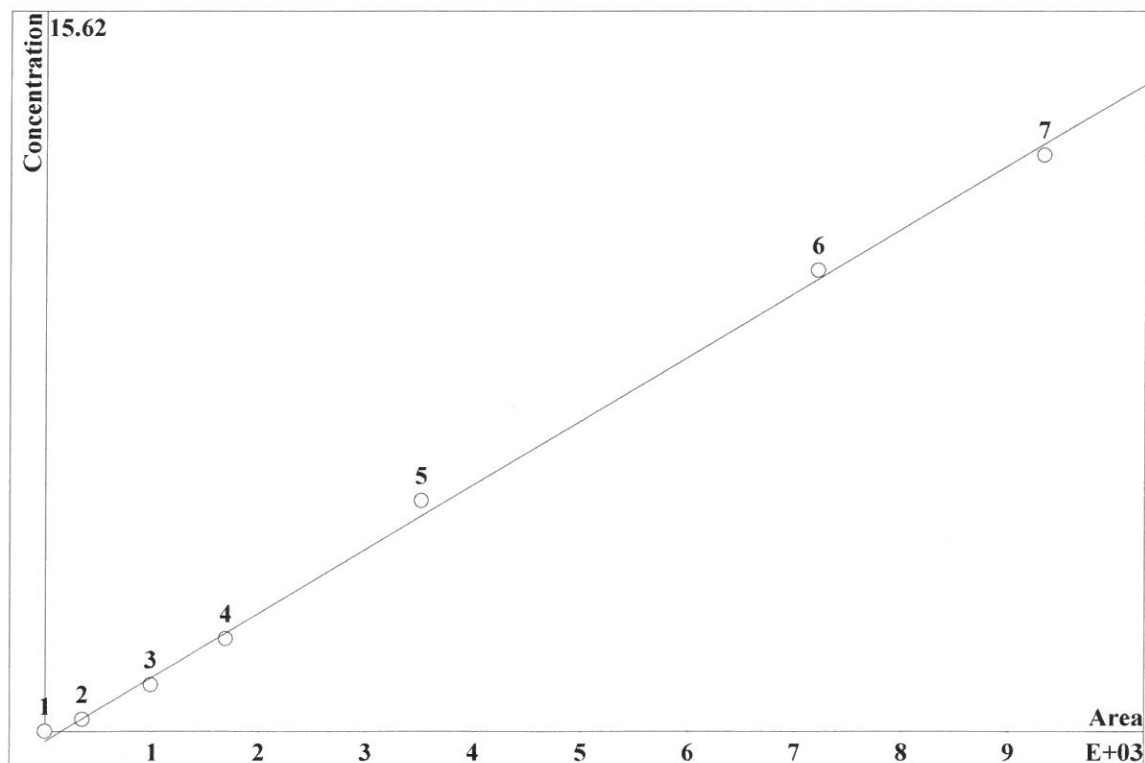


K3 = 0 K2 = 0 K1 = 0.0277933 K0 = -4.40358
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.297	349.8	0.25	20	23.35		
3	24.34	986	1	20	23.35		
4	44.04	1687	2	20	23.35		
5	93.31	3518	5	20	23.35		
6	203	7213	10	20	23.35		
7	266.9	9325	12.5	20	23.35		

CALIBRATION OF COMPONENT SO4

Method: AnionIC2-060817.mtw
 Equation: $Q = 0.0330868 \cdot A + 14.6116$
 RSD: 4.796 %
 Correlation coefficient: 0.999061

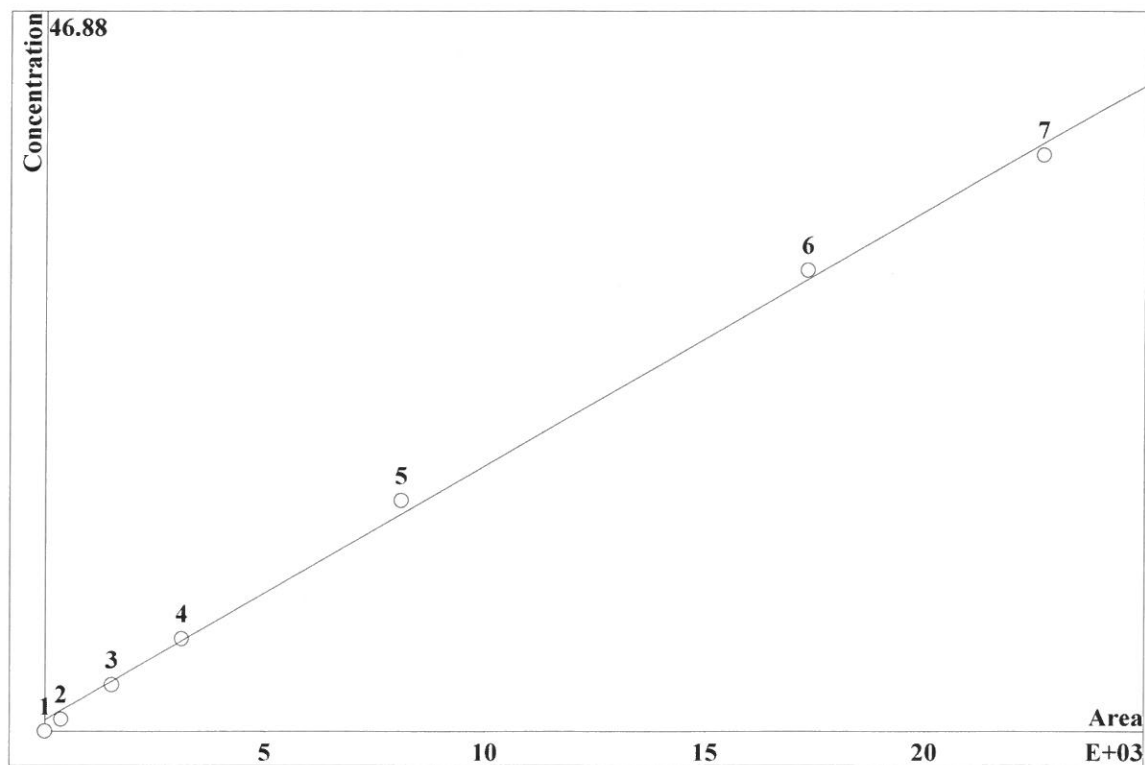

K3 = 0 K2 = 0 K1 = 0.0330868 K0 = 14.6116
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	10.99	373.8	0.75	20	25.16		
3	44.37	1523	3	20	25.16		
4	90.91	3108	6	20	25.16		
5	239.5	8090	15	20	25.16		
6	516.9	1.733e+04	30	20	25.16		
7	677.5	2.269e+04	37.5	20	25.16		

Report date: 7/6/2017 12:43:18 PM
Printed by: wet


Ident: STD1
Analysis from: 6/8/2017 10:57:23 AM
File: _2017-06-08_

Last save: 6/8/2017 11:25:23 AM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14599

Last save: 6/8/2017 9:52:06

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

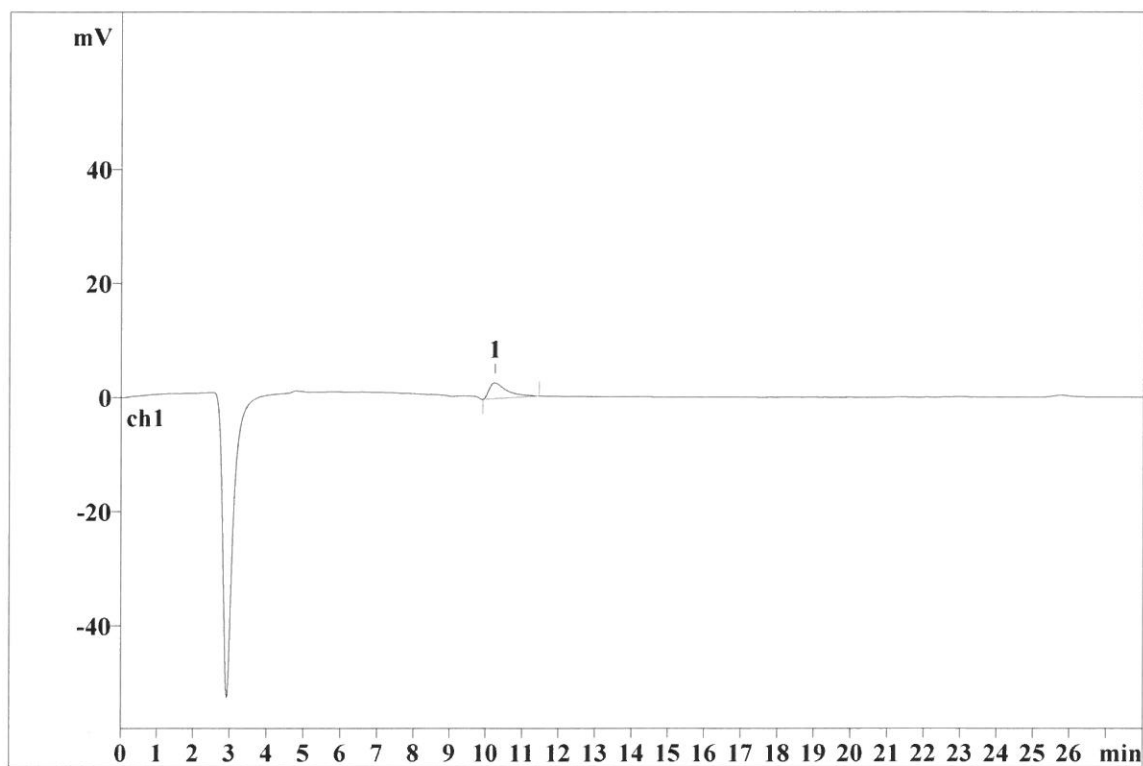

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.000	0.00	0.00	0.000	0.00

Report date: 7/6/2017 12:43:23 PM
Printed by: wet


Ident: STD2
Analysis from: 6/8/2017 11:28:21 AM
File: _2017-06-08_

Last save: 6/8/2017 11:56:22 AM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14600

Last save: 6/8/2017 11:25:2

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

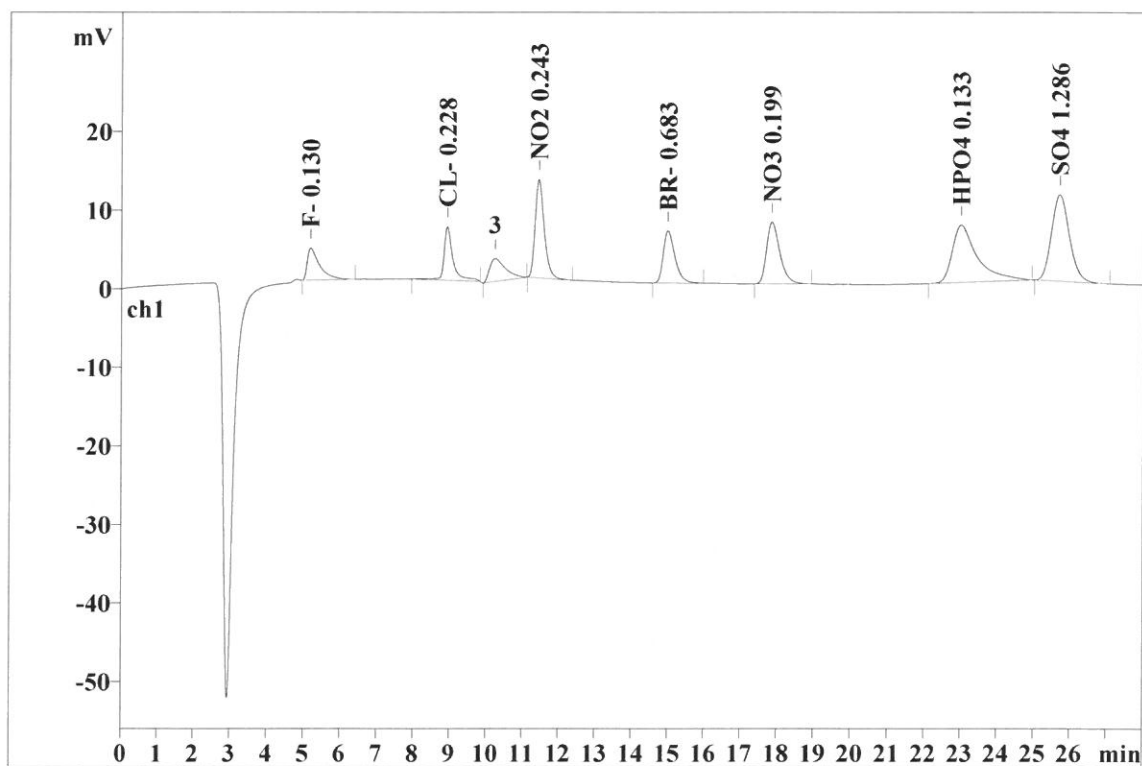

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.19	0.329	4.10	6.92	96.767	6.09
2	8.93	0.219	6.82	11.52	117.954	7.42
3	11.44	0.259	12.54	21.20	217.331	13.67
4	15.00	0.331	6.63	11.21	147.281	9.27
5	17.86	0.379	7.87	13.30	198.061	12.46
6	23.01	0.655	7.30	12.33	349.769	22.01
7	25.71	0.522	10.99	18.58	373.758	23.52
7	28.00	0.385	56.24	95.07	1500.921	94.43

Report date: 7/6/2017 12:43:28 PM
Printed by: wet


Ident: STD3
Analysis from: 6/8/2017 11:59:20 AM
File: _2017-06-08_

Last save: 6/8/2017 12:27:20 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14601

Last save: 6/8/2017 11:56:2

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

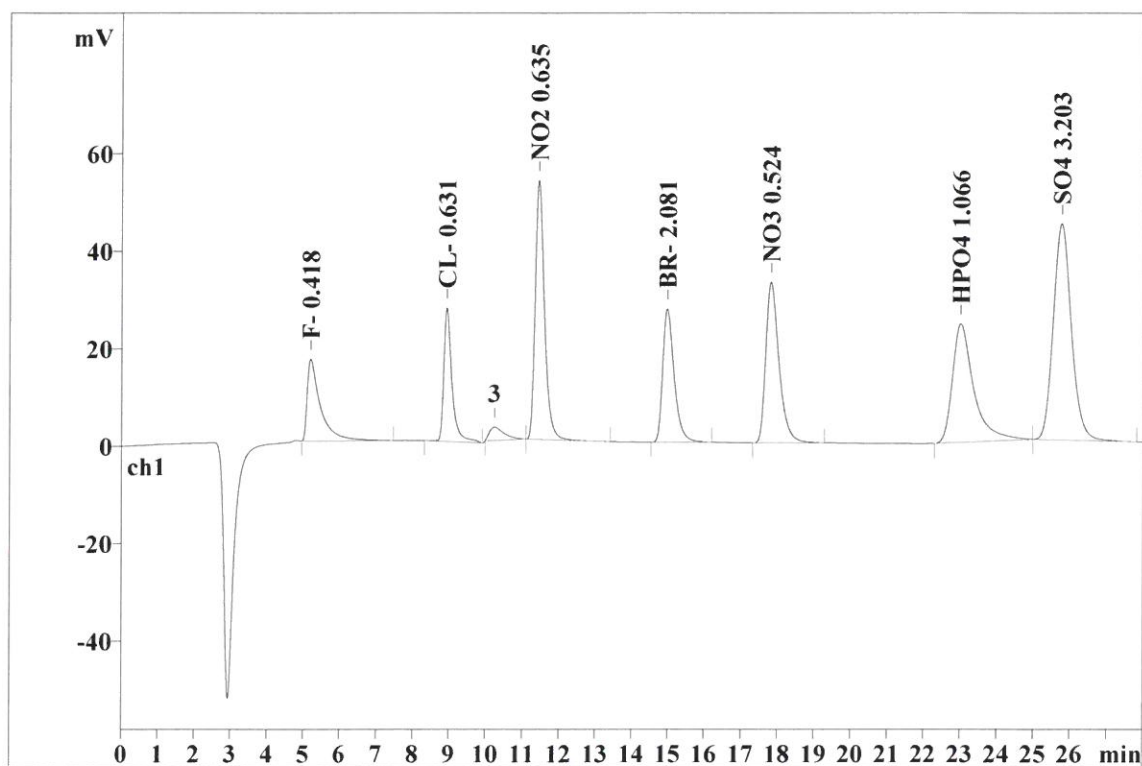

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.20	0.331	16.82	7.34	425.752	7.34
2	8.93	0.216	27.41	11.96	425.974	7.35
3	11.45	0.258	53.22	23.21	927.995	16.00
4	14.98	0.326	27.36	11.93	600.739	10.36
5	17.82	0.377	33.01	14.40	832.606	14.36
6	23.01	0.569	24.34	10.61	986.036	17.00
7	25.76	0.521	44.36	19.35	1523.030	26.26
7	28.00	0.371	226.53	98.80	5722.132	98.67

Report date: 7/6/2017 12:43:31 PM
Printed by: wet


Ident: STD4
Analysis from: 6/8/2017 12:30:17 PM
File: _2017-06-08_

Last save: 6/8/2017 12:58:17 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14602

Last save: 6/8/2017 12:27:2

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

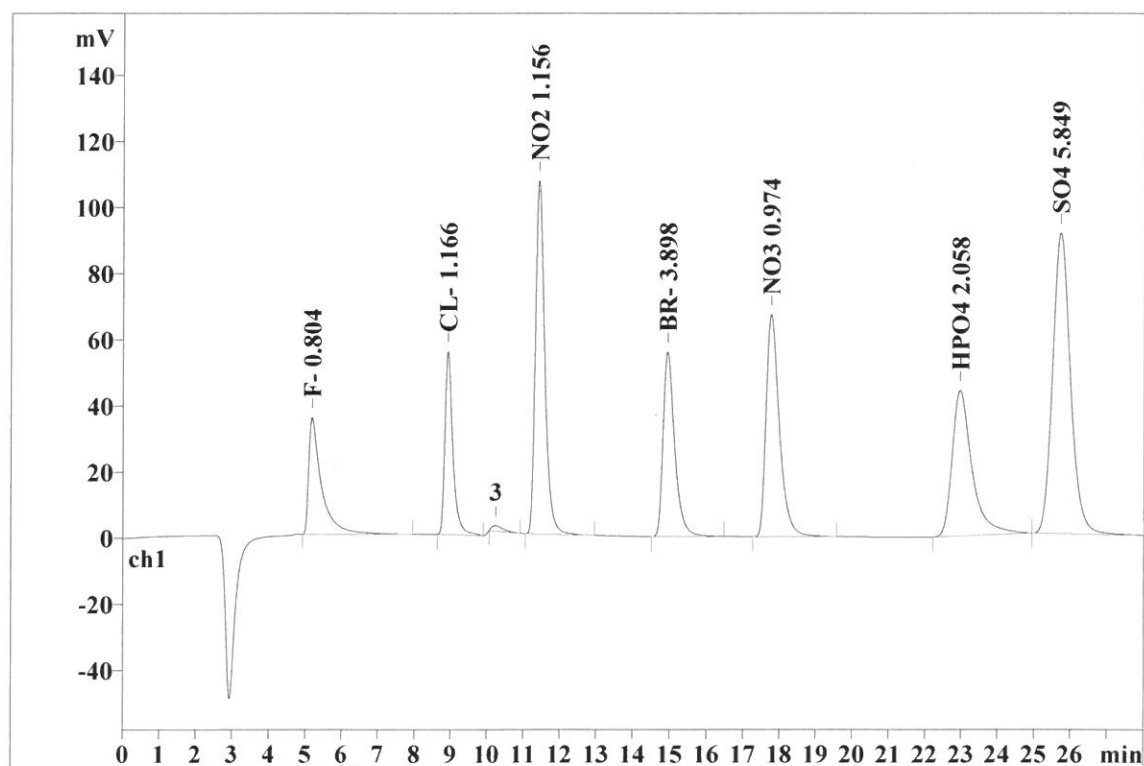

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.18	0.315	35.31	7.72	865.949	7.64
2	8.92	0.215	55.39	12.11	836.632	7.38
3	11.44	0.259	106.90	23.38	1872.101	16.51
4	14.94	0.325	55.90	12.22	1227.245	10.82
5	17.76	0.377	67.19	14.69	1705.574	15.04
6	22.97	0.544	44.04	9.63	1686.529	14.88
7	25.73	0.517	90.90	19.88	3108.135	27.42
7	28.00	0.364	455.64	99.64	11302.165	99.69

Report date: 7/6/2017 12:43:39 PM
Printed by: wet


Ident: STD5
Analysis from: 6/8/2017 1:01:16 PM
File: _2017-06-08_

Last save: 6/8/2017 1:29:16 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14603

Last save: 6/8/2017 12:58:1

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

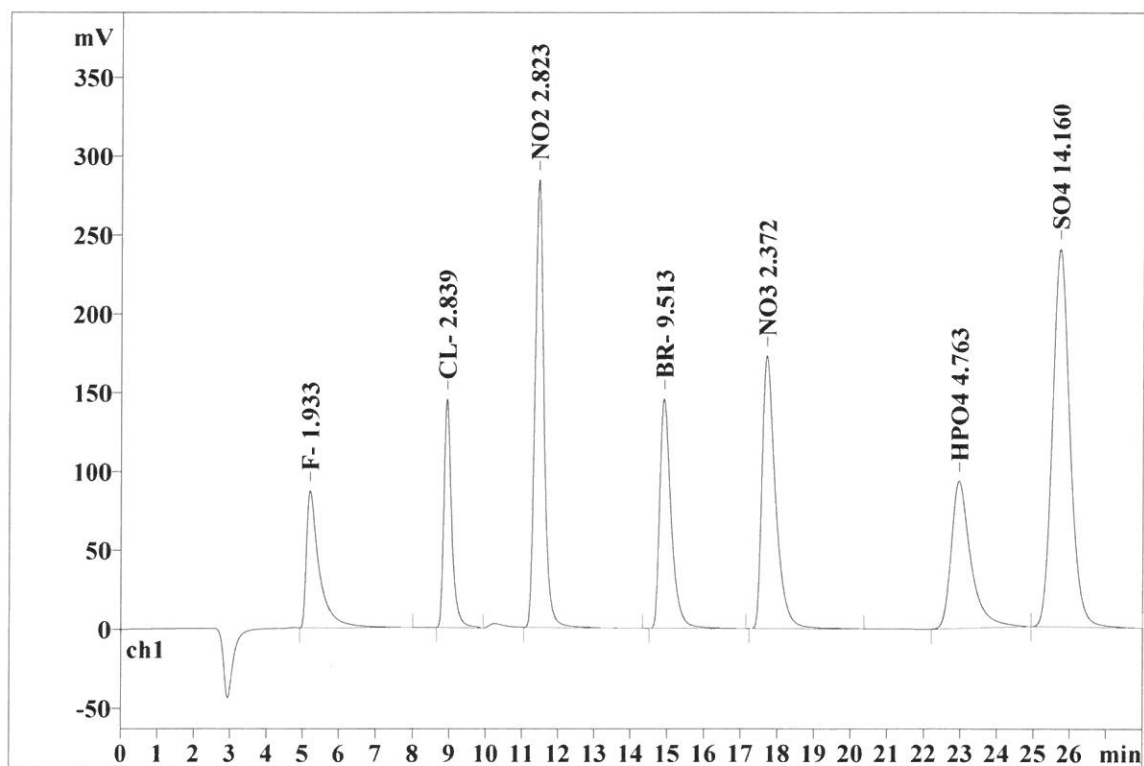

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.20	0.328	86.95	7.45	2163.327	7.62
2	8.92	0.210	145.16	12.44	2126.831	7.49
3	11.45	0.253	283.86	24.32	4883.553	17.20
4	14.91	0.320	145.56	12.47	3171.707	11.17
5	17.71	0.377	172.92	14.81	4432.055	15.61
6	22.96	0.540	93.31	7.99	3518.225	12.39
7	25.73	0.510	239.54	20.52	8090.250	28.50
7	28.00	0.362	1167.31	100.00	28385.948	100.00

Report date: 7/6/2017 12:43:44 PM
Printed by: wet


Ident: STD6
Analysis from: 6/8/2017 1:32:13 PM
File: _2017-06-08_

Last save: 6/8/2017 2:00:13 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14604

Last save: 6/8/2017 1:29:16

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

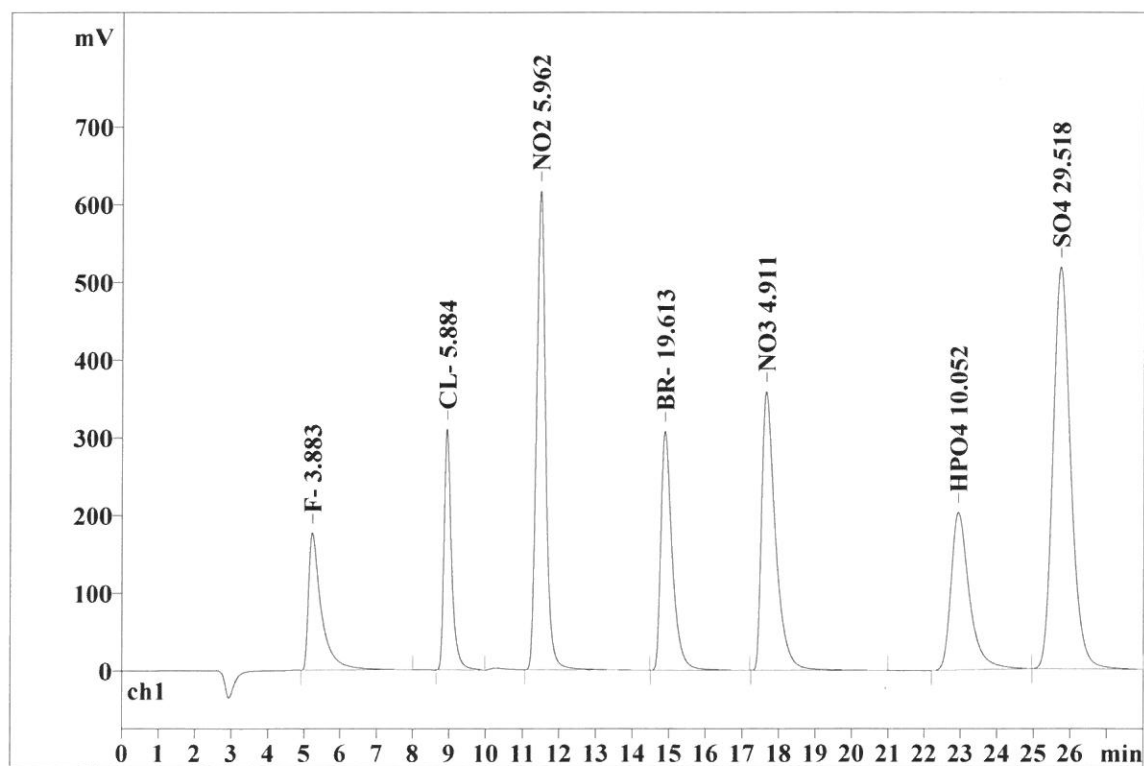

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.22	0.334	176.61	7.10	4409.863	7.34
2	8.94	0.206	310.16	12.46	4470.930	7.44
3	11.48	0.253	616.27	24.76	10599.485	17.65
4	14.89	0.317	307.53	12.35	6663.394	11.09
5	17.65	0.382	358.67	14.41	9382.927	15.62
6	22.94	0.515	202.97	8.15	7212.897	12.01
7	25.73	0.504	516.88	20.77	17327.478	28.85
7	28.00	0.359	2489.11	100.00	60066.973	100.00

Report date: 7/6/2017 12:43:50 PM
Printed by: wet


Ident: STD7
Analysis from: 6/8/2017 2:03:11 PM
File: _2017-06-08_

Last save: 6/8/2017 2:31:11 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14605

Last save: 6/8/2017 2:00:13

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

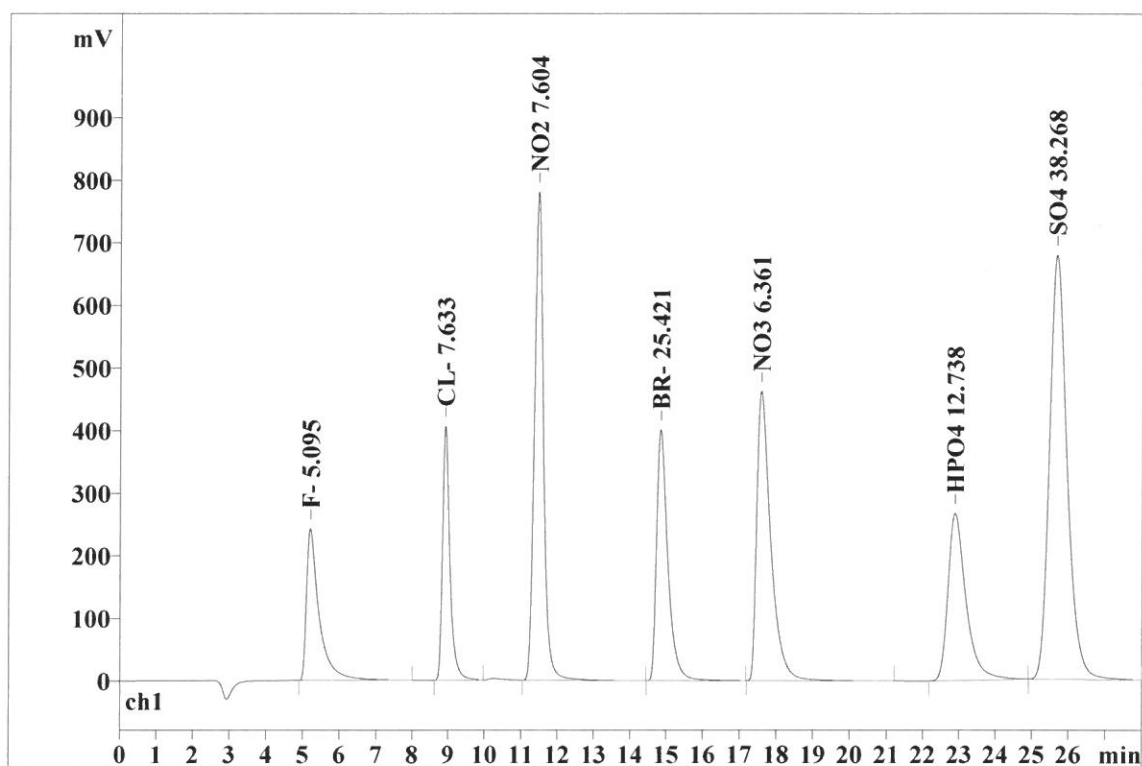

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.20	0.314	242.20	7.49	5777.014	7.40
2	8.92	0.204	405.89	12.55	5810.666	7.44
3	11.48	0.258	779.65	24.10	13618.960	17.44
4	14.85	0.315	400.64	12.38	8655.809	11.08
5	17.59	0.385	462.09	14.28	12214.587	15.64
6	22.88	0.508	266.94	8.25	9324.856	11.94
7	25.68	0.503	677.53	20.94	22690.021	29.06
7	28.00	0.355	3234.96	100.00	78091.913	100.00

Report date: 7/6/2017 12:43:58 PM
Printed by: wet


Ident: ICV
Analysis from: 6/8/2017 3:47:12 PM
File: _2017-06-08_

Last save: 6/8/2017 4:15:12 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14608

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

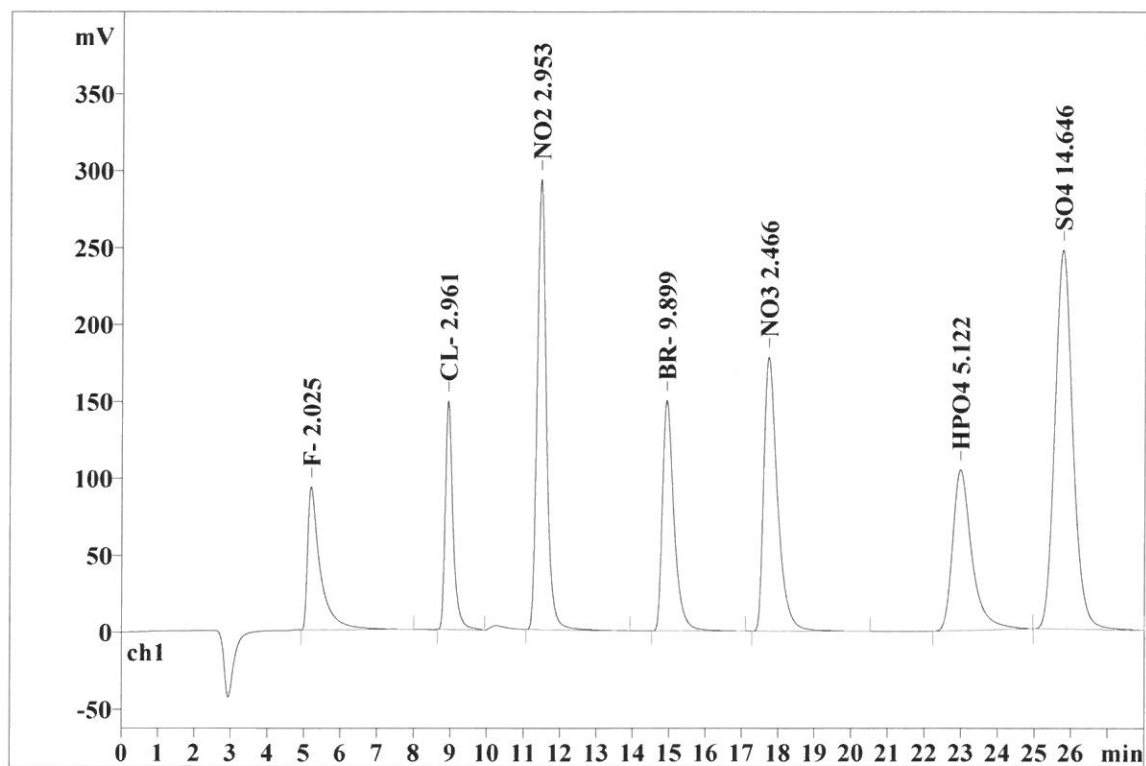

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.19	0.315	93.07	7.67	2261.540	7.60
2	8.94	0.212	148.90	12.26	2209.978	7.43
3	11.47	0.258	292.89	24.13	5131.328	17.25
4	14.93	0.322	149.89	12.35	3289.743	11.06
5	17.73	0.380	178.21	14.68	4606.693	15.48
6	22.98	0.529	104.59	8.61	3844.163	12.92
7	25.76	0.514	246.47	20.30	8411.568	28.27
7	28.00	0.361	1214.03	100.00	29755.013	100.00

Report date: 7/6/2017 12:44:03 PM
Printed by: wet


Ident: ICB
Analysis from: 6/8/2017 5:26:51 PM
File: _2017-06-08_

Last save: 6/8/2017 5:54:51 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14611

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

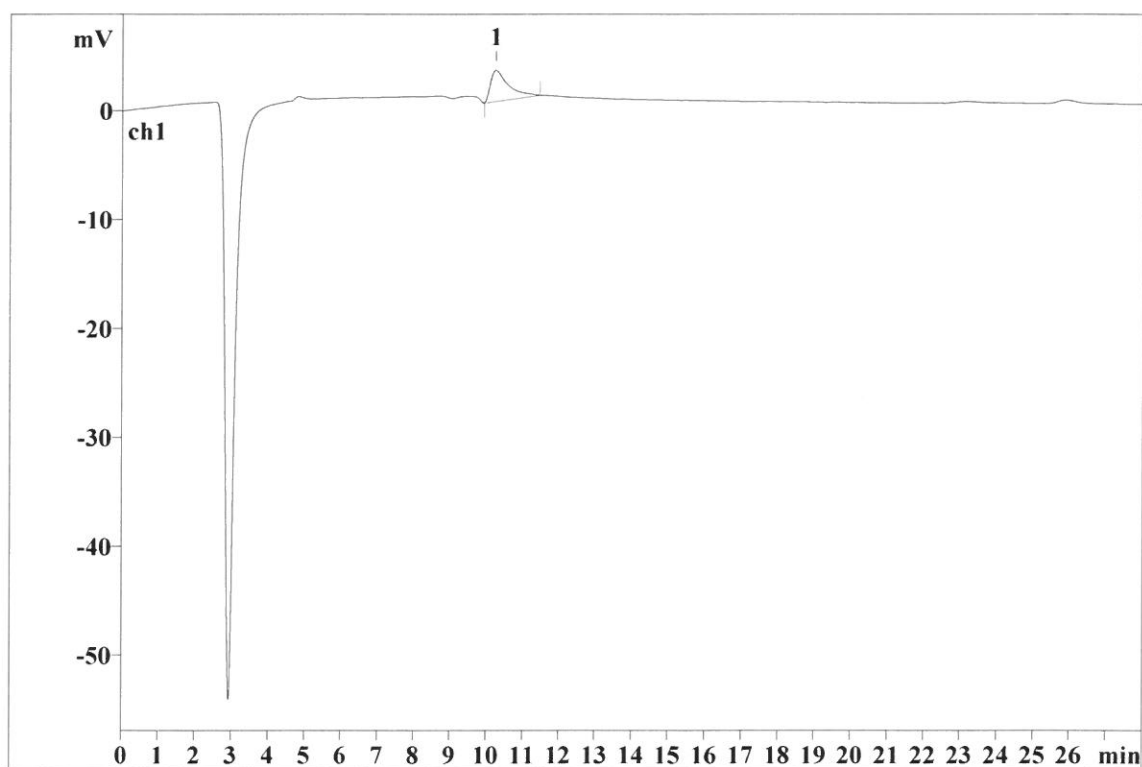

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.000	0.00	0.00	0.000	0.00

Report date: 8/1/2017 12:52:54 PM
 Printed by: wet


Ident: CCV
 Analysis from: 7/7/2017 4:48:26 PM
 File: _2017-07-07_

Last save: 7/7/2017 5:16:27 PM

Method: AnionIC2-060817.mtw
 Run operator: wet
 Analysis number: 14706

Last save: 6/8/2017 2:31:11

SAMPLE:
 : AK/AP
 Vial number: 2
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

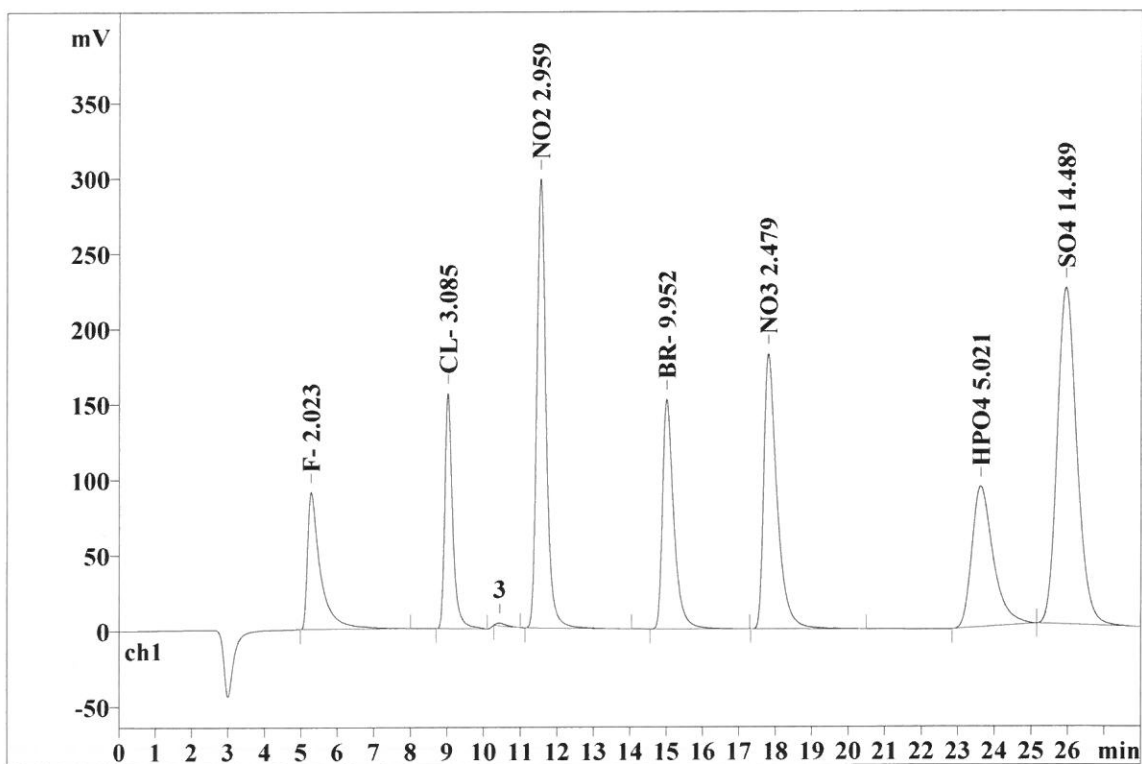

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.28	0.323	90.55	7.57	2258.826	7.59
2	9.03	0.211	155.61	13.01	2306.009	7.75
3	11.56	0.252	297.71	24.90	5141.092	17.27
4	15.02	0.316	152.03	12.71	3307.859	11.11
5	17.82	0.370	181.97	15.22	4631.154	15.56
6	23.63	0.598	93.03	7.78	3771.437	12.67
7	25.96	0.567	223.00	18.65	8316.339	27.94
7	28.00	0.377	1193.90	99.85	29732.715	99.89

This report has been created by IC Net
 METROHM LTD

Report date: 8/1/2017 12:53:00 PM
Printed by: wet


Ident: CCB
Analysis from: 7/7/2017 5:19:50 PM
File: _2017-07-07_

Last save: 7/7/2017 5:47:50 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14707

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

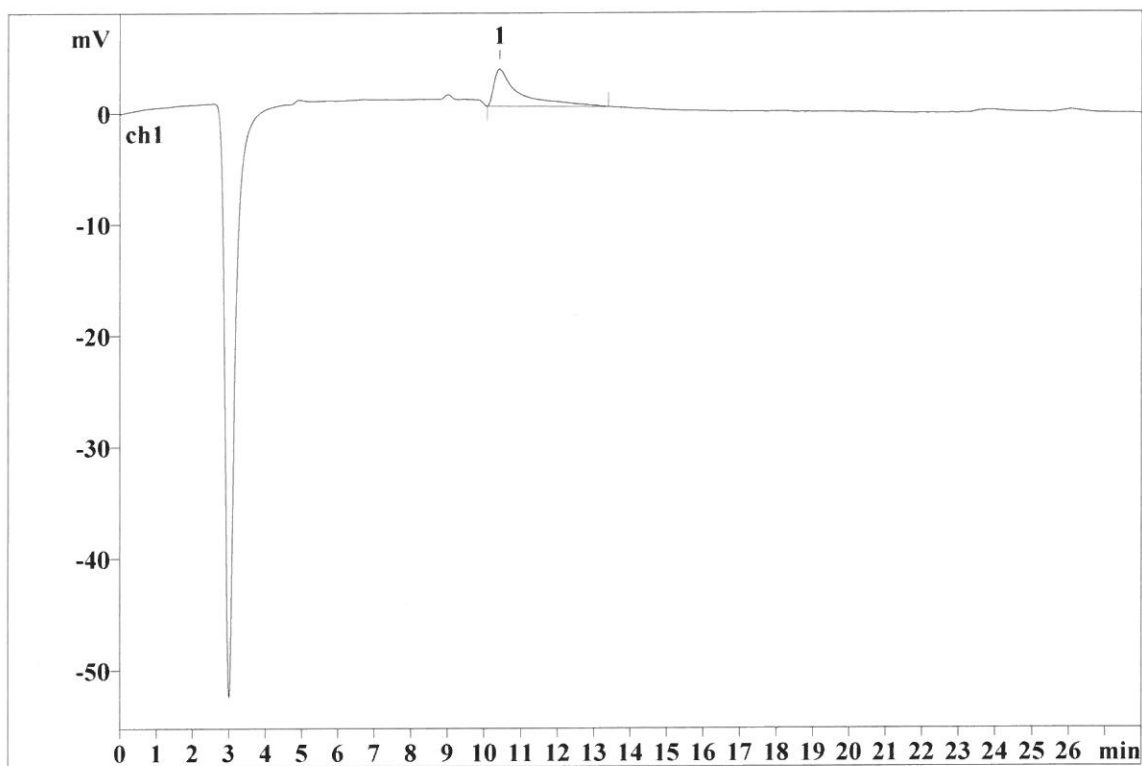

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.000	0.00	0.00	0.000	0.00

Report date: 8/1/2017 12:53:05 PM
Printed by: wet


Ident: LB89167BLW
Analysis from: 7/7/2017 5:50:54 PM
File: _2017-07-07_

Last save: 8/1/2017 12:52:16 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14708

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

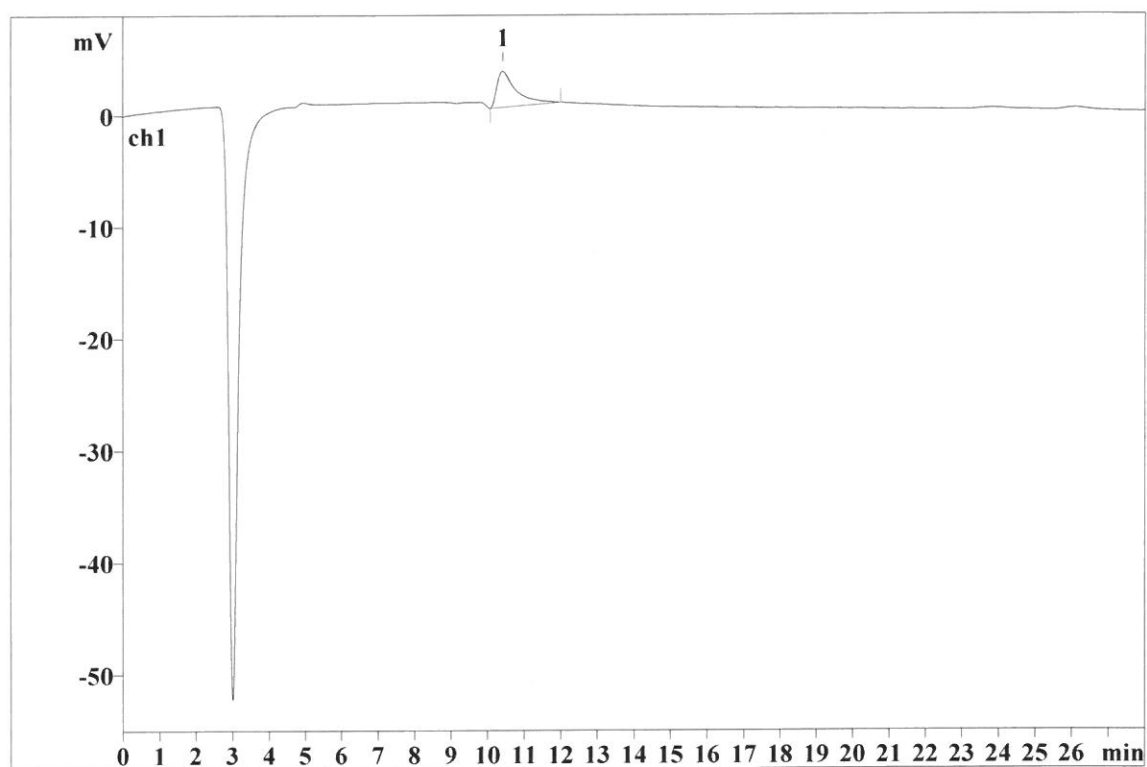

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.000	0.00	0.00	0.000	0.00

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:11 PM
Printed by: wet


Ident: LB89167BSW
Analysis from: 7/7/2017 6:21:53 PM
File: _2017-07-07_

Last save: 8/1/2017 12:52:17 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14709

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

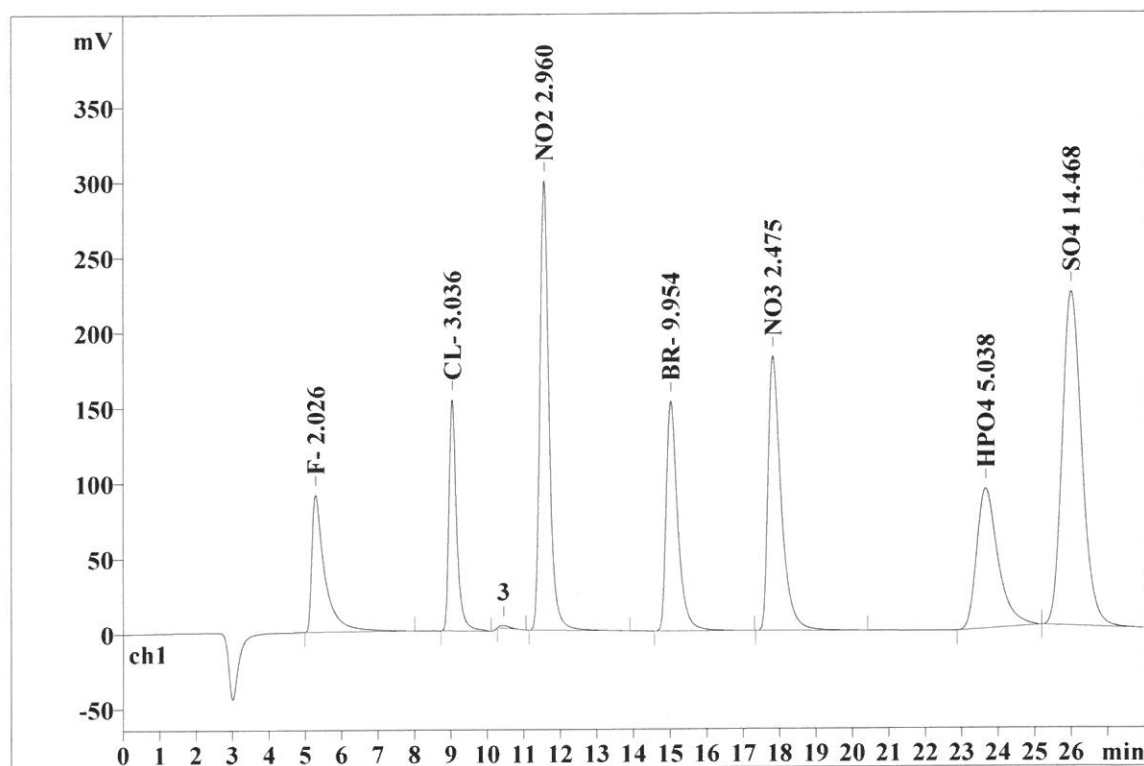

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.29	0.322	90.90	7.61	2262.071	7.61
2	9.04	0.211	153.41	12.84	2268.315	7.63
3	11.57	0.252	298.57	25.00	5143.868	17.30
4	15.02	0.315	152.50	12.77	3308.644	11.13
5	17.81	0.369	182.29	15.26	4622.620	15.55
6	23.66	0.601	92.89	7.78	3783.533	12.73
7	26.00	0.569	221.91	18.58	8304.010	27.93
7	28.00	0.377	1192.47	99.84	29693.060	99.87

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:18 PM
Printed by: wet


Ident: I4047-01
Analysis from: 7/7/2017 6:52:59 PM
File: _2017-07-07_

Last save: 8/1/2017 12:52:17 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14710

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

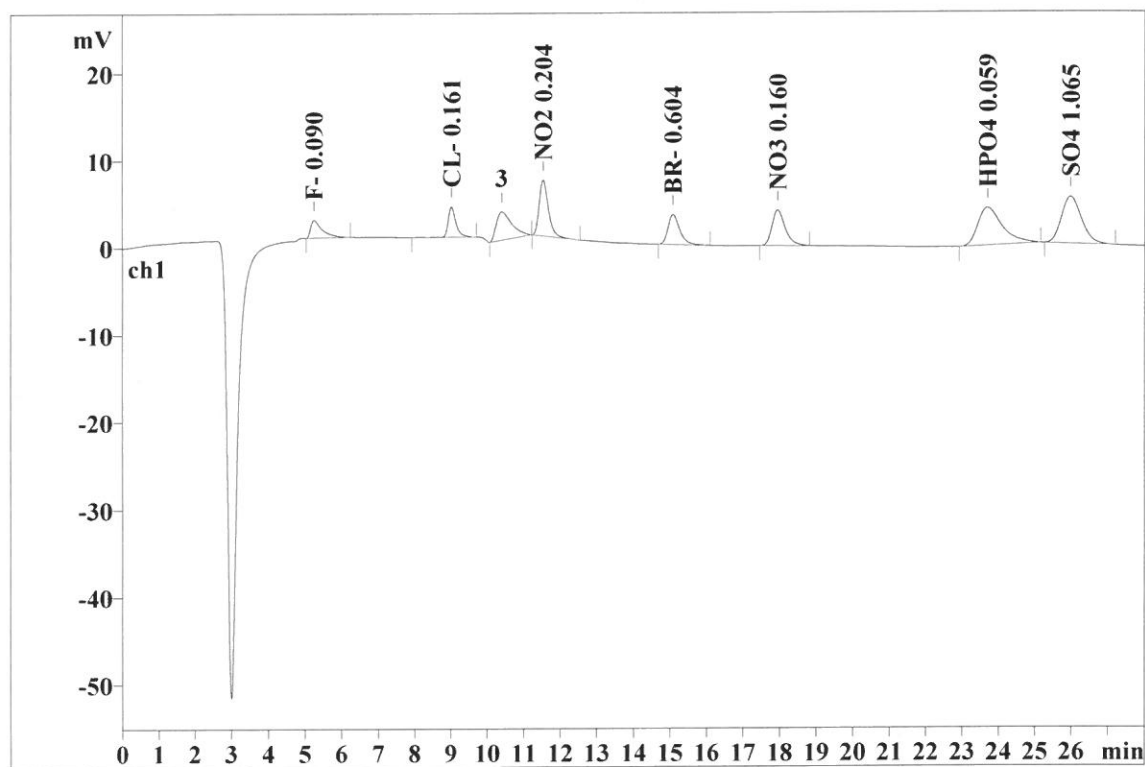

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.25	0.309	2.05	6.33	45.459	5.12
2	9.02	0.215	3.45	10.68	52.542	5.91
3	11.54	0.259	6.43	19.87	112.507	12.66
4	15.10	0.329	3.44	10.63	76.294	8.59
5	17.96	0.377	4.07	12.59	102.310	11.51
6	23.72	0.684	4.31	13.32	200.688	22.58
7	26.00	0.582	5.35	16.55	202.131	22.75
7	28.00	0.393	29.10	89.97	791.930	89.12

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:24 PM
Printed by: wet


Ident: I4047-02
Analysis from: 7/7/2017 7:23:57 PM
File: _2017-07-07_

Last save: 7/7/2017 7:51:57 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14711

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 29
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

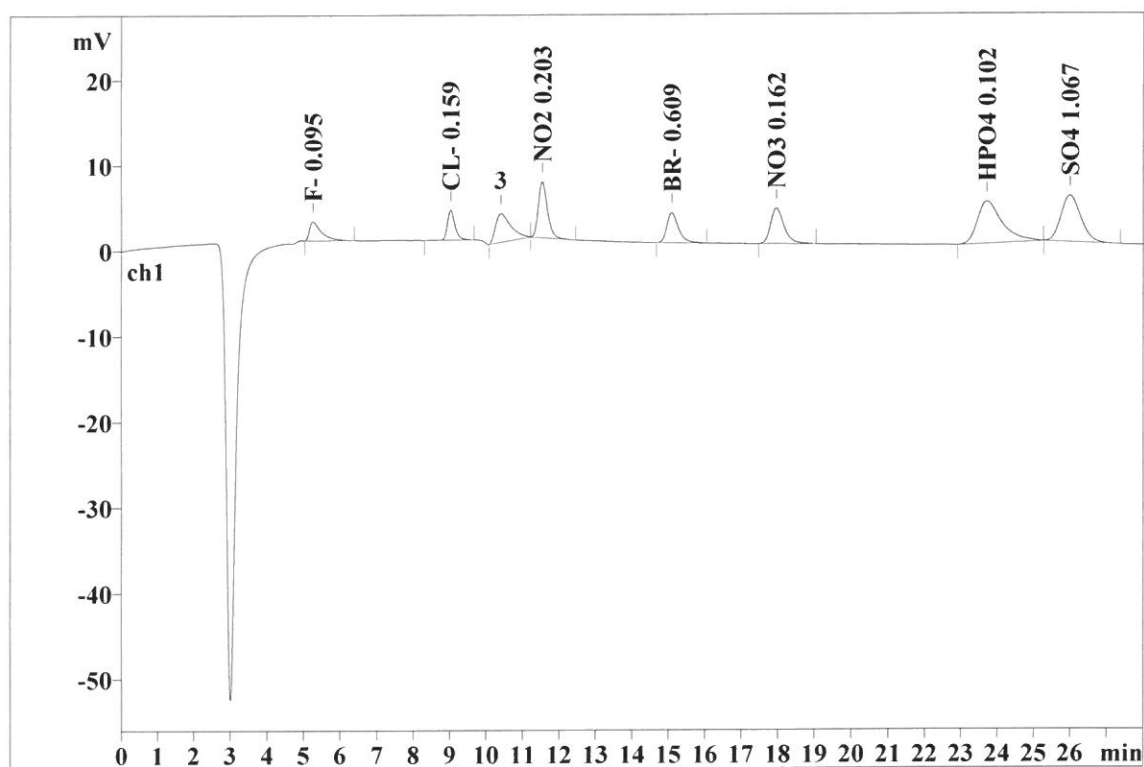

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.27	0.313	2.25	6.66	50.783	5.46
2	9.03	0.214	3.50	10.39	51.330	5.52
3	11.55	0.255	6.56	19.45	111.413	11.98
4	15.11	0.326	3.53	10.48	78.137	8.40
5	17.97	0.376	4.17	12.37	105.531	11.34
6	23.73	0.685	4.92	14.60	231.608	24.90
7	26.01	0.578	5.42	16.07	203.147	21.84
7	28.00	0.392	30.36	90.02	831.951	89.43

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:30 PM
Printed by: wet


Ident: I4047-03
Analysis from: 7/7/2017 7:54:55 PM
File: _2017-07-07_

Last save: 7/7/2017 8:22:55 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14712

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 30
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

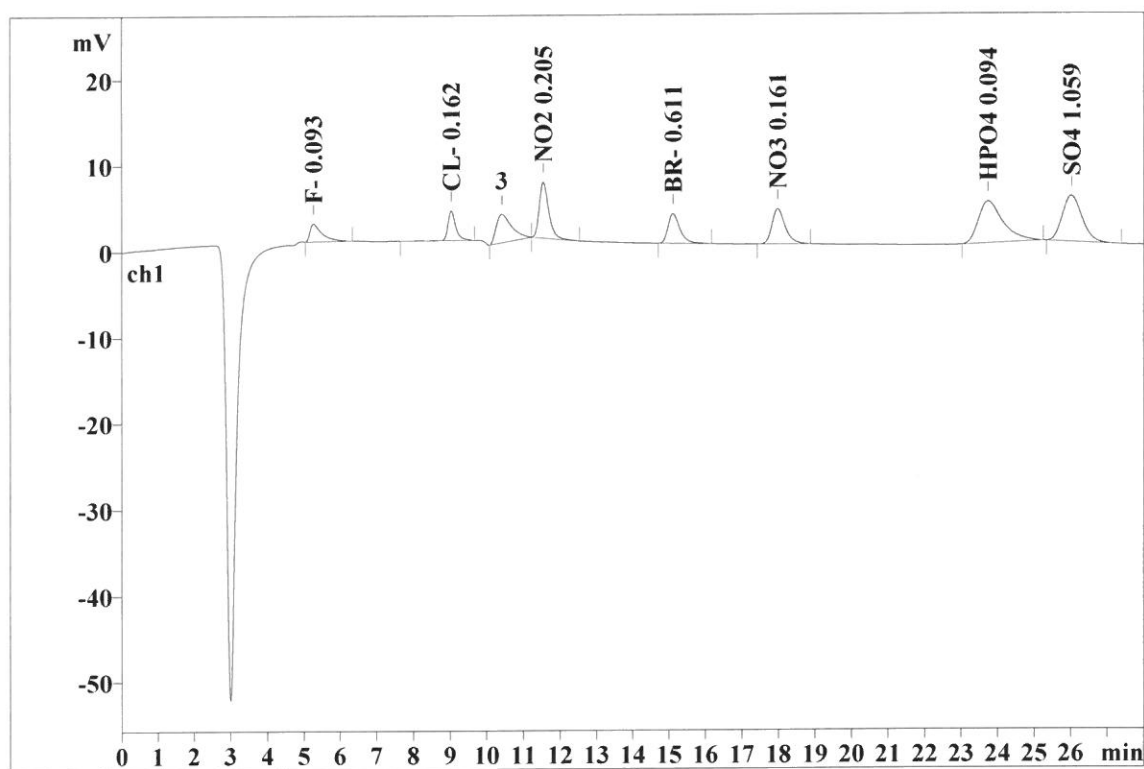

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.27	0.324	2.07	6.27	48.517	5.26
2	9.04	0.216	3.46	10.44	53.367	5.79
3	11.56	0.261	6.51	19.65	114.898	12.46
4	15.13	0.334	3.46	10.45	78.754	8.54
5	18.00	0.379	4.09	12.34	103.515	11.23
6	23.76	0.684	4.86	14.67	226.078	24.52
7	26.04	0.577	5.33	16.10	198.691	21.55
7	28.00	0.396	29.77	89.93	823.820	89.37

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:36 PM
Printed by: wet


Ident: I4047-04
Analysis from: 7/7/2017 8:25:53 PM
File: _2017-07-07_

Last save: 7/7/2017 8:53:53 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14713

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 31
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

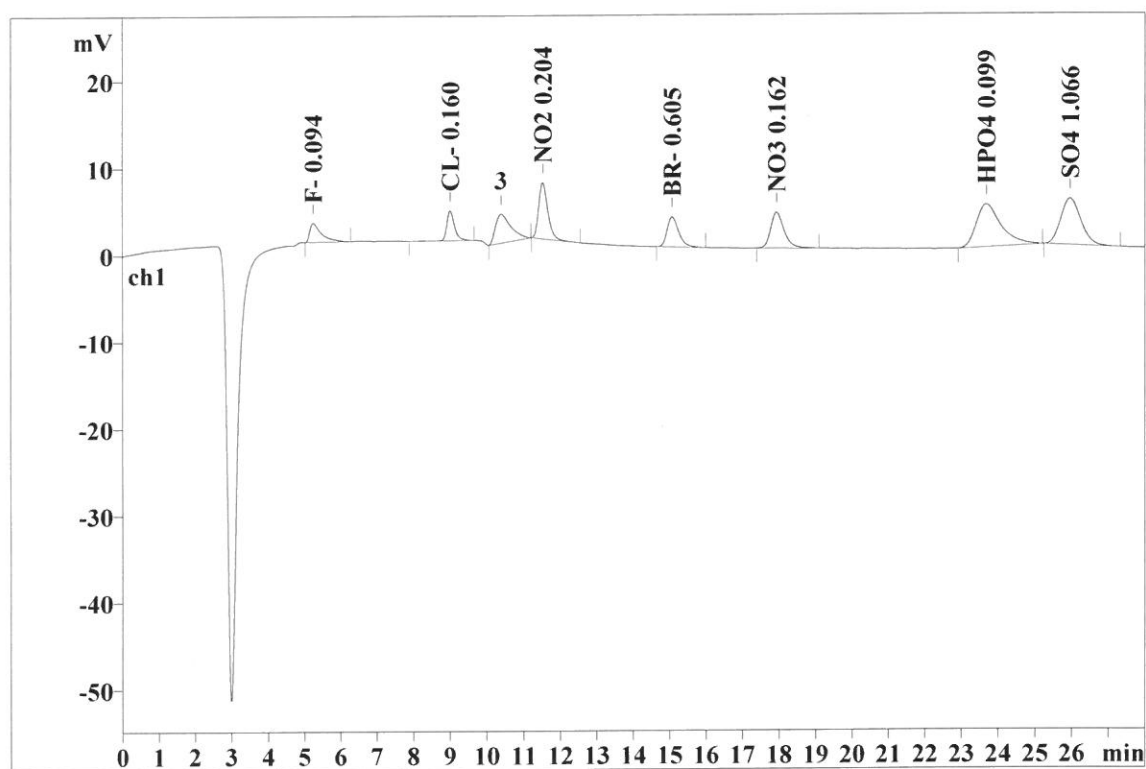

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.25	0.313	2.19	6.56	49.759	5.37
2	9.01	0.216	3.45	10.36	51.881	5.60
3	11.53	0.260	6.48	19.43	112.853	12.17
4	15.09	0.329	3.47	10.40	76.839	8.29
5	17.95	0.377	4.14	12.40	105.010	11.33
6	23.70	0.680	4.93	14.78	229.796	24.78
7	25.98	0.584	5.35	16.04	202.763	21.87
7	28.00	0.394	30.01	89.98	828.900	89.40

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:41 PM
Printed by: wet


Ident: I4047-05
Analysis from: 7/7/2017 8:56:53 PM
File: _2017-07-07_

Last save: 7/7/2017 9:24:52 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14714

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

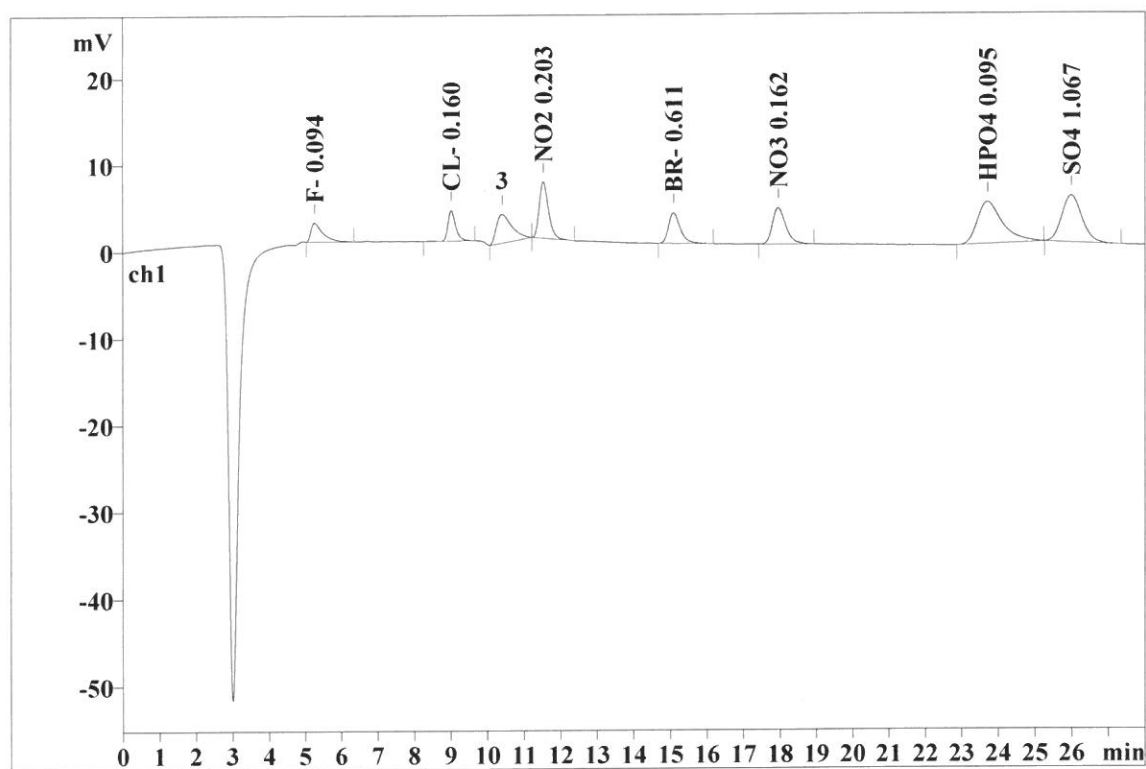

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.27	0.321	2.18	6.54	49.839	5.39
2	9.02	0.216	3.49	10.45	51.704	5.59
3	11.54	0.259	6.50	19.48	112.455	12.15
4	15.10	0.329	3.52	10.54	78.695	8.50
5	17.97	0.377	4.17	12.49	105.152	11.36
6	23.73	0.687	4.81	14.41	226.578	24.48
7	26.00	0.582	5.37	16.11	203.268	21.96
7	28.00	0.396	30.03	90.04	827.692	89.44

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:47 PM
Printed by: wet


Ident: I4047-06
Analysis from: 7/7/2017 9:27:50 PM
File: _2017-07-07_

Last save: 7/7/2017 9:55:50 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14715

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 29
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

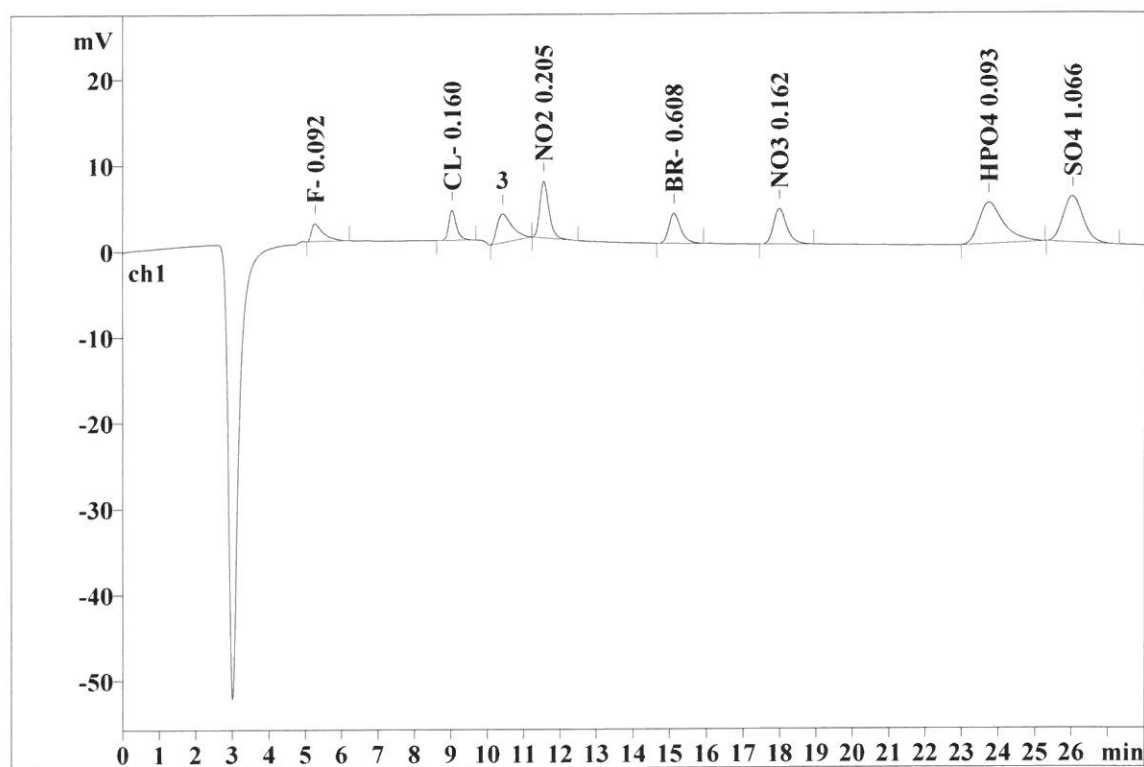

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.27	0.323	2.05	6.19	47.146	5.11
2	9.04	0.217	3.48	10.48	51.878	5.62
3	11.56	0.261	6.56	19.74	114.444	12.41
4	15.13	0.331	3.49	10.50	77.642	8.42
5	18.00	0.379	4.14	12.47	105.563	11.44
6	23.76	0.686	4.79	14.43	225.103	24.40
7	26.04	0.584	5.35	16.11	202.573	21.96
7	28.00	0.397	29.87	89.92	824.350	89.37

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:53:53 PM
Printed by: wet


Ident: I4047-07
Analysis from: 7/7/2017 9:58:48 PM
File: _2017-07-07_

Last save: 7/7/2017 10:26:48 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14716

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 30
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

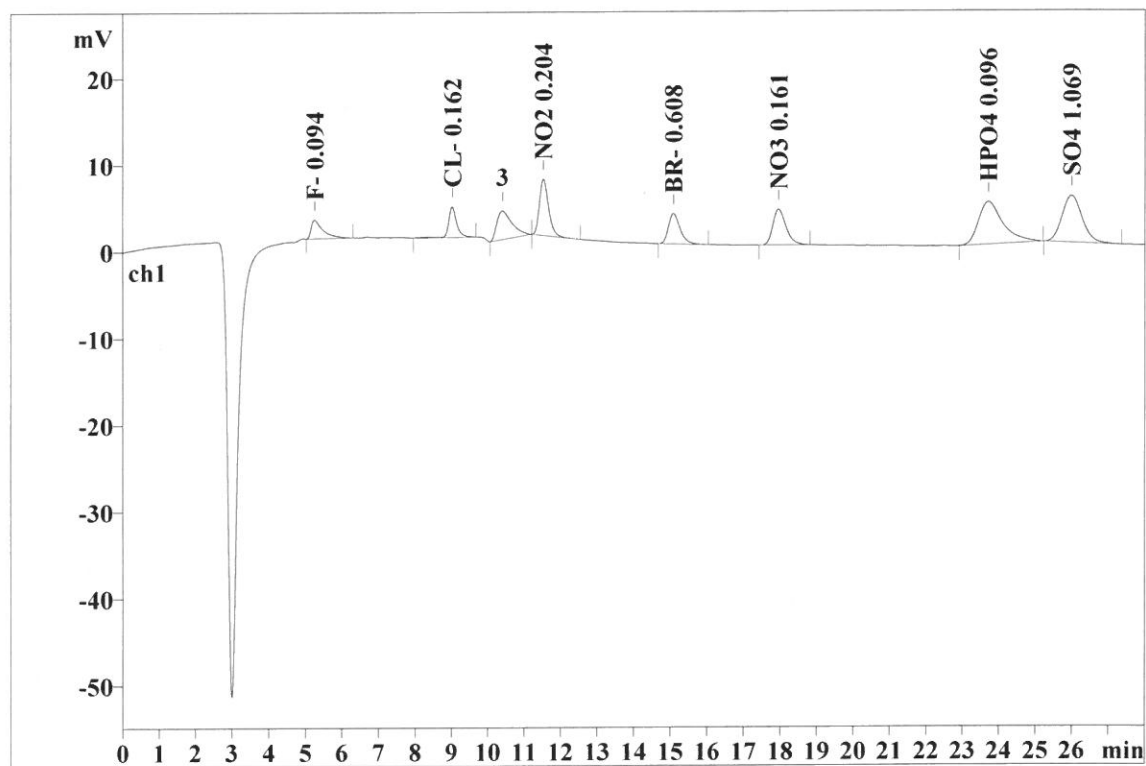

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.26	0.312	2.16	6.46	49.081	5.30
2	9.03	0.216	3.50	10.48	53.660	5.79
3	11.55	0.260	6.49	19.45	112.620	12.16
4	15.11	0.330	3.50	10.48	77.690	8.39
5	17.97	0.377	4.14	12.41	103.485	11.18
6	23.73	0.678	4.89	14.64	227.410	24.56
7	26.02	0.583	5.39	16.13	204.454	22.08
7	28.00	0.394	30.07	90.04	828.400	89.46

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:54:04 PM
Printed by: wet


Ident: I4047-07
Analysis from: 7/7/2017 10:29:46 PM
File: _2017-07-07_

Last save: 7/7/2017 10:57:46 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14717

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 31
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

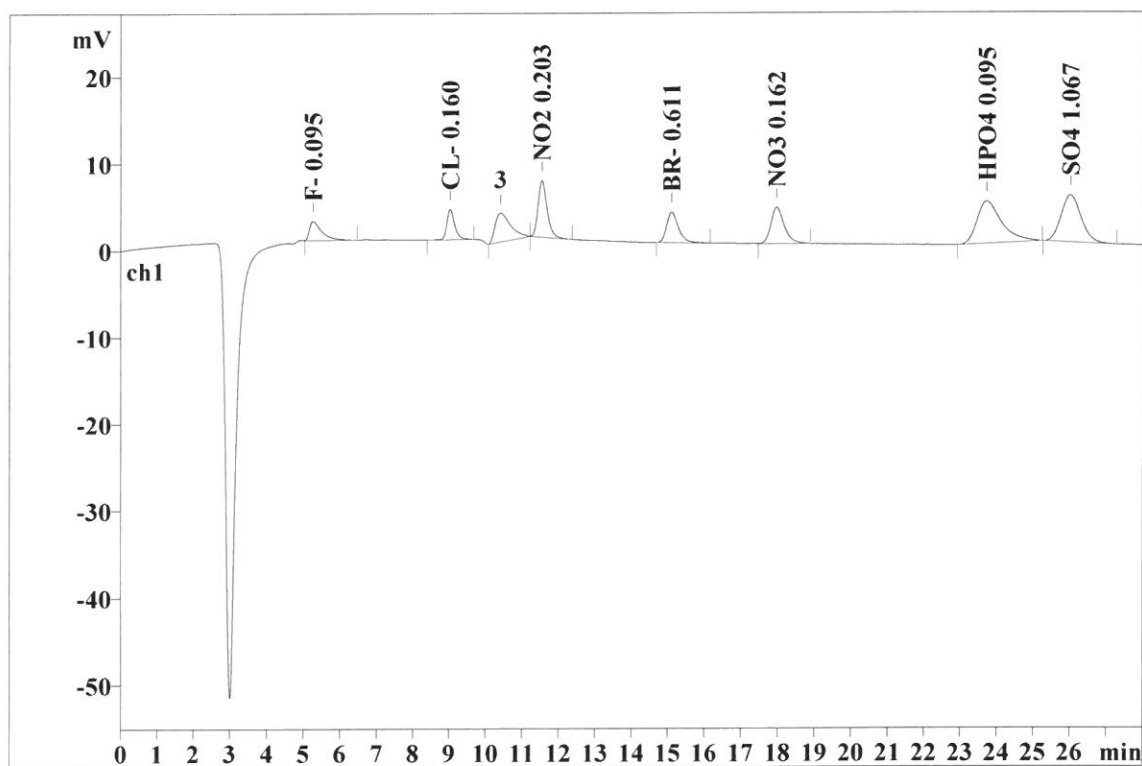

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.27	0.323	2.20	6.57	50.909	5.49
2	9.03	0.216	3.48	10.41	51.597	5.57
3	11.55	0.259	6.50	19.45	112.140	12.10
4	15.11	0.331	3.51	10.51	78.890	8.51
5	17.98	0.379	4.16	12.45	105.139	11.34
6	23.74	0.682	4.86	14.54	226.975	24.49
7	26.03	0.582	5.38	16.11	203.208	21.93
7	28.00	0.396	30.07	90.05	828.857	89.43

This report has been created by IC Net
METROHM LTD

Report date: 8/1/2017 12:54:11 PM
Printed by: wet


Ident: CCV
Analysis from: 7/7/2017 11:00:52 PM
File: _2017-07-07_

Last save: 7/7/2017 11:28:53 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14718

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

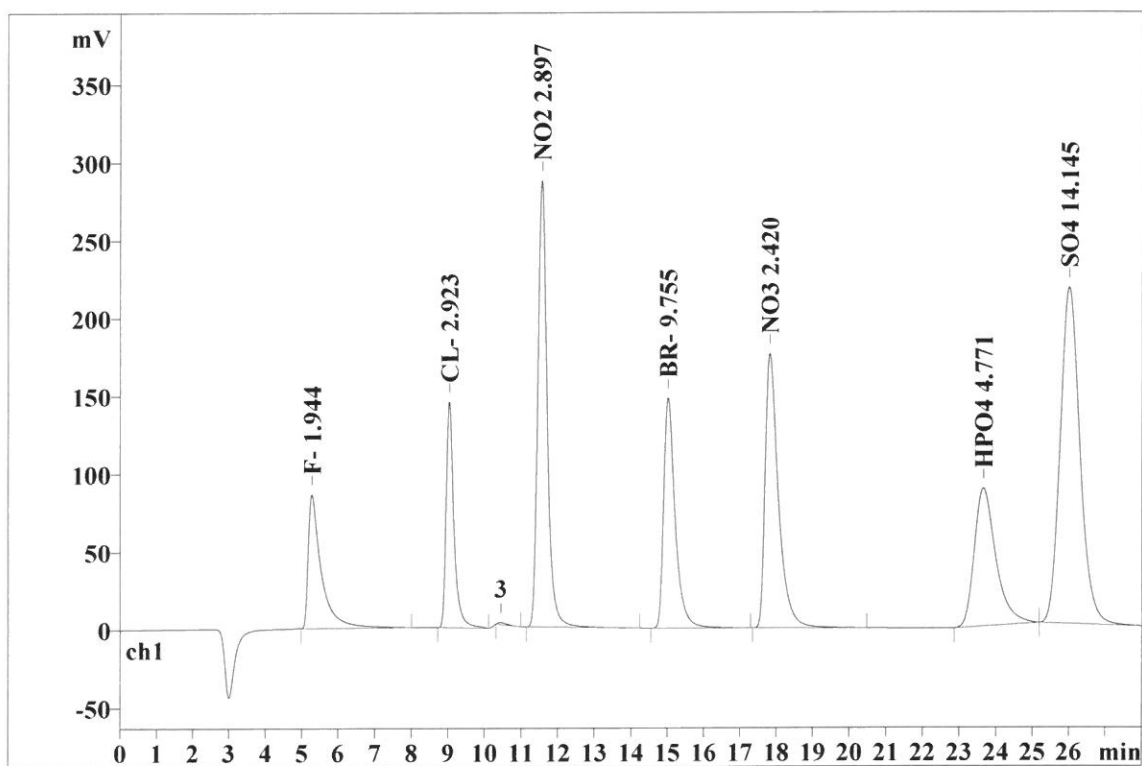

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.29	0.329	85.84	7.48	2168.199	7.51
2	9.04	0.214	144.87	12.63	2181.063	7.56
3	11.56	0.256	286.97	25.01	5027.556	17.42
4	15.02	0.318	147.60	12.86	3240.042	11.23
5	17.82	0.372	176.22	15.36	4515.649	15.65
6	23.67	0.597	88.54	7.72	3591.455	12.45
7	26.01	0.568	215.95	18.82	8108.638	28.10
7	28.00	0.379	1145.99	99.88	28832.601	99.92

Report date: 8/1/2017 12:54:16 PM
Printed by: wet


Ident: CCB
Analysis from: 7/7/2017 11:31:50 PM
File: _2017-07-07_

Last save: 7/7/2017 11:59:50 PM

Method: AnionIC2-060817.mtw
Run operator: wet
Analysis number: 14719

Last save: 6/8/2017 2:31:11

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

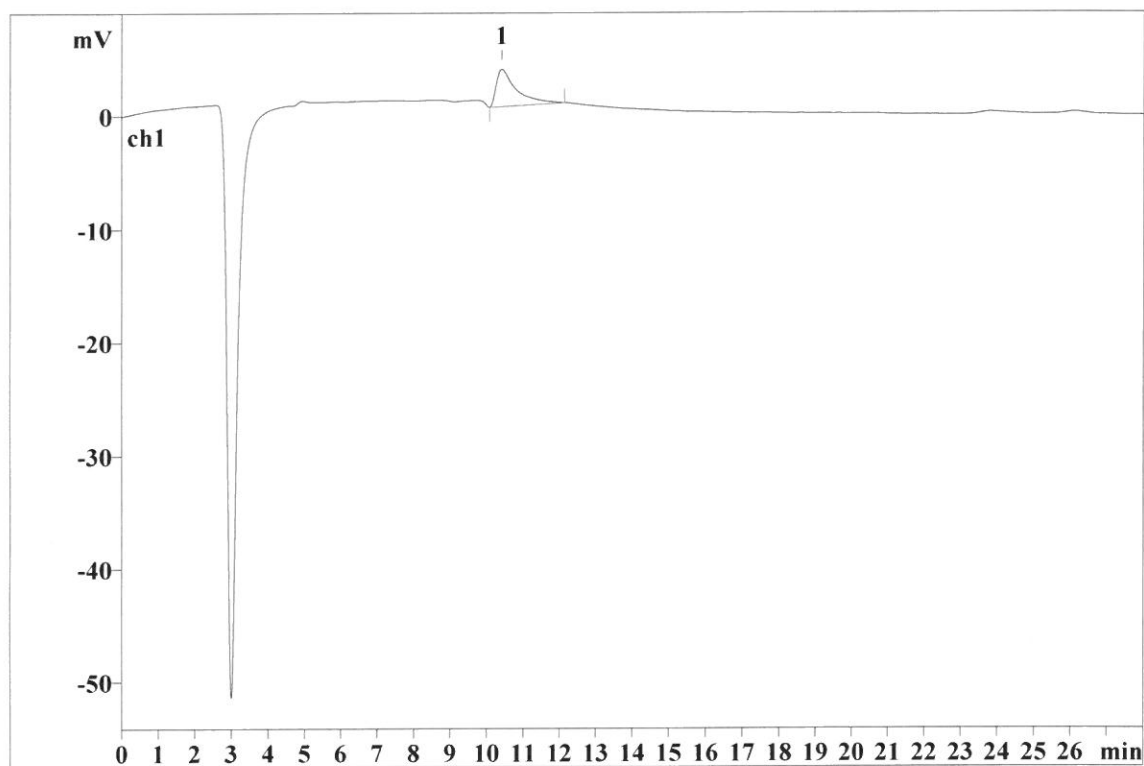

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.000	0.00	0.00	0.000	0.00