

ISM02.4


LB 89244

INSTRUMENT ID: CV2

Linear

 μ Abs.:

37796

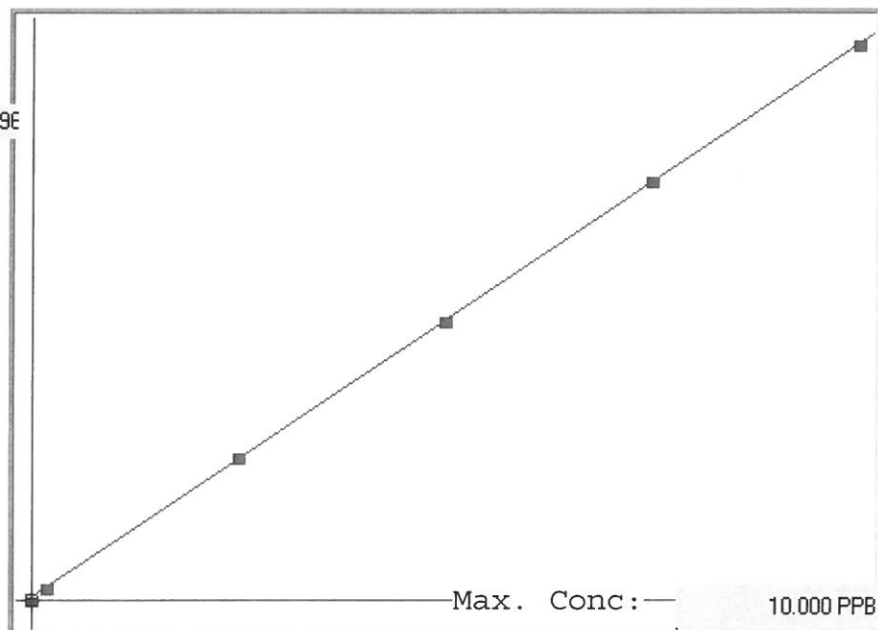

A= 0.0000e+000

B= 2.6534e-004

C= -5.4858e-002

Rho= 0.9999778

Accept=Accepted

glope
y=intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	-0.027	-0.027	105	0.000	105					-6
0.2	0.200	0.188	-0.012	914	0.0 %	914					2
2.5	2.500	2.542	0.042	9787	0.0 %	9787					0
5.0	5.000	5.008	0.008	19082	0.0 %	19082					0
7.5	7.500	7.515	0.015	28530	0.0 %	28530					0
10.0	10.000	9.974	-0.026	37796	0.0 %	37796					0

103
8/31/17

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	105	-		0 ISM02.4	PPB	8/3/2017 17:36	Std
	0.2 S0.2	914	-		0.2 ISM02.4	PPB	8/3/2017 17:38	Std
	2.5 S2.5	9787	-		2.5 ISM02.4	PPB	8/3/2017 17:40	Std
	5 S5	19082	-		5 ISM02.4	PPB	8/3/2017 17:42	Std
	7.5 S7.5	28530	-		7.5 ISM02.4	PPB	8/3/2017 17:45	Std
	10 S10	37796	-		10 ISM02.4	PPB	8/3/2017 17:47	Std
ICV	ICV	14721	3.8512 -		ISM02.4	PPB	8/3/2017 17:50	SMPL
ICB	ICB	0	-0.0549 -		ISM02.4	PPB	8/3/2017 17:52	SMPL
CCV089	CCV089	19282	5.0614 -		ISM02.4	PPB	8/3/2017 17:54	SMPL
CCB089	CCB089	-4	-0.0559 -		ISM02.4	PPB	8/3/2017 17:57	SMPL
PB101197BL	PBW003	94	-0.0299 -		ISM02.4	PPB	8/3/2017 17:59	SMPL
I4459-01	MBDWY1	3510	0.8765 -		ISM02.4	PPB	8/3/2017 18:01	SMPL
I4459-02	MBDWY1D	3424	0.8537 -		ISM02.4	PPB	8/3/2017 18:03	SMPL
I4459-03	MBDWY1S	7331	1.8903 -		ISM02.4	PPB	8/3/2017 18:06	SMPL
I4459-04	MBDWY2	30367	8.0026 -		ISM02.4	PPB	8/3/2017 18:08	SMPL
I4459-05	MBDX49	71199	18.8369 -		ISM02.4	PPB	8/3/2017 18:10	SMPL
I4459-06	MBDX50	4613	1.1691 -		ISM02.4	PPB	8/3/2017 18:13	SMPL
I4459-07	MBDX51	28907	7.6152 -		ISM02.4	PPB	8/3/2017 18:15	SMPL
I4459-08	MBDX52	167761	44.4584 -		ISM02.4	PPB	8/3/2017 18:17	SMPL
I4459-09	MBDX53	8572	2.2196 -		ISM02.4	PPB	8/3/2017 18:19	SMPL
I4459-10	MBDX54	24254	6.3806 -		ISM02.4	PPB	8/3/2017 18:22	SMPL
I4459-11	MBDX55	44783	11.8277 -		ISM02.4	PPB	8/3/2017 18:24	SMPL
I4459-05DLX5	MBDX49	14182	3.7082 -		ISM02.4	PPB	8/3/2017 18:26	SMPL
I4459-08DLX10	MBDX52	17396	4.5609 -		ISM02.4	PPB	8/3/2017 18:29	SMPL
I4459-11DLX2	MBDX55	22266	5.8531 -		ISM02.4	PPB	8/3/2017 18:31	SMPL
CCV090	CCV090	19138	5.0232 -		ISM02.4	PPB	8/3/2017 18:33	SMPL
CCB090	CCB090	-15	-0.0588 -		ISM02.4	PPB	8/3/2017 18:36	SMPL