

LB89263


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

35963

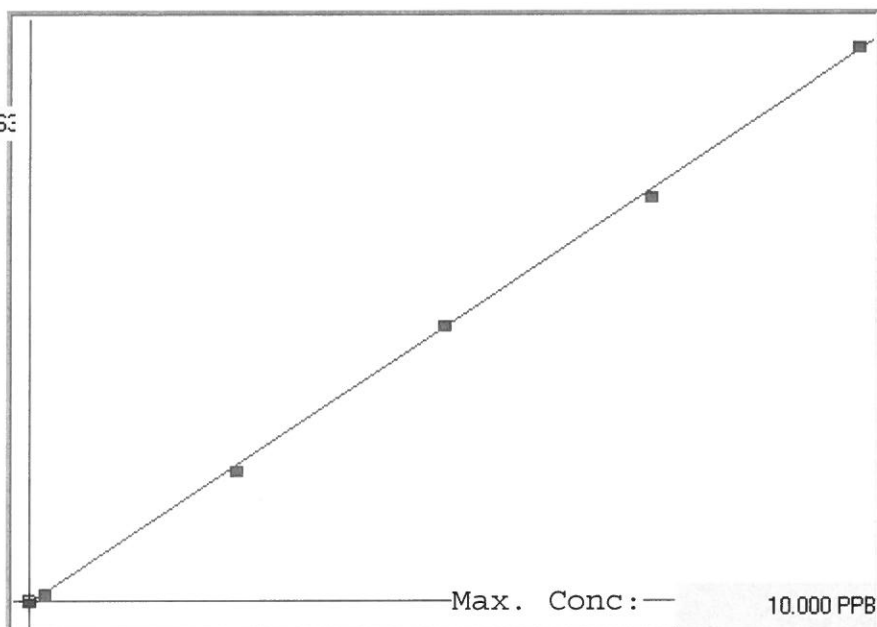

A= 0.0000e+000

B= 2.7878e-004

C= 5.4659e-002

Rho= 0.9998009

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.056	0.056	5	0.000	5				
0.2	0.200	0.202	0.002	529	0.0 %	529				
2.5	2.500	2.433	-0.067	8531	0.0 %	8531				
5.0	5.000	5.053	0.053	17930	0.0 %	17930				
7.5	7.500	7.375	-0.125	26259	0.0 %	26259				
10.0	10.000	10.080	0.080	35963	0.0 %	35963				

LB89263 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Aug 2017 11:09:15

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	5	-	0.00007470A	PPB	04 Aug 2017 11:28:59	S	Std
0.2 - 1	50.2	529	-	0.20007470A	PPB	04 Aug 2017 11:31:17	S	Std
2.5 - 1	52.5	8531	-	2.50007470A	PPB	04 Aug 2017 11:33:25	S	Std
5.0 - 1	55	17930	-	5.00007470A	PPB	04 Aug 2017 11:35:33	S	Std
7.5 - 1	57.5	26259	-	7.50007470A	PPB	04 Aug 2017 11:37:41	S	Std
10.0 - 1	510	35963	-	10.00007470A	PPB	04 Aug 2017 11:42:16	S	Std
ICV95 - 1	ICV95	13085	3.8652	-7470A	PPB	04 Aug 2017 11:44:55	U	SMPL
ICB95 - 1	ICB95	-154	-0.0274	-7470A	PPB	04 Aug 2017 11:47:01	U	SMPL
CCV93 - 1	CCV93	17325	5.1119	-7470A	PPB	04 Aug 2017 11:49:08	U	SMPL
CCB93 - 1	CCB93	-121	-0.0177	-7470A	PPB	04 Aug 2017 11:51:14	U	SMPL
CRA - 1	CRA	567	0.1846	-7470A	PPB	04 Aug 2017 11:53:21	U	SMPL
HighStd - 1	HighStd	36168	10.1376	-7470A	PPB	04 Aug 2017 11:55:58	U	SMPL
ChkStd - 1	ChkStd	24393	6.8550	-7470A	PPB	04 Aug 2017 11:58:04	U	SMPL
PB101256BL - 1	PBW	-193	0.0009	-7470A	PPB	04 Aug 2017 12:00:13	U	SMPL
PB101256BS - 1	LCSW	11542	3.2724	-7470A	PPB	04 Aug 2017 12:02:21	U	SMPL
PB101256TB - 1	PB101208TB	-88	0.0301	-7470A	PPB	04 Aug 2017 12:04:29	U	SMPL
I4555-02 - 1	SV21074LM	14218	4.0184	-7470A	PPB	04 Aug 2017 12:06:37	U	SMPL
I4555-08 - 1	2013	-104	0.0257	-7470A	PPB	04 Aug 2017 12:08:45	U	SMPL
I4555-13 - 1	2043	-23	0.0482	-7470A	PPB	04 Aug 2017 12:10:54	U	SMPL
I4584-03 - 1	OK-01-080217	-16	0.0502	-7470A	PPB	04 Aug 2017 12:13:00	U	SMPL
CCV94 - 1	CCV94	17547	4.9464	-7470A	PPB	04 Aug 2017 12:15:07	U	SMPL
CCB94 - 1	CCB94	-107	0.0248	-7470A	PPB	04 Aug 2017 12:17:14	U	SMPL
I4585-03 - 1	OR-01-080217	-15	0.0505	-7470A	PPB	04 Aug 2017 12:19:20	U	SMPL
I4585-03DUP - 1	OR-01-080217DUP	-17	0.0499	-7470A	PPB	04 Aug 2017 12:21:27	U	SMPL
I4585-03MS - 1	OR-01-080217MS	11542	3.2724	-7470A	PPB	04 Aug 2017 12:23:34	U	SMPL
I4585-03MSD - 1	OR-01-080217MSD	11610	3.2913	-7470A	PPB	04 Aug 2017 12:25:41	U	SMPL
I4586-03 - 1	HARDWICK-SOIL-COMP	-106	0.0251	-7470A	PPB	04 Aug 2017 12:27:49	U	SMPL
I4591-03 - 1	DRUM-1-2-COMP	-50	0.0407	-7470A	PPB	04 Aug 2017 12:29:56	U	SMPL
I4591-07 - 1	GRAVEL-PILE	-34	0.0452	-7470A	PPB	04 Aug 2017 12:32:04	U	SMPL
PB101257BL - 1	PBW	-16	0.0502	-7470A	PPB	04 Aug 2017 12:34:13	U	SMPL
PB101257BS - 1	LCSW	11370	3.2244	-7470A	PPB	04 Aug 2017 12:36:21	U	SMPL
CCV95 - 1	CCV95	17664	4.9791	-7470A	PPB	04 Aug 2017 12:38:28	U	SMPL
CCB95 - 1	CCB95	-93	0.0287	-7470A	PPB	04 Aug 2017 12:40:35	U	SMPL
I4555-01 - 1	SV21074LM	267090	74.5144	-7470A	PPB	04 Aug 2017 12:42:43	U	SMPL
I4555-01DUP - 1	SV21074LMDUP	265128	73.9674	-7470A	PPB	04 Aug 2017 12:44:49	U	SMPL
I4555-01MS - 1	SV21074LMMS	275857	76.9585	-7470A	PPB	04 Aug 2017 12:47:15	U	SMPL
I4555-01MSD - 1	SV21074LMMSD	275549	76.8726	-7470A	PPB	04 Aug 2017 12:49:42	U	SMPL
I4585-03LX5 - 1		-282	-0.0240	-7470A	PPB	04 Aug 2017 12:54:59	U	SMPL
I4585-03A - 1		13250	3.7485	-7470A	PPB	04 Aug 2017 12:57:06	U	SMPL
I4555-01LX5 - 1		50983	14.2678	-7470A	PPB	04 Aug 2017 12:59:14	U	SMPL
I4555-01A - 1		276337	77.0923	-7470A	PPB	04 Aug 2017 13:01:22	U	SMPL
CCV96 - 1	CCV96	16420	4.6323	-7470A	PPB	04 Aug 2017 13:03:32	U	SMPL
CCB96 - 1	CCB96	-342	-0.0407	-7470A	PPB	04 Aug 2017 13:05:57	U	SMPL
I4555-01DLX10 - 1		24209	6.8037	-7470A	PPB	04 Aug 2017 13:08:05	U	SMPL
I4555-01DUPDLX10 - 1		24439	6.8678	-7470A	PPB	04 Aug 2017 13:10:13	U	SMPL
I4555-01MSDLX10 - 1		26177	7.3523	-7470A	PPB	04 Aug 2017 13:12:21	U	SMPL
I4555-01MSDDLX10 - 1		26953	7.5687	-7470A	PPB	04 Aug 2017 13:14:30	U	SMPL
I4555-01LDLX50 - 1		4756	1.3805	-7470A	PPB	04 Aug 2017 13:16:39	U	SMPL
I4555-01ADLX10 - 1		26426	7.4217	-7470A	PPB	04 Aug 2017 13:18:48	U	SMPL
CCV97 - 1	CCV97	17310	4.8804	-7470A	PPB	04 Aug 2017 13:23:03	U	SMPL
CCB97 - 1	CCB97	-134	0.0173	-7470A	PPB	04 Aug 2017 13:25:11	U	SMPL