


7470A

LB 89461

INSTRUMENT ID: CV2

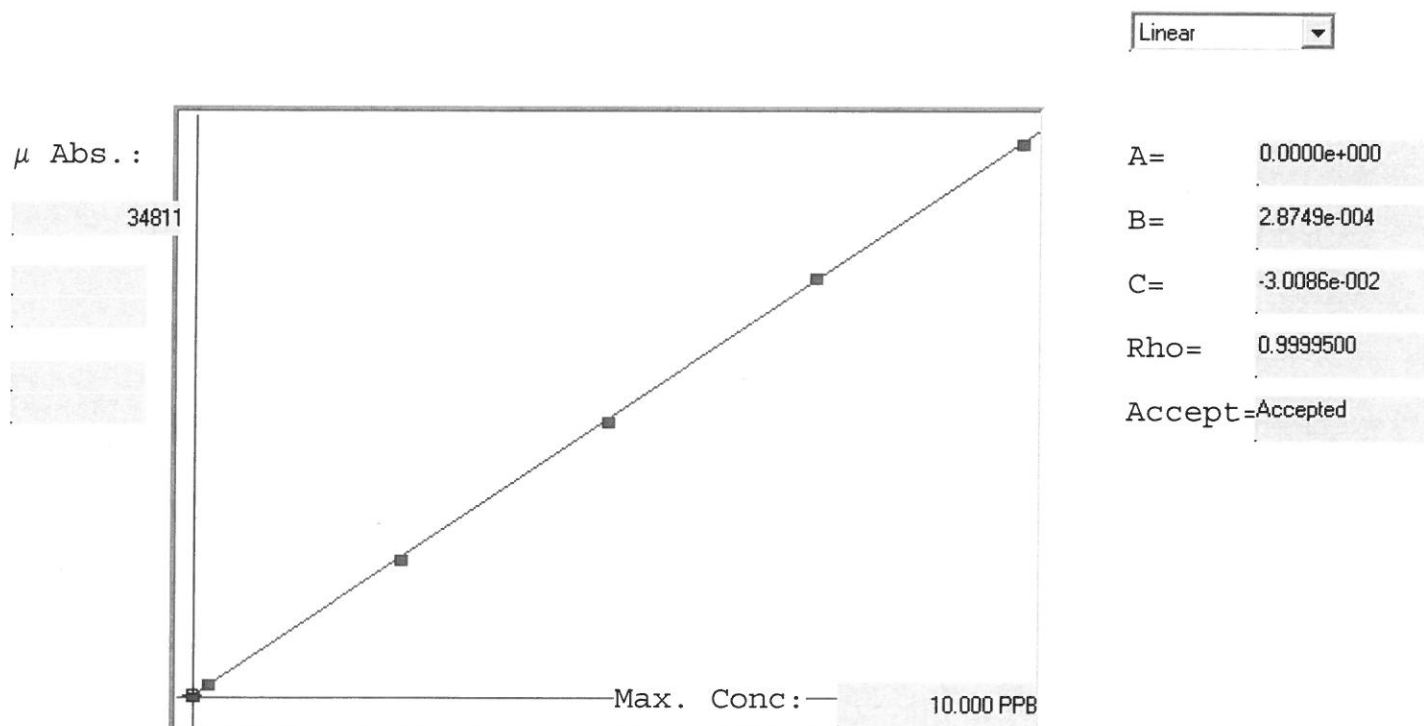

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	123	0.000	123				
0.2	0.200	0.223	0.023	880	0.0 %	880				
2.5	2.500	2.470	-0.030	8698	0.0 %	8698				
5.0	5.000	4.957	-0.043	17348	0.0 %	17348				
7.5	7.500	7.566	0.066	26424	0.0 %	26424				
10.0	10.000	9.978	-0.022	34811	0.0 %	34811				

LB89461 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Aug 2017 16:39:52

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	90	123	-	0.0000	7470A	PPB	14 Aug 2017 16:42:03	S	Std
0.2 - 1	50.2	880	-	0.2000	7470A	PPB	14 Aug 2017 16:44:12	S	Std
2.5 - 1	22.5	8698	-	2.5000	7470A	PPB	14 Aug 2017 16:46:20	S	Std
5.0 - 1	55	17348	-	5.0000	7470A	PPB	14 Aug 2017 16:48:28	S	Std
7.5 - 1	57.5	26424	-	7.5000	7470A	PPB	14 Aug 2017 16:55:54	S	Std
10.0 - 1	510	34811	-	10.0000	7470A	PPB	14 Aug 2017 16:58:01	S	Std
ICV11 - 1	ICV11	13685	3.9042	-	7470A	PPB	14 Aug 2017 17:00:38	U	SMPL
ICB11 - 1	ICB11	-15	-0.0344	-	7470A	PPB	14 Aug 2017 17:02:45	U	SMPL
CCV63 - 1	CCV63	17169	4.9058	-	7470A	PPB	14 Aug 2017 17:04:51	U	SMPL
CCB63 - 1	CCB63	-8	-0.0324	-	7470A	PPB	14 Aug 2017 17:06:58	U	SMPL
CRA - 1	CRA	831	0.2088	-	7470A	PPB	14 Aug 2017 17:11:30	U	SMPL
HighStd - 1	HighStd	35181	10.0840	-	7470A	PPB	14 Aug 2017 17:13:36	U	SMPL
ChkStd - 1	ChkStd	24392	6.9823	-	7470A	PPB	14 Aug 2017 17:15:43	U	SMPL
PB101532BL - 1	PBW	-32	-0.0393	-	7470A	PPB	14 Aug 2017 17:17:52	U	SMPL
PB101532BS - 1	LCSW	13409	3.8248	-	7470A	PPB	14 Aug 2017 17:20:01	U	SMPL
I4349-05 - 1	0511B	24534	7.0231	-	7470A	PPB	14 Aug 2017 17:28:35	U	SMPL
CCV64 - 1	CCV64	16975	4.8500	-	7470A	PPB	14 Aug 2017 17:32:50	U	SMPL
CCB64 - 1	CCB64	-13	-0.0338	-	7470A	PPB	14 Aug 2017 17:34:58	U	SMPL