


7471A

LB 89522
INSTRUMENT ID: CV1

Linear

 μ Abs.:

40442

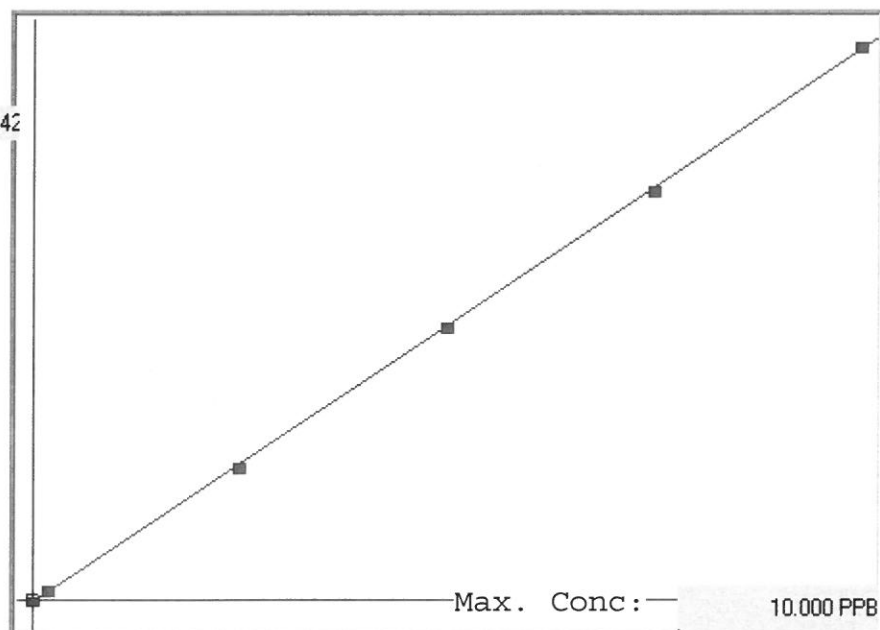

A= 0.0000e+000

B= 2.4721e-004

C= 4.9203e-002

Rho= 0.9999570

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.015	0.015	-140	0.000	-140				
0.2	0.200	0.233	0.033	745	0.0 %	745				
2.5	2.500	2.461	-0.039	9756	0.0 %	9756				
5.0	5.000	4.987	-0.013	19972	0.0 %	19972				
7.5	7.500	7.458	-0.042	29968	0.0 %	29968	0			
10.0	10.000	10.047	0.047	40442	0.0 %	40442				

LB89522 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 16 Aug 2017 12:22:09

Sample ID	Extended ID	µ Abs	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	-140	-	0.0007471A	PPB	16 Aug 2017 12:28:57	S	Std
0.2 - 1	50.2	745	-	0.20007471A	PPB	16 Aug 2017 12:31:15	S	Std
2.5 - 1	52.5	9756	-	2.50007471A	PPB	16 Aug 2017 12:33:32	S	Std
5.0 - 1	55	19972	-	5.00007471A	PPB	16 Aug 2017 12:35:50	S	Std
7.5 - 1	57.5	29968	-	7.50007471A	PPB	16 Aug 2017 12:38:07	S	Std
10.0 - 1	510	40442	-	10.00007471A	PPB	16 Aug 2017 12:40:24	S	Std
ICV15 - 1	ICV15	14873	3.7260	-7471A	PPB	16 Aug 2017 12:43:14	U	SMPL
ICB15 - 1	ICB15	-398	-0.0492	-7471A	PPB	16 Aug 2017 12:45:30	U	SMPL
CCV85 - 1	CCV85	18464	4.6137	-7471A	PPB	16 Aug 2017 12:47:46	U	SMPL
CCB85 - 1	CCB85	-416	-0.0536	-7471A	PPB	16 Aug 2017 12:50:02	U	SMPL
CRA - 1	CRA	505	0.1740	-7471A	PPB	16 Aug 2017 12:52:18	U	SMPL
HighStd - 1	HighStd	41087	10.2064	-7471A	PPB	16 Aug 2017 12:54:33	U	SMPL
ChkStd - 1	ChkStd	27267	6.7899	-7471A	PPB	16 Aug 2017 12:56:49	U	SMPL
PB101574BL - 1	PBS	-256	-0.0141	-7471A	PPB	16 Aug 2017 12:59:07	U	SMPL
PB101574BS - 1	LCSS	14540	3.6437	-7471A	PPB	16 Aug 2017 13:01:26	U	SMPL
I4659-02 - 1	WC-1	4907	1.2623	-7471A	PPB	16 Aug 2017 13:03:43	U	SMPL
I4799-01 - 1	AU-05-081417-A	2054	0.5570	-7471A	PPB	16 Aug 2017 13:06:00	U	SMPL
I4799-04 - 1	AU-05-081417-B	860	0.2618	-7471A	PPB	16 Aug 2017 13:08:18	U	SMPL
I4808-01 - 1	SASP2P-TP106-I(0-5)COMP	5008	1.2872	-7471A	PPB	16 Aug 2017 13:10:36	U	SMPL
I4808-03 - 1	SASP-TP106-K(0-5)COMP	571	0.1904	-7471A	PPB	16 Aug 2017 13:12:52	U	SMPL
CCV86 - 1	CCV86	18942	4.7319	-7471A	PPB	16 Aug 2017 13:15:08	U	SMPL
CCB86 - 1	CCB86	-373	-0.0430	-7471A	PPB	16 Aug 2017 13:17:23	U	SMPL
I4811-01 - 1	EP-12	4339	1.1219	-7471A	PPB	16 Aug 2017 13:19:40	U	SMPL
I4811-02 - 1	EP-18	910	0.2742	-7471A	PPB	16 Aug 2017 13:21:56	U	SMPL
I4811-03 - 1	EP-23	300	0.1234	-7471A	PPB	16 Aug 2017 13:24:12	U	SMPL
I4811-04 - 1	E4-24	176	0.0927	-7471A	PPB	16 Aug 2017 13:26:28	U	SMPL
I4811-04DUP - 1	E4-24DUP	190	0.0962	-7471A	PPB	16 Aug 2017 13:28:45	U	SMPL
I4811-05 - 1	I4811-04MS	15624	3.9116	-7471A	PPB	16 Aug 2017 13:31:02	U	SMPL
I4811-06 - 1	I4811-04MSD	15360	3.8464	-7471A	PPB	16 Aug 2017 13:33:19	U	SMPL
I4811-07 - 1	DUP	49040	12.1724	-7471A	PPB	16 Aug 2017 13:40:13	U	SMPL
I4814-01 - 1	WHITE-TWP-COMPOST	2254	0.6064	-7471A	PPB	16 Aug 2017 13:42:30	U	SMPL
I4815-01 - 1	TR-05-081517-A	7271	1.8467	-7471A	PPB	16 Aug 2017 13:44:48	U	SMPL
CCV87 - 1	CCV87	19239	4.8053	-7471A	PPB	16 Aug 2017 13:47:05	U	SMPL
CCB87 - 1	CCB87	-324	-0.0309	-7471A	PPB	16 Aug 2017 13:49:21	U	SMPL
I4815-04 - 1	TR-05-081517-B	9793	2.4701	-7471A	PPB	16 Aug 2017 13:51:38	U	SMPL
I4817-01 - 1	SU-03-081517	861	0.2621	-7471A	PPB	16 Aug 2017 13:53:54	U	SMPL
I4818-01 - 1	3-4-CLEAN-DENSEGRADE	119	0.0786	-7471A	PPB	16 Aug 2017 13:56:11	U	SMPL
I4819-01 - 1	1-1-2-DENSE-GRADE	2265	0.6091	-7471A	PPB	16 Aug 2017 13:58:27	U	SMPL
I4821-01 - 1	FK-GF-02-009-A	1274	0.3641	-7471A	PPB	16 Aug 2017 14:00:44	U	SMPL
I4821-03 - 1	FK-GF-02-009-B	1512	0.4230	-7471A	PPB	16 Aug 2017 14:03:01	U	SMPL
I4825-01 - 1	TP-A-B-COMP	16400	4.1035	-7471A	PPB	16 Aug 2017 14:05:18	U	SMPL
PB101575BL - 1	PBS	-198	0.0003	-7471A	PPB	16 Aug 2017 14:07:35	U	SMPL
PB101575BS - 1	LCSS	14578	3.6530	-7471A	PPB	16 Aug 2017 14:09:53	U	SMPL
I4820-01 - 1	E2-I10-ESW	131869	32.6487	-7471A	PPB	16 Aug 2017 14:12:10	U	SMPL
CCV88 - 1	CCV88	18485	4.6189	-7471A	PPB	16 Aug 2017 14:14:26	U	SMPL
CCB88 - 1	CCB88	-411	-0.0524	-7471A	PPB	16 Aug 2017 14:16:45	U	SMPL
I4820-01DUP - 1	E2-I10-ESWDUP	129317	32.0178	-7471A	PPB	16 Aug 2017 14:19:02	U	SMPL
I4820-02 - 1	I4820-01MS	140161	34.6986	-7471A	PPB	16 Aug 2017 14:21:19	U	SMPL
I4820-03 - 1	I4820-01MSD	148373	36.7286	-7471A	PPB	16 Aug 2017 14:26:21	U	SMPL
I4820-04 - 1	E2-I10-ESW-DUP	248139	61.3919	-7471A	PPB	16 Aug 2017 14:28:40	U	SMPL
I4820-05 - 1	E2-I10-BASE	105164	26.0469	-7471A	PPB	16 Aug 2017 14:31:03	U	SMPL
I4820-06 - 1	E2-I8-WSW	92436	22.9004	-7471A	PPB	16 Aug 2017 14:33:39	U	SMPL
I4820-07 - 1	E2-I8-BASE	116098	28.7499	-7471A	PPB	16 Aug 2017 14:35:59	U	SMPL
I4820-08 - 1	E2-I8-BASE	8551	2.1631	-7471A	PPB	16 Aug 2017 14:38:19	U	SMPL
I4820-09 - 1	E2-I8-WSW	47503	11.7925	-7471A	PPB	16 Aug 2017 14:40:39	U	SMPL
I4820-10 - 1	E2-I9-BASE	7258	1.8435	-7471A	PPB	16 Aug 2017 14:42:56	U	SMPL
CCV89 - 1	CCV89	19099	4.7707	-7471A	PPB	16 Aug 2017 14:45:14	U	SMPL
CCB89 - 1	CCB89	-387	-0.0465	-7471A	PPB	16 Aug 2017 14:47:30	U	SMPL
I4820-11 - 1	E2-K7-BASE	19110	4.7734	-7471A	PPB	16 Aug 2017 14:49:47	U	SMPL
I4820-12 - 1	E2-K8-BASE	18780	4.6918	-7471A	PPB	16 Aug 2017 14:52:03	U	SMPL
I4820-13 - 1	E2-J8-BASE	114836	28.4379	-7471A	PPB	16 Aug 2017 14:54:21	U	SMPL
I4820-14 - 1	E2-J7-BASE	3735	0.9725	-7471A	PPB	16 Aug 2017 14:56:38	U	SMPL
I4820-15 - 1	E2-J7-WSW	5106	1.3115	-7471A	PPB	16 Aug 2017 14:58:57	U	SMPL
I4820-16 - 1	E2-K6-WSW	7176	1.8232	-7471A	PPB	16 Aug 2017 15:01:14	U	SMPL
I4811-04LX5 - 1		-246	-0.0116	-7471A	PPB	16 Aug 2017 15:03:31	U	SMPL
I4811-04A - 1		17000	4.2518	-7471A	PPB	16 Aug 2017 15:05:49	U	SMPL
I4820-01LX5 - 1		24512	6.1088	-7471A	PPB	16 Aug 2017 15:08:06	U	SMPL
I4820-01A - 1		144672	35.8137	-7471A	PPB	16 Aug 2017 15:10:23	U	SMPL
CCV90 - 1	CCV90	18582	4.6429	-7471A	PPB	16 Aug 2017 15:12:41	U	SMPL
CCB90 - 1	CCB90	-440	-0.0596	-7471A	PPB	16 Aug 2017 15:15:02	U	SMPL
I4811-07DLX2 - 1		26684	6.6458	-7471A	PPB	16 Aug 2017 15:17:20	U	SMPL
I4820-01DLX10 - 1		12349	3.1020	-7471A	PPB	16 Aug 2017 15:29:21	U	SMPL
I4820-01DUPDLX10 - 1		11698	2.9411	-7471A	PPB	16 Aug 2017 15:31:38	U	SMPL
I4820-02DLX10 - 1		14255	3.5732	-7471A	PPB	16 Aug 2017 15:33:55	U	SMPL
I4820-03DLX10 - 1		14809	3.7102	-7471A	PPB	16 Aug 2017 15:36:12	U	SMPL
I4820-01LDLX50 - 1		2110	0.5708	-7471A	PPB	16 Aug 2017 15:38:29	U	SMPL
I4820-01ADLX10 - 1		14327	3.5910	-7471A	PPB	16 Aug 2017 15:40:46	U	SMPL
I4820-04DLX10 - 1		25226	6.2853	-7471A	PPB	16 Aug 2017 15:43:04	U	SMPL
I4820-05DLX5 - 1		20075	5.0120	-7471A	PPB	16 Aug 2017 15:45:22	U	SMPL
I4820-06DLX5 - 1		17677	4.4192	-7471A	PPB	16 Aug 2017 15:47:40	U	SMPL
CCV91 - 1	CCV91	18904	4.7225	-7471A	PPB	16 Aug 2017 15:49:57	U	SMPL
CCB91 - 1	CCB91	-343	-0.0356	-7471A	PPB	16 Aug 2017 15:52:14	U	SMPL
I4820-07DLX5 - 1		22584	5.6322	-7471A	PPB	16 Aug 2017 15:54:31	U	SMPL
I4820-09DLX2 - 1		23489	5.8559	-7471A	PPB	16 Aug 2017 15:56:48	U	SMPL
I4820-13DLX5 - 1		22887	5.7071	-7471A	PPB	16 Aug 2017 16:12:52	U	SMPL
CCV92 - 1	CCV92	19046	4.7576	-7471A	PPB	16 Aug 2017 16:15:09	U	SMPL
CCB92 - 1	CCB92	-350	-0.0373	-7471A	PPB	16 Aug 2017 16:17:26	U	SMPL