

7470A


LB89587

INSTRUMENT ID: CV2

Linear

 μ Abs.:

34519

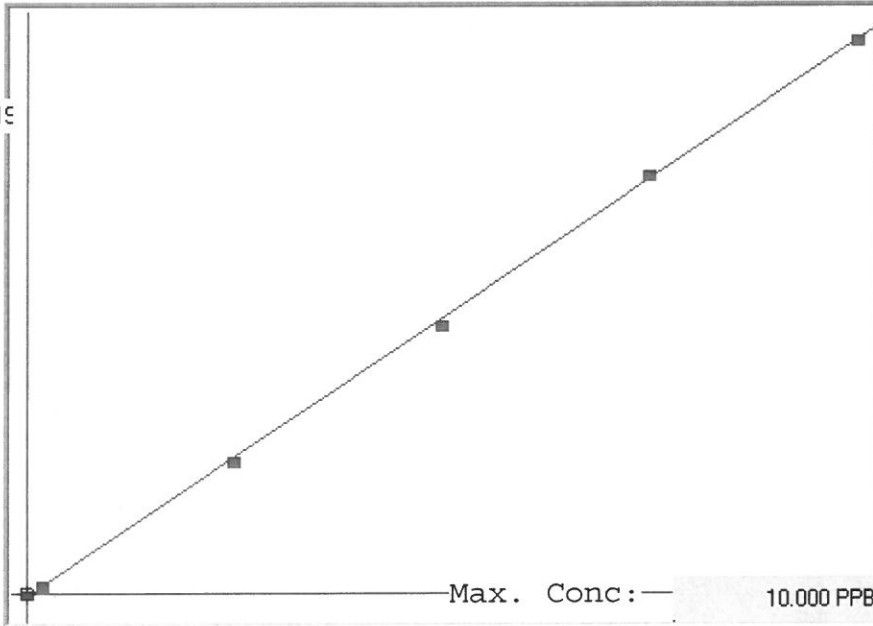

A= 0.0000e+000

B= 2.8777e-004

C= 6.1160e-002

Rho= 0.9998800

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.029	0.029	-113	0.000	-113				
0.2	0.200	0.232	0.032	595	0.0 %	595				
2.5	2.500	2.459	-0.041	8334	0.0 %	8334				
5.0	5.000	4.903	-0.097	16826	0.0 %	16826				
7.5	7.500	7.582	0.082	26134	0.0 %	26134				
10.0	10.000	9.995	-0.005	34519	0.0 %	34519				

LB89587 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 18 Aug 2017 10:58:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-113	-	0.0000	7470A	PPB	18 Aug 2017 11:13:11	S	Std
0.2 - 1	50.2	595	-	0.2000	7470A	PPB	18 Aug 2017 11:15:19	S	Std
2.5 - 1	52.5	8334	-	2.5000	7470A	PPB	18 Aug 2017 11:17:28	S	Std
5.0 - 1	55	16826	-	5.0000	7470A	PPB	18 Aug 2017 11:19:36	S	Std
7.5 - 1	57.5	26134	-	7.5000	7470A	PPB	18 Aug 2017 11:21:44	S	Std
10.0 - 1	510	34519	-	10.0000	7470A	PPB	18 Aug 2017 11:26:26	S	Std
ICV18 - 1	ICV18	13242	3.8718	-	7470A	PPB	18 Aug 2017 11:28:56	U	SMPL
ICB18 - 1	ICB18	-308	-0.0275	-	7470A	PPB	18 Aug 2017 11:31:03	U	SMPL
CCV06 - 1	CCV06	17059	4.9702	-	7470A	PPB	18 Aug 2017 11:33:10	U	SMPL
CCB06 - 1	CCB06	-310	-0.0280	-	7470A	PPB	18 Aug 2017 11:35:17	U	SMPL
CRA - 1	CRA	576	0.2269	-	7470A	PPB	18 Aug 2017 11:37:25	U	SMPL
HighStd - 1	HighStd	34551	10.0039	-	7470A	PPB	18 Aug 2017 11:39:31	U	SMPL
ChkStd - 1	ChkStd	24001	6.9679	-	7470A	PPB	18 Aug 2017 11:41:38	U	SMPL
PB101651BL - 1	PBW	-355	-0.0410	-	7470A	PPB	18 Aug 2017 11:43:47	U	SMPL
PB101651BS - 1	LCSW	13068	3.8217	-	7470A	PPB	18 Aug 2017 11:45:56	U	SMPL
PB101651TB - 1	PB101608TB	-278	-0.0188	-	7470A	PPB	18 Aug 2017 11:48:04	U	SMPL
I4844-03 - 1	OR-03-081617	-218	-0.0016	-	7470A	PPB	18 Aug 2017 11:50:12	U	SMPL
I4845-03 - 1	OK-03-81617	-185	0.0079	-	7470A	PPB	18 Aug 2017 11:52:20	U	SMPL
I4847-05 - 1	PVSC-A-COMP	-185	0.0079	-	7470A	PPB	18 Aug 2017 11:54:28	U	SMPL
I4847-10 - 1	PVSC-B-COMP	-166	0.0134	-	7470A	PPB	18 Aug 2017 11:56:35	U	SMPL
CCV07 - 1	CCV07	16853	4.9109	-	7470A	PPB	18 Aug 2017 11:58:42	U	SMPL
CCB07 - 1	CCB07	-292	-0.0229	-	7470A	PPB	18 Aug 2017 12:00:49	U	SMPL
I4848-02 - 1	A2882	-186	0.0076	-	7470A	PPB	18 Aug 2017 12:02:56	U	SMPL
I4852-03 - 1	VNJ-207	-197	0.0045	-	7470A	PPB	18 Aug 2017 12:05:03	U	SMPL
I4852-06 - 1	VNJ-242	-181	0.0091	-	7470A	PPB	18 Aug 2017 12:07:09	U	SMPL
I4853-02 - 1	LX-1	-179	0.0096	-	7470A	PPB	18 Aug 2017 12:09:16	U	SMPL
I4853-04 - 1	LX-2	-181	0.0091	-	7470A	PPB	18 Aug 2017 12:11:24	U	SMPL
I4853-04DUP - 1	LX-2DUP	-205	0.0022	-	7470A	PPB	18 Aug 2017 12:13:32	U	SMPL
I4853-04MS - 1	LX-2MS	13079	3.8249	-	7470A	PPB	18 Aug 2017 12:15:40	U	SMPL
I4853-04MSD - 1	LX-2MSD	11807	3.4589	-	7470A	PPB	18 Aug 2017 12:17:48	U	SMPL
PB101652BL - 1	PBW	-234	-0.0062	-	7470A	PPB	18 Aug 2017 12:19:57	U	SMPL
PB101652BS - 1	LCSW	13297	3.8876	-	7470A	PPB	18 Aug 2017 12:22:04	U	SMPL
CCV08 - 1	CCV08	16918	4.9296	-	7470A	PPB	18 Aug 2017 12:24:11	U	SMPL
CCB08 - 1	CCB08	-289	-0.0220	-	7470A	PPB	18 Aug 2017 12:26:18	U	SMPL
I4820-17 - 1	E2-FB-8-15-17	-385	-0.0496	-	7470A	PPB	18 Aug 2017 12:28:25	U	SMPL
I4848-01 - 1	A2882	-121	0.0263	-	7470A	PPB	18 Aug 2017 12:30:32	U	SMPL
I4848-01DUP - 1	A2882DUP	-108	0.0301	-	7470A	PPB	18 Aug 2017 12:32:39	U	SMPL
I4848-01MS - 1	A2882MS	11175	3.2770	-	7470A	PPB	18 Aug 2017 12:34:46	U	SMPL
I4848-01MSD - 1	A2882MSD	10874	3.1904	-	7470A	PPB	18 Aug 2017 12:36:54	U	SMPL
I4853-04LX5 - 1		-256	-0.0125	-	7470A	PPB	18 Aug 2017 12:39:02	U	SMPL
I4853-04A - 1		14017	4.0948	-	7470A	PPB	18 Aug 2017 12:41:11	U	SMPL
I4848-01LX5 - 1		-253	-0.0116	-	7470A	PPB	18 Aug 2017 12:43:19	U	SMPL
I4848-01A - 1		11515	3.3748	-	7470A	PPB	18 Aug 2017 12:45:28	U	SMPL
CCV09 - 1	CCV09	17108	4.9843	-	7470A	PPB	18 Aug 2017 12:47:35	U	SMPL
CCB09 - 1	CCB09	-256	-0.0125	-	7470A	PPB	18 Aug 2017 12:49:43	U	SMPL