


7470A

L989638
INSTRUMENT ID: CV4

Linear

 μ Abs.:

33411

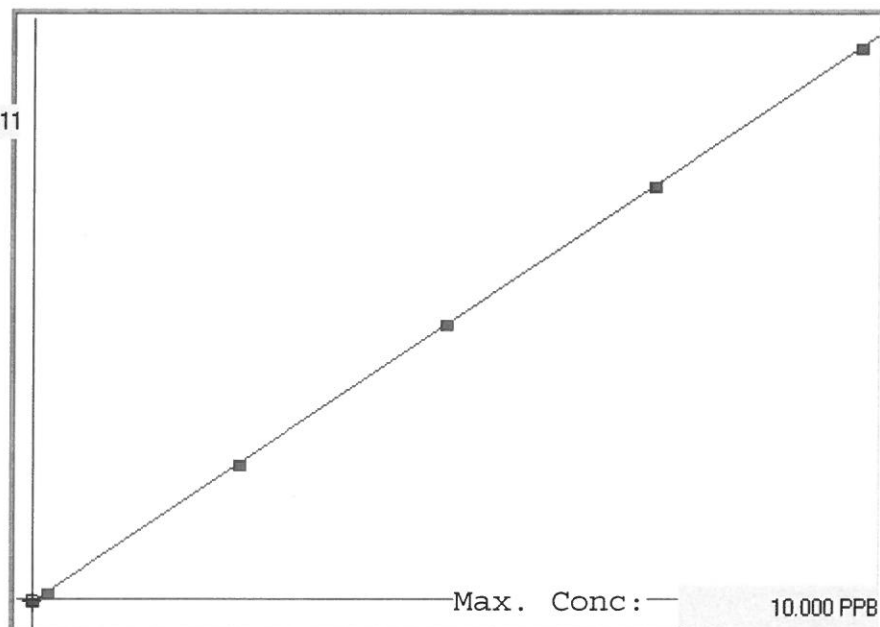

A= 0.0000e+000

B= 2.9727e-004

C= 6.0341e-002

Rho= 0.9999890

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	-187	0.000	-187				
0.2	0.200	0.193	-0.007	446	0.0 %	446				
2.5	2.500	2.482	-0.018	8146	0.0 %	8146				
5.0	5.000	5.036	0.036	16737	0.0 %	16737				
7.5	7.500	7.492	-0.008	25001	0.0 %	25001				
10.0	10.000	9.992	-0.008	33411	0.0 %	33411				

LB89638 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Aug 2017 09:36:54

Sample ID	Extended ID	µ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-187	-	0.00007470A	PPB	22 Aug 2017 09:44:43	S	Std
0.2 - 1	50.2	446	-	0.20007470A	PPB	22 Aug 2017 09:46:51	S	Std
2.5 - 1	52.5	8146	-	2.50007470A	PPB	22 Aug 2017 09:49:00	S	Std
5.0 - 1	55	16737	-	5.00007470A	PPB	22 Aug 2017 09:51:08	S	Std
7.5 - 1	57.5	25001	-	7.50007470A	PPB	22 Aug 2017 09:53:16	S	Std
10.0 - 1	57.5	33411	-	10.00007470A	PPB	22 Aug 2017 09:55:23	S	Std
ICV23 - 1	ICV23	12878	3.8886	-7470A	PPB	22 Aug 2017 09:58:01	U	SMPL
ICB23 - 1	ICB23	-202	0.0003	-7470A	PPB	22 Aug 2017 10:00:07	U	SMPL
CCV25 - 1	CCV25	16296	4.9046	-7470A	PPB	22 Aug 2017 10:02:14	U	SMPL
CCB25 - 1	CCB25	-298	-0.0282	-7470A	PPB	22 Aug 2017 10:04:21	U	SMPL
CRA - 1	CRA	452	0.1947	-7470A	PPB	22 Aug 2017 10:06:28	U	SMPL
HighStd - 1	HighStd	33049	9.8848	-7470A	PPB	22 Aug 2017 10:08:35	U	SMPL
ChkStd - 1	ChkStd	24111	7.2278	-7470A	PPB	22 Aug 2017 10:10:41	U	SMPL
PB101729BL - 1	PBW	-469	-0.0791	-7470A	PPB	22 Aug 2017 10:12:50	U	SMPL
PB101729BS - 1	LCSW	13131	3.9638	-7470A	PPB	22 Aug 2017 10:14:59	U	SMPL
PB101729TB - 1	PB101682TB	-158	0.0134	-7470A	PPB	22 Aug 2017 10:17:07	U	SMPL
I4869-05 - 1	SASP2P-TP-106-A(0-5)COMP	56	0.0770	-7470A	PPB	22 Aug 2017 10:19:15	U	SMPL
I4869-06 - 1	SASP2P-TP-106-B(0-5)COMP	-116	0.0259	-7470A	PPB	22 Aug 2017 10:21:23	U	SMPL
I4872-21 - 1	SB-07-COMP	-313	-0.0327	-7470A	PPB	22 Aug 2017 10:23:32	U	SMPL
I4872-22 - 1	SB-04-COMP	-266	-0.0187	-7470A	PPB	22 Aug 2017 10:25:38	U	SMPL
CCV26 - 1	CCV26	16720	5.0307	-7470A	PPB	22 Aug 2017 10:27:45	U	SMPL
CCB26 - 1	CCB26	-236	-0.0098	-7470A	PPB	22 Aug 2017 10:29:52	U	SMPL
I4872-23 - 1	SB-08-COMP	-331	-0.0381	-7470A	PPB	22 Aug 2017 10:31:59	U	SMPL
I4872-24 - 1	SB-11-COMP	-322	-0.0354	-7470A	PPB	22 Aug 2017 10:34:06	U	SMPL
I4872-25 - 1	SB-12-COMP	-226	-0.0068	-7470A	PPB	22 Aug 2017 10:36:13	U	SMPL
I4872-26 - 1	SB-13-COMP	-300	-0.0288	-7470A	PPB	22 Aug 2017 10:38:20	U	SMPL
I4872-27 - 1	SB-14-COMP	-308	-0.0312	-7470A	PPB	22 Aug 2017 10:40:28	U	SMPL
I4872-28 - 1	SB-15-COMP	-277	-0.0220	-7470A	PPB	22 Aug 2017 10:42:35	U	SMPL
I4872-29 - 1	SB-20-COMP	-273	-0.0208	-7470A	PPB	22 Aug 2017 10:44:44	U	SMPL
I4872-30 - 1	SB-31-COMP	-277	-0.0220	-7470A	PPB	22 Aug 2017 10:46:52	U	SMPL
I4889-05 - 1	SASP2P-TP-106-L(0-5)COMP	-269	-0.0196	-7470A	PPB	22 Aug 2017 10:49:01	U	SMPL
I4892-03 - 1	HR-06-081817	-245	-0.0125	-7470A	PPB	22 Aug 2017 10:51:07	U	SMPL
CCV27 - 1	CCV27	16647	5.0090	-7470A	PPB	22 Aug 2017 10:53:14	U	SMPL
CCB27 - 1	CCB27	-143	0.0178	-7470A	PPB	22 Aug 2017 10:55:21	U	SMPL
I4898-03 - 1	NB-08-081817-A	-186	0.0050	-7470A	PPB	22 Aug 2017 10:57:28	U	SMPL
I4898-06 - 1	NB-08-081817-B	-35	0.0499	-7470A	PPB	22 Aug 2017 10:59:35	U	SMPL
I4898-06DUP - 1	NB-08-081817-BDUP	-17	0.0553	-7470A	PPB	22 Aug 2017 11:01:42	U	SMPL
I4898-06MS - 1	NB-08-081817-BMS	13070	3.9456	-7470A	PPB	22 Aug 2017 11:03:49	U	SMPL
I4898-06MSD - 1	NB-08-081817-BMSD	12991	3.9222	-7470A	PPB	22 Aug 2017 11:05:56	U	SMPL
PB101730BL - 1	PBW	-146	0.0169	-7470A	PPB	22 Aug 2017 11:08:03	U	SMPL
PB101730BS - 1	LCSW	12721	3.8419	-7470A	PPB	22 Aug 2017 11:10:12	U	SMPL
PB101730TB - 1	PB101692TB	-265	-0.0184	-7470A	PPB	22 Aug 2017 11:12:20	U	SMPL
I4900-02 - 1	CONTROL-HOUSE-RAMP	-203	-0.0000	-7470A	PPB	22 Aug 2017 11:14:29	U	SMPL
I4900-04 - 1	CONTROL-HOUSE-STAIR	-36	0.0496	-7470A	PPB	22 Aug 2017 11:16:36	U	SMPL
CCV28 - 1	CCV28	16777	5.0476	-7470A	PPB	22 Aug 2017 11:18:43	U	SMPL
CCB28 - 1	CCB28	-265	-0.0184	-7470A	PPB	22 Aug 2017 11:20:50	U	SMPL
I4900-06 - 1	CONTROL-LOADING-DOCK	-49	0.0458	-7470A	PPB	22 Aug 2017 11:22:58	U	SMPL
I4900-08 - 1	220-1-WALL	-71	0.0392	-7470A	PPB	22 Aug 2017 11:25:05	U	SMPL
I4900-10 - 1	220-1-CONCRETE	-81	0.0363	-7470A	PPB	22 Aug 2017 11:27:12	U	SMPL
I4900-12 - 1	DEADMEN	22	0.0669	-7470A	PPB	22 Aug 2017 11:29:19	U	SMPL
I4900-14 - 1	TRENWA	68	0.0806	-7470A	PPB	22 Aug 2017 11:31:27	U	SMPL
I4900-16 - 1	220-1-STONE	60	0.0782	-7470A	PPB	22 Aug 2017 11:33:35	U	SMPL
I4900-18 - 1	220-2-STONE	77	0.0832	-7470A	PPB	22 Aug 2017 11:35:43	U	SMPL
I4900-20 - 1	220-2-CONCRETE	72	0.0817	-7470A	PPB	22 Aug 2017 11:37:51	U	SMPL
I4900-22 - 1	PUMP-HOUSE	-2	0.0597	-7470A	PPB	22 Aug 2017 11:40:00	U	SMPL
I4900-22DUP - 1	PUMP-HOUSEDUP	-53	0.0446	-7470A	PPB	22 Aug 2017 11:42:07	U	SMPL
CCV29 - 1	CCV29	16722	5.0313	-7470A	PPB	22 Aug 2017 11:44:14	U	SMPL
CCB29 - 1	CCB29	-179	0.0071	-7470A	PPB	22 Aug 2017 11:46:21	U	SMPL
I4900-22MS - 1	PUMP-HOUSEMS	13136	3.9653	-7470A	PPB	22 Aug 2017 11:48:29	U	SMPL
I4900-22MSD - 1	PUMP-HOUSEMSD	12650	3.8208	-7470A	PPB	22 Aug 2017 11:50:36	U	SMPL
I4898-06LX5 - 1		-158	0.0134	-7470A	PPB	22 Aug 2017 11:52:43	U	SMPL
I4898-06A - 1		14279	4.3050	-7470A	PPB	22 Aug 2017 11:54:51	U	SMPL
I4900-22LX5 - 1		-151	0.0155	-7470A	PPB	22 Aug 2017 11:56:58	U	SMPL
I4900-22A - 1		14067	4.2420	-7470A	PPB	22 Aug 2017 11:59:07	U	SMPL
CCV30 - 1	CCV30	16866	5.0741	-7470A	PPB	22 Aug 2017 12:01:15	U	SMPL
CCB30 - 1	CCB30	-210	-0.0021	-7470A	PPB	22 Aug 2017 12:03:23	U	SMPL