


7471A

LB 89652
INSTRUMENT ID 1.CV1

Linear

 μ Abs.:

40471

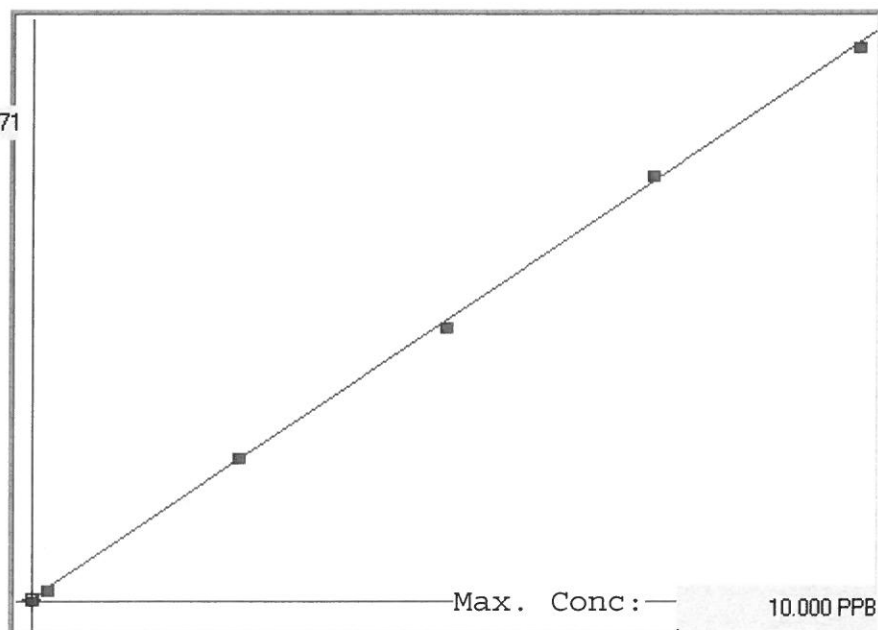

A= 0.0000e+000

B= 2.4646e-004

C= -4.4882e-002

Rho= 0.9997612

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.003	0.003	193	0.000	193				
0.2	0.200	0.173	-0.027	886	0.0 %	886				
2.5	2.500	2.559	0.059	10565	0.0 %	10565				
5.0	5.000	4.897	-0.103	20050	0.0 %	20050				
7.5	7.500	7.639	0.139	31175	0.0 %	31175	0			
10.0	10.000	9.930	-0.070	40471	0.0 %	40471				

LB89652 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 22 Aug 2017 16:20:45

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	193	-	0.00007471A	PPB		22 Aug 2017 16:26:34	S	Std
0.2 - 1	50.2	886	-	0.20007471A	PPB		22 Aug 2017 16:28:52	S	Std
2.5 - 1	52.5	10565	-	2.50007471A	PPB		22 Aug 2017 16:31:09	S	Std
5.0 - 1	55	20050	-	5.00007471A	PPB		22 Aug 2017 16:33:27	S	Std
7.5 - 1	57.5	31175	-	7.50007471A	PPB		22 Aug 2017 16:35:44	S	Std
10.0 - 1	50	40471	-	10.00007471A	PPB		22 Aug 2017 16:38:01	S	Std
ICV24 - 1	ICV24	15702	3.8251	-7471A	PPB		22 Aug 2017 16:40:52	U	SMPL
ICB24 - 1	ICB24	32	-0.0370	-7471A	PPB		22 Aug 2017 16:43:07	U	SMPL
CCV31 - 1	CCV31	20156	4.9228	-7471A	PPB		22 Aug 2017 16:45:24	U	SMPL
CCB31 - 1	CCB31	33	-0.0367	-7471A	PPB		22 Aug 2017 16:47:40	U	SMPL
CRA - 1	CRA	842	0.1626	-7471A	PPB		22 Aug 2017 16:49:57	U	SMPL
HighStd - 1	HighStd	40816	10.0147	-7471A	PPB		22 Aug 2017 16:52:13	U	SMPL
ChkStd - 1	ChkStd	28858	7.0675	-7471A	PPB		22 Aug 2017 16:54:29	U	SMPL
PB101734BL - 1	PBS	-92	-0.0676	-7471A	PPB		22 Aug 2017 16:56:47	U	SMPL
PB101734BS - 1	LCSS	13916	3.3849	-7471A	PPB		22 Aug 2017 16:59:05	U	SMPL
I4901-01 - 1	TEC-BE1-1-3-COMP	28697	7.0278	-7471A	PPB		22 Aug 2017 17:01:22	U	SMPL
I4901-03 - 1	TEC-BE1-3-12-COMP	1306	0.2770	-7471A	PPB		22 Aug 2017 17:03:39	U	SMPL
I4908-01 - 1	TR-04-082117-A	3262	0.7591	-7471A	PPB		22 Aug 2017 17:05:58	U	SMPL
I4908-04 - 1	TR-04-082117-B	65655	16.1365	-7471A	PPB		22 Aug 2017 17:08:16	U	SMPL
I4909-01 - 1	SU-04-082117	2451	0.5592	-7471A	PPB		22 Aug 2017 17:10:32	U	SMPL
CCV32 - 1	CCV32	19930	4.8671	-7471A	PPB		22 Aug 2017 17:12:51	U	SMPL
CCB32 - 1	CCB32	8	-0.0429	-7471A	PPB		22 Aug 2017 17:15:07	U	SMPL
I4912-01 - 1	FENCE-POSTS-PILED-COMP	396	0.0527	-7471A	PPB		22 Aug 2017 17:17:22	U	SMPL
I4913-01 - 1	TEC-BE2-1-3-COMP	26937	6.5940	-7471A	PPB		22 Aug 2017 17:19:38	U	SMPL
I4913-02 - 1	TEC-BE2-3-12-COMP	2048	0.4599	-7471A	PPB		22 Aug 2017 17:21:55	U	SMPL
I4914-01 - 1	289-COMP	2881	0.6652	-7471A	PPB		22 Aug 2017 17:24:11	U	SMPL
I4914-04 - 1	165-COMP	3440	0.8029	-7471A	PPB		22 Aug 2017 17:26:28	U	SMPL
I4914-04DUP - 1	165-COMPDUP	3152	0.7320	-7471A	PPB		22 Aug 2017 17:28:45	U	SMPL
I4914-04MS - 1	165-COMPMS	19520	4.7660	-7471A	PPB		22 Aug 2017 17:31:02	U	SMPL
I4914-04MSD - 1	165-COMPMSD	19138	4.6719	-7471A	PPB		22 Aug 2017 17:33:19	U	SMPL
I4915-01 - 1	72-11991-GRAVEL-COMP	1377	0.2945	-7471A	PPB		22 Aug 2017 17:35:37	U	SMPL
I4915-04 - 1	72-11991-DEBRIS-COMP	336	0.0379	-7471A	PPB		22 Aug 2017 17:37:53	U	SMPL
CCV33 - 1	CCV33	20238	4.9430	-7471A	PPB		22 Aug 2017 17:40:10	U	SMPL
CCB33 - 1	CCB33	53	-0.0318	-7471A	PPB		22 Aug 2017 17:42:26	U	SMPL
I4914-04LX5 - 1		805	0.1535	-7471A	PPB		22 Aug 2017 17:44:42	U	SMPL
I4914-04A - 1		20127	4.9156	-7471A	PPB		22 Aug 2017 17:46:58	U	SMPL
I4908-04DLX5 - 1		12908	3.1364	-7471A	PPB		22 Aug 2017 17:49:14	U	SMPL
CCV34 - 1	CCV34	20083	4.9048	-7471A	PPB		22 Aug 2017 17:51:31	U	SMPL
CCB34 - 1	CCB34	59	-0.0303	-7471A	PPB		22 Aug 2017 17:53:48	U	SMPL