


7470A

LB 89766
INSTRUMENT ID: CV2

Linear

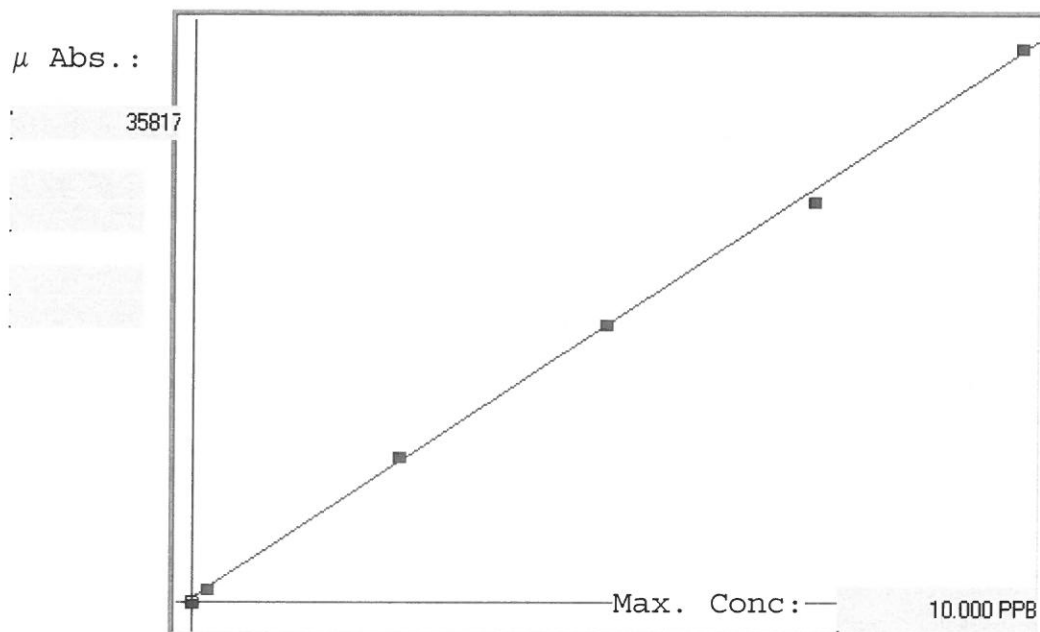

A= 0.0000e+000

B= 2.8356e-004

C= -6.6581e-002

Rho= 0.9995837

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.056	-0.056	36	0.000	36				
0.2	0.200	0.195	-0.005	924	0.0 %	924				
2.5	2.500	2.634	0.134	9523	0.0 %	9523				
5.0	5.000	5.032	0.032	17980	0.0 %	17980				
7.5	7.500	7.305	-0.195	25998	0.0 %	25998				
10.0	10.000	10.090	0.090	35817	0.0 %	35817				

LB89766 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 29 Aug 2017 11:45:01

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30	36	-	0.00007470A	PPB		29 Aug 2017 11:53:58	S	Std
0.2 - 1	30.2	924	-	0.20007470A	PPB		29 Aug 2017 11:56:06	S	Std
2.5 - 1	32.5	9523	-	2.50007470A	PPB		29 Aug 2017 11:58:15	S	Std
5.0 - 1	35	17980	-	5.00007470A	PPB		29 Aug 2017 12:00:23	S	Std
7.5 - 1	37.5	25998	-	7.50007470A	PPB		29 Aug 2017 12:02:31	S	Std
10.0 - 1	310	35817	-	10.00007470A	PPB		29 Aug 2017 12:04:37	S	Std
ICV33 - 1	ICV33	14170	3.9515	-7470A	PPB		29 Aug 2017 12:08:02	U	SMPL
ICB33 - 1	ICB33	-23	-0.0731	-7470A	PPB		29 Aug 2017 12:12:34	U	SMPL
CCV76 - 1	CCV76	17500	4.8958	-7470A	PPB		29 Aug 2017 12:14:41	U	SMPL
CCB76 - 1	CCB76	-91	-0.0924	-7470A	PPB		29 Aug 2017 12:19:11	U	SMPL
CRA - 1	CRA	936	0.1988	-7470A	PPB		29 Aug 2017 12:21:17	U	SMPL
HighStd - 1	HighStd	35309	9.9457	-7470A	PPB		29 Aug 2017 12:23:23	U	SMPL
ChkStd - 1	ChkStd	24738	6.9482	-7470A	PPB		29 Aug 2017 12:25:30	U	SMPL
PB101867BL - 1	PBW	-85	-0.0907	-7470A	PPB		29 Aug 2017 12:30:17	U	SMPL
PB101867BS - 1	LCSW	13515	3.7658	-7470A	PPB		29 Aug 2017 12:32:24	U	SMPL
PB101867TB - 1	PB101841TB	-139	-0.1060	-7470A	PPB		29 Aug 2017 12:34:31	U	SMPL
I4980-02 - 1	H26-WC1	-103	-0.0958	-7470A	PPB		29 Aug 2017 12:36:39	U	SMPL
I4981-02 - 1	S14-WC-01	-54	-0.0819	-7470A	PPB		29 Aug 2017 12:38:47	U	SMPL
I4985-02 - 1	WC-1	28	-0.0586	-7470A	PPB		29 Aug 2017 12:40:55	U	SMPL
I4986-03 - 1	SU-01-82517	-23	-0.0731	-7470A	PPB		29 Aug 2017 12:43:02	U	SMPL
CCV77 - 1	CCV77	17474	4.8884	-7470A	PPB		29 Aug 2017 12:45:09	U	SMPL
CCB77 - 1	CCB77	-84	-0.0904	-7470A	PPB		29 Aug 2017 12:47:15	U	SMPL
I4988-03 - 1	FF1-COMP	-77	-0.0884	-7470A	PPB		29 Aug 2017 12:49:23	U	SMPL
I4988-06 - 1	FF2-COMP	-185	-0.1190	-7470A	PPB		29 Aug 2017 12:51:29	U	SMPL
I4988-09 - 1	FF3-COMP	-218	-0.1284	-7470A	PPB		29 Aug 2017 12:53:36	U	SMPL
I4988-12 - 1	FF4-COMP	-107	-0.0969	-7470A	PPB		29 Aug 2017 12:55:43	U	SMPL
I4988-15 - 1	FF5-COMP	-138	-0.1057	-7470A	PPB		29 Aug 2017 12:57:50	U	SMPL
I4989-03 - 1	BERGEN-GEN-S1-COMP	-165	-0.1134	-7470A	PPB		29 Aug 2017 12:59:58	U	SMPL
I4989-06 - 1	BERGEN-GEN-S2-COMP	-121	-0.1009	-7470A	PPB		29 Aug 2017 13:02:06	U	SMPL
I4989-09 - 1	BERGEN-GEN-S3-COMP	-119	-0.1003	-7470A	PPB		29 Aug 2017 13:04:14	U	SMPL
I4989-12 - 1	BERGEN-GEN-S4-COMP	-107	-0.0969	-7470A	PPB		29 Aug 2017 13:06:22	U	SMPL
I4993-03 - 1	HR-05-082517	-95	-0.0935	-7470A	PPB		29 Aug 2017 13:08:29	U	SMPL
CCV78 - 1	CCV78	17456	4.8833	-7470A	PPB		29 Aug 2017 13:10:36	U	SMPL
CCB78 - 1	CCB78	-124	-0.1017	-7470A	PPB		29 Aug 2017 13:15:24	U	SMPL
I4994-03 - 1	EO-01-082517-A	-67	-0.0856	-7470A	PPB		29 Aug 2017 13:17:30	U	SMPL
I4994-06 - 1	EO-01-082517-B	1	-0.0663	-7470A	PPB		29 Aug 2017 13:21:31	U	SMPL
I4994-09 - 1	EO-01-082517-C	-17	-0.0714	-7470A	PPB		29 Aug 2017 13:23:38	U	SMPL
I4994-09DUP - 1	EO-01-082517-CDUP	-60	-0.0836	-7470A	PPB		29 Aug 2017 13:25:45	U	SMPL
I4994-09MS - 1	EO-01-082517-CMS	13370	3.7247	-7470A	PPB		29 Aug 2017 13:27:52	U	SMPL
I4994-09MSD - 1	EO-01-082517-CMSD	13274	3.6974	-7470A	PPB		29 Aug 2017 13:30:00	U	SMPL
PB101889BL - 1	PBW	-241	-0.1349	-7470A	PPB		29 Aug 2017 13:32:08	U	SMPL
PB101889BS - 1	LCSW	13700	3.8182	-7470A	PPB		29 Aug 2017 13:34:16	U	SMPL
I5001-06 - 1	MW-113	102	-0.0377	-7470A	PPB		29 Aug 2017 13:36:25	U	SMPL
I5001-06DUP - 1	MW-113DUP	-312	-0.1551	-7470A	PPB		29 Aug 2017 13:38:32	U	SMPL
CCV79 - 1	CCV79	17285	4.8348	-7470A	PPB		29 Aug 2017 13:40:39	U	SMPL
CCB79 - 1	CCB79	-77	-0.0884	-7470A	PPB		29 Aug 2017 13:42:46	U	SMPL
I5001-06MS - 1	MW-113MS	10769	2.9871	-7470A	PPB		29 Aug 2017 13:44:53	U	SMPL
I5001-06MSD - 1	MW-113MSD	10404	2.8836	-7470A	PPB		29 Aug 2017 13:47:00	U	SMPL
I5001-08 - 1	EB-2017-08-26	-278	-0.1454	-7470A	PPB		29 Aug 2017 13:51:20	U	SMPL
I5001-11 - 1	MW-113	-214	-0.1273	-7470A	PPB		29 Aug 2017 13:53:27	U	SMPL
I5001-12 - 1	MW-115	-240	-0.1346	-7470A	PPB		29 Aug 2017 13:55:35	U	SMPL
I4994-09LX5 - 1		93	-0.0402	-7470A	PPB		29 Aug 2017 13:57:43	U	SMPL
I4994-09A - 1		14480	4.0394	-7470A	PPB		29 Aug 2017 13:59:51	U	SMPL
I5001-06LX5 - 1		-118	-0.1000	-7470A	PPB		29 Aug 2017 14:02:00	U	SMPL
I5001-06A - 1		14314	3.9923	-7470A	PPB		29 Aug 2017 14:06:51	U	SMPL
I5001-07 - 1	MW-115	-138	-0.1057	-7470A	PPB		29 Aug 2017 14:11:23	U	SMPL
CCV80 - 1	CCV80	17925	5.0163	-7470A	PPB		29 Aug 2017 14:13:30	U	SMPL
CCB80 - 1	CCB80	-69	-0.0861	-7470A	PPB		29 Aug 2017 14:15:37	U	SMPL