


ISM02.4

LB 89794
INSTRUMENT ID: CV1

Linear

 μ Abs.:

41148

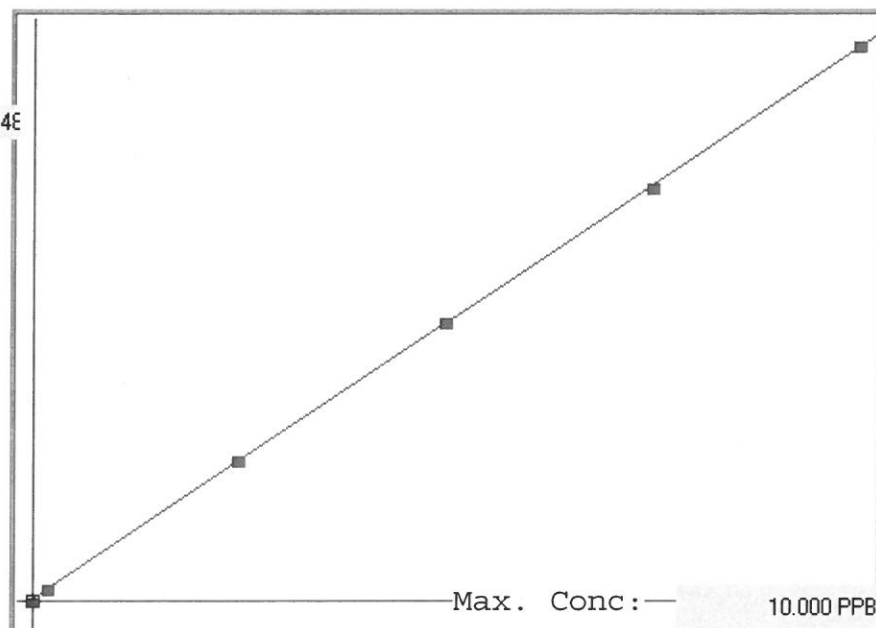

A= 0.0000e+000

B= 2.4404e-004

C= -2.6721e-002

Rho= 0.9999768

Accept=Accepted

slope
 $y = 1/m \times \text{except}$

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	O/D
0.00	0.000	-0.025	-0.025	9	0.000	9					-
0.2	0.200	0.204	0.004	944	0.0 %	944					2
2.5	2.500	2.533	0.033	10487	0.0 %	10487					1
5.0	5.000	5.014	0.014	20657	0.0 %	20657					0
7.5	7.500	7.459	-0.041	30674	0.0 %	30674					-1
10.0	10.000	10.015	0.015	41148	0.0 %	41148					0

ns
8/30/17

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	9	-		0 ISM02.4	PPB	8/30/2017 15:16	Std
	0.2 S0.2	944	-		0.2 ISM02.4	PPB	8/30/2017 15:19	Std
	2.5 S2.5	10487	-		2.5 ISM02.4	PPB	8/30/2017 15:21	Std
	5 S5	20657	-		5 ISM02.4	PPB	8/30/2017 15:23	Std
	7.5 S7.5	30674	-		7.5 ISM02.4	PPB	8/30/2017 15:26	Std
	10 S10	41148	-		10 ISM02.4	PPB	8/30/2017 15:28	Std
ICV	ICV	15723	3.8103 -		ISM02.4	PPB	8/30/2017 15:31	SMPL
ICB	ICB	-179	-0.0704 -		ISM02.4	PPB	8/30/2017 15:36	SMPL
CCV092	CCV092	20561	4.991 -		ISM02.4	PPB	8/30/2017 15:38	SMPL
CCB092	CCB092	-283	-0.0958 -		ISM02.4	PPB	8/30/2017 15:41	SMPL
PB101924BL	PBW003	-190	-0.0731 -		ISM02.4	PPB	8/30/2017 15:43	SMPL
I4928-01	MBDX59	11996	2.9008 -		ISM02.4	PPB	8/30/2017 15:45	SMPL
I4928-02	MBDX60	206338	50.3279 -		ISM02.4	PPB	8/30/2017 15:47	SMPL
I4928-03	MBDX61	424152	HIGH -		ISM02.4	PPB	8/30/2017 15:50	
I4928-04	MBDX61D	421111	HIGH -		ISM02.4	PPB	8/30/2017 15:52	
I4928-05	MBDX61S	428346	HIGH -		ISM02.4	PPB	8/30/2017 15:54	
CCV093	CCV093	19330	4.6906 -		ISM02.4	PPB	8/30/2017 15:56	SMPL
CCB093	CCB093	-309	-0.1021 -		ISM02.4	PPB	8/30/2017 16:01	SMPL
I4928-02DLX10	MBDX60	18168	4.407 -		ISM02.4	PPB	8/30/2017 16:03	SMPL
I4928-03DLX10	MBDX61	55863	13.6061 -		ISM02.4	PPB	8/30/2017 16:06	SMPL
I4928-04DLX10	MBDX61D	60055	14.6291 -		ISM02.4	PPB	8/30/2017 16:08	SMPL
I4928-05DLX10	MBDX61S	59827	14.5734 -		ISM02.4	PPB	8/30/2017 16:10	SMPL
I4928-03DL2X50	MBDX61	10266	2.4786 -		ISM02.4	PPB	8/30/2017 16:12	SMPL
I4928-04DL2X50	MBDX61D	11550	2.7919 -		ISM02.4	PPB	8/30/2017 16:15	SMPL
I4928-05DL2X50	MBDX61S	11946	2.8886 -		ISM02.4	PPB	8/30/2017 16:17	SMPL
CCV094	CCV094	20543	4.9866 -		ISM02.4	PPB	8/30/2017 16:19	SMPL
CCB094	CCB094	-281	-0.0953 -		ISM02.4	PPB	8/30/2017 16:24	SMPL