


ISM02.4

LB 89824
INSTRUMENT ID: CV1

Linear

 μ Abs.:

41032

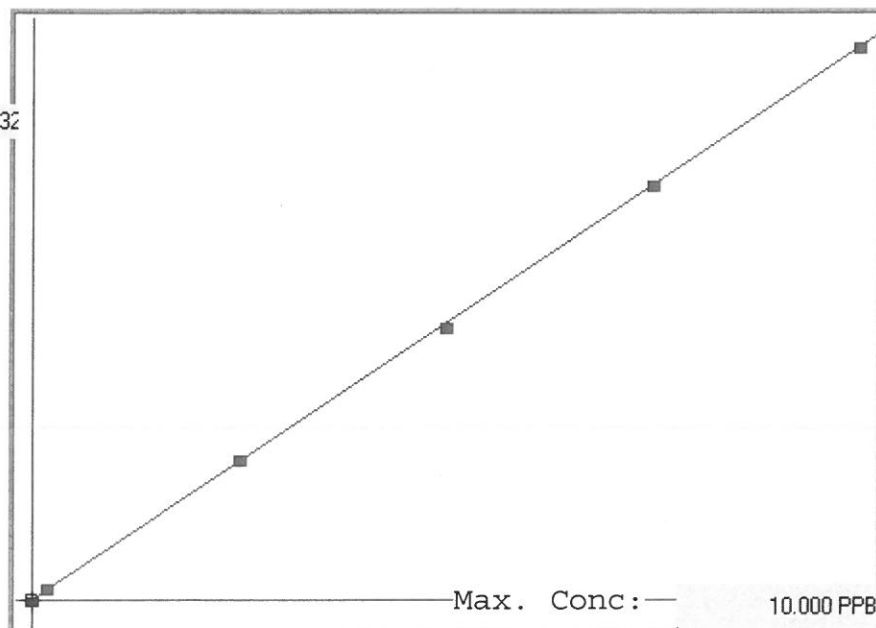

A= 0.0000e+000

B= 2.4393e-004

C= 1.4535e-003

Rho= 0.9999726

Accept=Accepted

slope
7.13165cent

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/d
0.00	0.000	-0.015	-0.015	-68	0.000	-68					-
0.2	0.200	0.214	0.014	871	0.0 %	871					7
2.5	2.500	2.534	0.034	10384	0.0 %	10384					1
5.0	5.000	4.948	-0.052	20279	0.0 %	20279					-1
7.5	7.500	7.509	0.009	30776	0.0 %	30776					0
10.0	10.000	10.010	0.010	41032	0.0 %	41032					0

NB
9/8/17

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Stnd Conc	Method	Units	Date	Type
	0 S0	-68	-		0 ISM02.4	PPB	9/1/2017 8:24	Std
	0.2 S0.2	871	-		0.2 ISM02.4	PPB	9/1/2017 8:26	Std
	2.5 S2.5	10384	-		2.5 ISM02.4	PPB	9/1/2017 8:29	Std
	5 S5	20279	-		5 ISM02.4	PPB	9/1/2017 8:31	Std
	7.5 S7.5	30776	-		7.5 ISM02.4	PPB	9/1/2017 8:33	Std
	10 S10	41032	-		10 ISM02.4	PPB	9/1/2017 8:35	Std
ICV	ICV	15531	3.7899 -		ISM02.4	PPB	9/1/2017 8:38	SMPL
ICB	ICB	-259	-0.0617 -		ISM02.4	PPB	9/1/2017 8:40	SMPL
CCV010	CCV010	20648	5.0381 -		ISM02.4	PPB	9/1/2017 8:43	SMPL
CCB010	CCB010	-260	-0.062 -		ISM02.4	PPB	9/1/2017 8:45	SMPL
PB101986BL	PBW003	-39	-0.0081 -		ISM02.4	PPB	9/1/2017 8:47	SMPL
I5037-07	MBDCZ9	-340	-0.0815 -		ISM02.4	PPB	9/1/2017 8:49	SMPL
PB101987BL	PBW003	-23	-0.0042 -		ISM02.4	PPB	9/1/2017 8:52	SMPL
I5038-07	MBDD00	-330	-0.079 -		ISM02.4	PPB	9/1/2017 8:54	SMPL
CCV011	CCV011	20631	5.0339 -		ISM02.4	PPB	9/1/2017 8:56	SMPL
CCB011	CCB011	-253	-0.0603 -		ISM02.4	PPB	9/1/2017 8:58	SMPL