

LB90113 DP

Result archive

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DP

9/15/2017 18:06

Sample id	Test id	Result	Status	Date	Errors
ICV ICV	CNEPA-NEW	93.695	man acc	9/15/2017	
ICB ICB	CNEPA-NEW	1.237	man acc	9/15/2017	
CCV001 CCV001	CNEPA-NEW	239.402	man acc	9/15/2017	
CCB001 CCB001	CNEPA-NEW	0.868	man acc	9/15/2017	
PB102358BL PBW00	CNEPA-NEW	0.955	man acc	9/15/2017	
I5241-01 MC0AA1	CNEPA-NEW	3.738	man acc	9/15/2017	
I5241-02 MC0AA1D	CNEPA-NEW	3.964	man acc	9/15/2017	
I5241-03 MC0AA1S	CNEPA-NEW	78.910	man acc	9/15/2017	
CCV002 CCV002	CNEPA-NEW	252.559	man acc	9/15/2017	
CCB002 CCB002	CNEPA-NEW	1.591	man acc	9/15/2017	

LB90113

DD

Aquakem v. 7.2AQ1

Results from time period:

Fri Sep 15 16:17:50 2017

Fri Sep 15 17:59:53 2017

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NEW	P	1.6627	µg/l	9/15/2017 17:26:40
S5.0	A	CNEPA-NEW	P	4.8628	µg/l	9/15/2017 17:26:41
S10.0	A	CNEPA-NEW	P	10.6521	µg/l	9/15/2017 17:26:42
S100.0	A	CNEPA-NEW	P	99.0403	µg/l	9/15/2017 17:26:43
S250.0	A	CNEPA-NEW	P	247.2038	µg/l	9/15/2017 17:26:44
S500.0	A	CNEPA-NEW	P	501.5784	µg/l	9/15/2017 17:26:45
ICV ICV	S	CNEPA-NEW	P	93.6951	µg/l	9/15/2017 17:55:03
ICB ICB	S	CNEPA-NEW	P	1.2366	µg/l	9/15/2017 17:55:04
CCV001 CCV001	S	CNEPA-NEW	P	239.4023	µg/l	9/15/2017 17:55:07
CCB001 CCB001	S	CNEPA-NEW	P	0.8678	µg/l	9/15/2017 17:55:09
PB102358BL PBW005	S	CNEPA-NEW	P	0.9546	µg/l	9/15/2017 17:55:10
I5241-01 MC0AA1	S	CNEPA-NEW	P	3.7382	µg/l	9/15/2017 17:55:12
I5241-02 MC0AA1D	S	CNEPA-NEW	P	3.9635	µg/l	9/15/2017 17:59:49
I5241-03 MC0AA1S	S	CNEPA-NEW	P	78.9101	µg/l	9/15/2017 17:59:50
CCV002 CCV002	S	CNEPA-NEW	P	252.5588	µg/l	9/15/2017 17:59:51
CCB002 CCB002	S	CNEPA-NEW	P	1.5914	µg/l	9/15/2017 17:59:52

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : DP

9/15/2017 17:30

Test CNEPA-NEW (Instrument ID: CN)


Accepted 9/15/2017 17:30

Factor (slope) 940.1

Bias (Y-intercept) 0.006

Coeff. of det. 0.999927

Errors

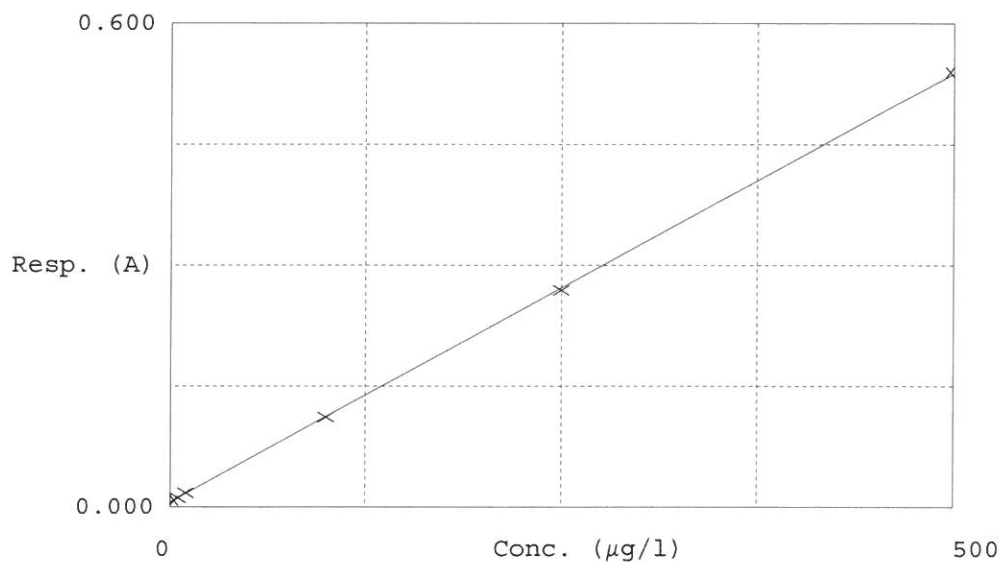

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN50.0	0.008	1.6627	0.0000	
2	5.0PPBCN50.0	0.011	4.8628	5.0000	
3	10PPBCN50.0	0.018	10.6521	10.0000	
4	100PPBCN50.0	0.112	99.0403	100.0000	
5	250PPBCN50.0	0.269	247.2038	250.0000	
6	500PPBCN50.0	0.540	501.5784	500.0000	

P. H. H. H. H.
97.25%
106.52%
99.04%
98.88%
100.31%

DP
09/15/17