


LB 90125

245.1

INSTRUMENT 1102 CV2

 μ Abs.:

30462

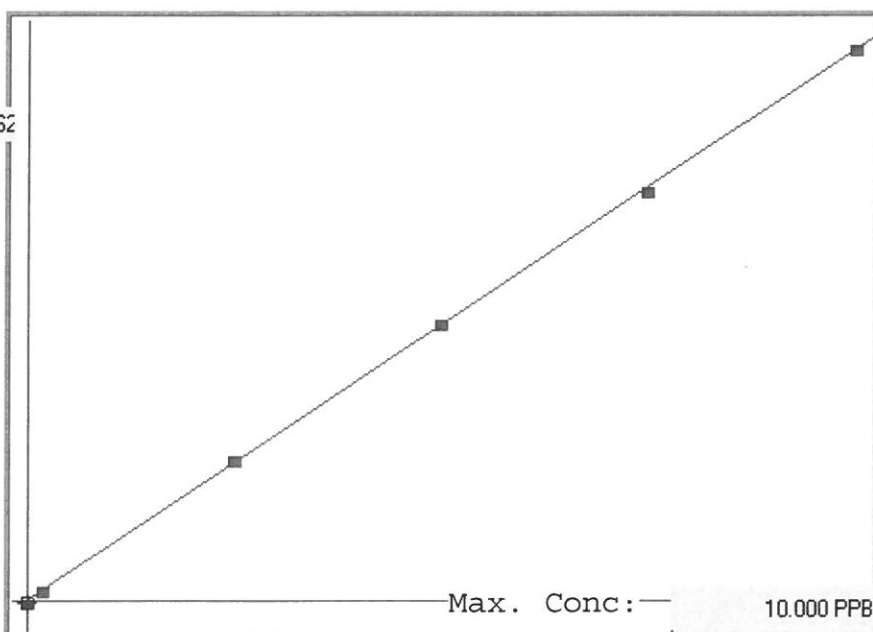

Linear

A= 0.0000e+000

B= 3.2916e-004

C= -2.1399e-003

Rho= 0.9999339

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.039	-0.039	-113	0.000	-113				
0.2	0.200	0.204	0.004	627	0.0 %	627				
2.5	2.500	2.553	0.053	7764	0.0 %	7764				
5.0	5.000	5.028	0.028	15281	0.0 %	15281				
7.5	7.500	7.429	-0.071	22577	0.0 %	22577				
10.0	10.000	10.025	0.025	30462	0.0 %	30462				

LB90125 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 18 Sep 2017 09:59:36

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-113	-	0.0000	245.1	PPB	18 Sep 2017 10:30:12	S	Std
0.2 - 1	50.2	627	-	0.2000	245.1	PPB	18 Sep 2017 10:32:20	S	Std
2.5 - 1	52.5	7764	-	2.5000	245.1	PPB	18 Sep 2017 10:34:29	S	Std
5.0 - 1	55	15281	-	5.0000	245.1	PPB	18 Sep 2017 10:36:37	S	Std
7.5 - 1	57.5	22577	-	7.5000	245.1	PPB	18 Sep 2017 10:38:45	S	Std
10.0 - 1	510	30462	-	10.0000	245.1	PPB	18 Sep 2017 10:43:22	S	Std
ICV61 - 1	ICV61	12189	4.0100	-245.1		PPB	18 Sep 2017 10:45:53	U	SMPL
ICB61 - 1	ICB61	-184	-0.0627	-245.1		PPB	18 Sep 2017 10:47:59	U	SMPL
CCV46 - 1	CCV46	15424	5.0748	-245.1		PPB	18 Sep 2017 10:50:06	U	SMPL
CCB46 - 1	CCB46	-287	-0.0966	-245.1		PPB	18 Sep 2017 10:52:12	U	SMPL
CRA - 1	CRA	553	0.1799	-245.1		PPB	18 Sep 2017 10:54:20	U	SMPL
HighStd - 1	HighStd	30939	10.1817	-245.1		PPB	18 Sep 2017 10:56:26	U	SMPL
ChkStd - 1	ChkStd	22548	7.4197	-245.1		PPB	18 Sep 2017 10:58:33	U	SMPL
PB102364BL - 1	PBW	-260	-0.0877	-245.1		PPB	18 Sep 2017 11:00:42	U	SMPL
PB102364BS - 1	LCSW	13268	4.3651	-245.1		PPB	18 Sep 2017 11:02:50	U	SMPL
I5251-01 - 1	GROUNDWATER	-187	-0.0637	-245.1		PPB	18 Sep 2017 11:07:24	U	SMPL
I5251-01DUP - 1	GROUNDWATERDUP	-151	-0.0518	-245.1		PPB	18 Sep 2017 11:09:31	U	SMPL
I5251-01MS - 1	GROUNDWATERMS	14052	4.6232	-245.1		PPB	18 Sep 2017 11:11:39	U	SMPL
I5251-01MSD - 1	GROUNDWATERMSD	14410	4.7410	-245.1		PPB	18 Sep 2017 11:13:48	U	SMPL
I5260-01 - 1	091317-SIDI-E-D-B	-312	-0.1048	-245.1		PPB	18 Sep 2017 11:15:54	U	SMPL
CCV47 - 1	CCV47	15285	5.0290	-245.1		PPB	18 Sep 2017 11:18:01	U	SMPL
CCB47 - 1	CCB47	-180	-0.0614	-245.1		PPB	18 Sep 2017 11:20:08	U	SMPL
I5260-02 - 1	091317-SIDI-E-D-S	-248	-0.0838	-245.1		PPB	18 Sep 2017 11:22:15	U	SMPL
I5260-03 - 1	091317-SIDI-E-U-B	-254	-0.0857	-245.1		PPB	18 Sep 2017 11:24:21	U	SMPL
I5260-04 - 1	091317-SIDI-E-U-S	-212	-0.0719	-245.1		PPB	18 Sep 2017 11:26:28	U	SMPL
I5260-05 - 1	091317-TIDO-E-D-M	-194	-0.0660	-245.1		PPB	18 Sep 2017 11:28:35	U	SMPL
I5260-06 - 1	091317-TIDO-E-U-M	-172	-0.0588	-245.1		PPB	18 Sep 2017 11:30:43	U	SMPL
I5262-01 - 1	091417-SIDI-E-D-B	-263	-0.0887	-245.1		PPB	18 Sep 2017 11:32:50	U	SMPL
I5262-02 - 1	091417-SIDI-E-D-S	-262	-0.0884	-245.1		PPB	18 Sep 2017 11:34:58	U	SMPL
I5262-03 - 1	091417-SIDI-E-U-B	-203	-0.0690	-245.1		PPB	18 Sep 2017 11:37:06	U	SMPL
I5262-04 - 1	091417-SIDI-E-U-S	-188	-0.0640	-245.1		PPB	18 Sep 2017 11:39:15	U	SMPL
CCV48 - 1	CCV48	15360	5.0537	-245.1		PPB	18 Sep 2017 11:41:22	U	SMPL
CCB48 - 1	CCB48	-228	-0.0772	-245.1		PPB	18 Sep 2017 11:43:29	U	SMPL
I5251-01LX5 - 1		-167	-0.0571	-245.1		PPB	18 Sep 2017 11:45:37	U	SMPL
I5251-01A - 1		14534	4.7818	-245.1		PPB	18 Sep 2017 11:47:43	U	SMPL
CCV49 - 1	CCV49	15078	4.9609	-245.1		PPB	18 Sep 2017 11:49:51	U	SMPL
CCB49 - 1	CCB49	-165	-0.0565	-245.1		PPB	18 Sep 2017 11:51:58	U	SMPL