

LB90211

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DP

9/20/2017 17:39

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.019	0.0	0.114	
ICB1	0.006	0.0	0.003	
CCV1	1.007	0.0	0.113	
CCB1	0.008	0.0	0.003	
PB102423BL	0.009	0.0	0.003	
PB102423BS	1.000	0.0	0.112	
I5274-25	1.614	0.0	0.179	
I5275-05	0.018	0.0	0.004	
I5275-06	0.091	0.0	0.012	
PB102424BL	0.006	0.0	0.003	
PB102424BS	1.010	0.0	0.113	
I5275-01	0.011	0.0	0.003	
I5275-02	0.083	0.0	0.011	
CCV2	1.032	0.0	0.116	
CCB2	0.005	0.0	0.003	

N	15
Mean	0.461
SD	0.5711
CV%	123.84

LB90211

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 20 16:41:58 2017

Wed Sep 20 17:37:06 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.056	mg/l	9/20/2017 16:41:58	
0.1PPM	A	Phenolics-	P	0.1013	mg/l	9/20/2017 16:41:59	
0.25PPM	A	Phenolics-	P	0.2568	mg/l	9/20/2017 16:42:00	
0.50PPM	A	Phenolics-	P	0.4993	mg/l	9/20/2017 16:42:01	
1.0PPM	A	Phenolics-	P	0.9752	mg/l	9/20/2017 16:42:02	
2.0PPM	A	Phenolics-	P	2.0115	mg/l	9/20/2017 16:42:03	
ICV1	S	Phenolics-	P	1.019	mg/l	9/20/2017 17:23:06	
ICB1	S	Phenolics-	P	0.0055	mg/l	9/20/2017 17:23:07	
CCV1	S	Phenolics-	P	1.0073	mg/l	9/20/2017 17:23:08	
CCB1	S	Phenolics-	P	0.0078	mg/l	9/20/2017 17:23:09	
PB102423BL	S	Phenolics-	P	0.0087	mg/l	9/20/2017 17:23:10	
PB102423BS	S	Phenolics-	P	0.9998	mg/l	9/20/2017 17:23:11	
I5274-25	S	Phenolics-	P	1.6136	mg/l	9/20/2017 17:23:12	
I5275-05	S	Phenolics-	P	0.0176	mg/l	9/20/2017 17:23:15	
I5275-06	S	Phenolics-	P	0.0911	mg/l	9/20/2017 17:33:08	
PB102424BL	S	Phenolics-	P	0.0063	mg/l	9/20/2017 17:33:10	
PB102424BS	S	Phenolics-	P	1.0096	mg/l	9/20/2017 17:33:11	
I5275-01	S	Phenolics-	P	0.0113	mg/l	9/20/2017 17:33:14	
I5275-02	S	Phenolics-	P	0.0831	mg/l	9/20/2017 17:33:15	
CCV2	S	Phenolics-	P	1.0324	mg/l	9/20/2017 17:33:17	
CCB2	S	Phenolics-	P	0.0048	mg/l	9/20/2017 17:33:18	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DP

9/20/2017 16:44


Test Phenolics-

Accepted 9/20/2017 16:44

Factor 9.1
Bias 0.002

Coeff. of det. 0.999703

Errors

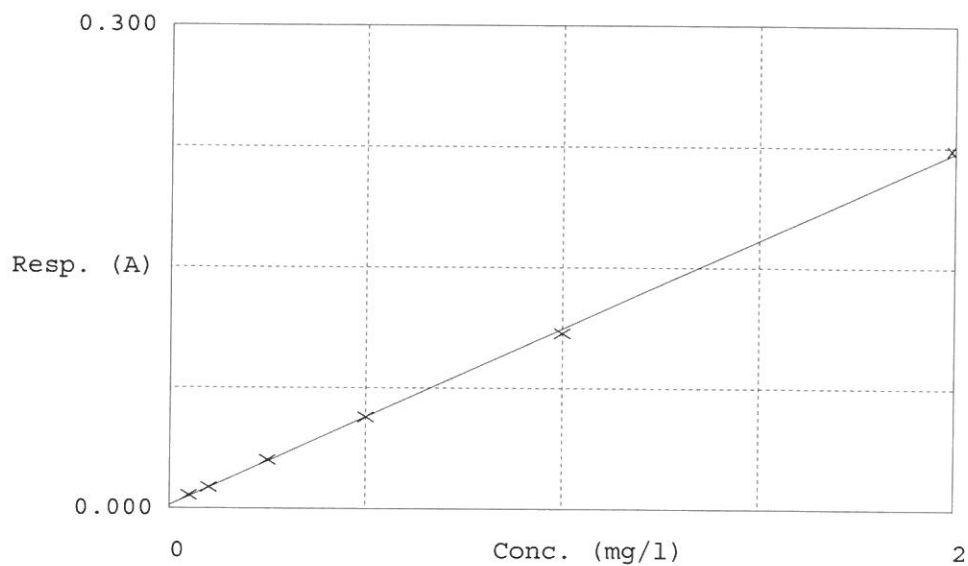

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.008	0.0560	0.0500	
2	Phenol-2	0.013	0.1013	0.1000	
3	Phenol-2	0.030	0.2568	0.2500	
4	Phenol-2	0.057	0.4993	0.5000	
5	Phenol-2	0.109	0.9752	1.0000	
6	Phenol-2	0.223	2.0115	2.0000	