


7470A

LB90243
INSTRUMENT ID: CV1

Linear

 μ Abs.:

34360

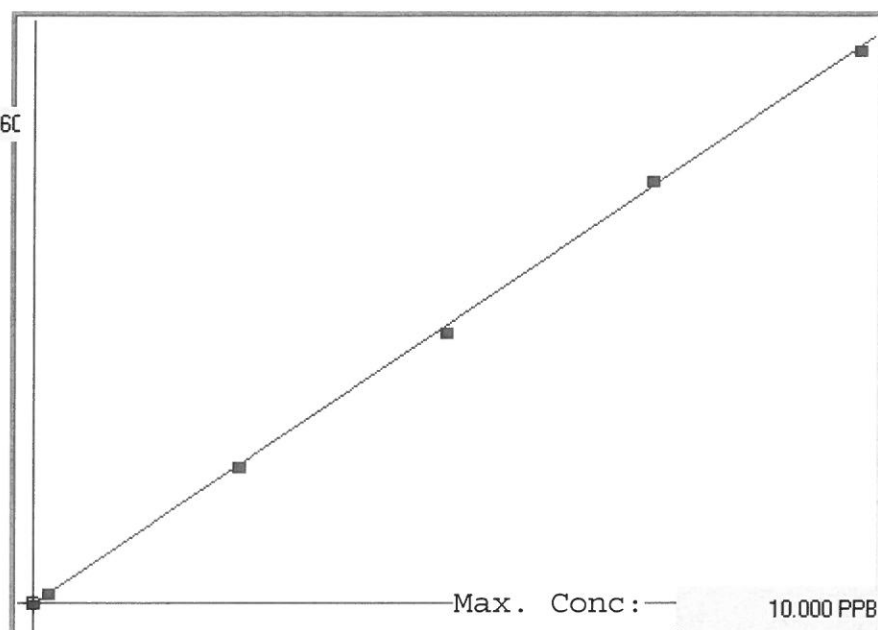

A= 0.0000e+000

B= 2.8863e-004

C= 3.6904e-002

Rho= 0.9998080

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.015	0.015	-77	0.000	-77				
0.2	0.200	0.213	0.013	610	0.0 %	610				
2.5	2.500	2.497	-0.003	8523	0.0 %	8523				
5.0	5.000	4.891	-0.109	16818	0.0 %	16818				
7.5	7.500	7.630	0.130	26309	0.0 %	26309				
10.0	10.000	9.954	-0.046	34360	0.0 %	34360				

LB90243 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 22 Sep 2017 09:01:04				
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	50	-77	-	0.0000	7470A	PPB	22 Sep 2017 09:05:05	S Std
0.2 - 1	50.2	610	-	0.2000	7470A	PPB	22 Sep 2017 09:07:14	S Std
2.5 - 1	52.5	8523	-	2.5000	7470A	PPB	22 Sep 2017 09:09:22	S Std
5.0 - 1	55	16818	-	5.0000	7470A	PPB	22 Sep 2017 09:11:30	S Std
7.5 - 1	57.5	26309	-	7.5000	7470A	PPB	22 Sep 2017 09:13:38	S Std
10.0 - 1	510	34360	-	10.0000	7470A	PPB	22 Sep 2017 09:15:45	S Std
ICV69 - 1	ICV69	14055	4.0935	-	7470A	PPB	22 Sep 2017 09:18:25	U SMPL
ICB69 - 1	ICB69	-197	-0.0200	-	7470A	PPB	22 Sep 2017 09:20:31	U SMPL
CCV83 - 1	CCV83	17592	5.1144	-	7470A	PPB	22 Sep 2017 09:22:38	U SMPL
CCB83 - 1	CCB83	-225	-0.0280	-	7470A	PPB	22 Sep 2017 09:24:44	U SMPL
CRA - 1	CRA	610	0.2130	-	7470A	PPB	22 Sep 2017 09:26:52	U SMPL
HighStd - 1	HighStd	35452	10.2693	-	7470A	PPB	22 Sep 2017 09:28:58	U SMPL
ChkStd - 1	ChkStd	24140	7.0043	-	7470A	PPB	22 Sep 2017 09:31:05	U SMPL
PB102518BL - 1	PBW	-238	-0.0318	-	7470A	PPB	22 Sep 2017 09:33:14	U SMPL
PB102518BS - 1	LCSW	13468	3.9241	-	7470A	PPB	22 Sep 2017 09:35:23	U SMPL
PB102518TB - 1	PB102483TB	-218	-0.0260	-	7470A	PPB	22 Sep 2017 09:37:30	U SMPL
I5309-04 - 1	TP-1-4-COMP	-89	0.0112	-	7470A	PPB	22 Sep 2017 09:39:38	U SMPL
I5309-08 - 1	TP-5-COMP	-73	0.0158	-	7470A	PPB	22 Sep 2017 09:41:46	U SMPL
I5329-03 - 1	CL-01092017-COMP	-75	0.0153	-	7470A	PPB	22 Sep 2017 09:43:55	U SMPL
I5330-03 - 1	HD-01092017-COMP	-89	0.0112	-	7470A	PPB	22 Sep 2017 09:46:02	U SMPL
CCV84 - 1	CCV84	17063	4.9617	-	7470A	PPB	22 Sep 2017 09:48:09	U SMPL
CCB84 - 1	CCB84	-213	-0.0246	-	7470A	PPB	22 Sep 2017 09:50:16	U SMPL
I5331-03 - 1	HR-05-92017-A	-71	0.0164	-	7470A	PPB	22 Sep 2017 09:52:24	U SMPL
I5331-06 - 1	HR-05-92017-B	-75	0.0153	-	7470A	PPB	22 Sep 2017 09:54:31	U SMPL
I5331-09 - 1	HR-05-92017-C	-66	0.0179	-	7470A	PPB	22 Sep 2017 09:56:38	U SMPL
I5333-02 - 1	SV-30745L	-99	0.0083	-	7470A	PPB	22 Sep 2017 09:58:45	U SMPL
I5335-02 - 1	SP-COMP	-136	-0.0023	-	7470A	PPB	22 Sep 2017 10:00:53	U SMPL
I5335-03 - 1	SP-CONCRETE	-90	0.0109	-	7470A	PPB	22 Sep 2017 10:03:00	U SMPL
I5336-03 - 1	TR-05-092017	-69	0.0170	-	7470A	PPB	22 Sep 2017 10:05:08	U SMPL
I5339-02 - 1	FRAC-TANK-573094	-55	0.0210	-	7470A	PPB	22 Sep 2017 10:07:17	U SMPL
I5339-02DUP - 1	FRAC-TANK-573094DUP	-75	0.0153	-	7470A	PPB	22 Sep 2017 10:09:26	U SMPL
I5339-02MS - 1	FRAC-TANK-573094MS	13089	3.8147	-	7470A	PPB	22 Sep 2017 10:11:33	U SMPL
CCV85 - 1	CCV85	17217	5.0062	-	7470A	PPB	22 Sep 2017 10:13:40	U SMPL
CCB85 - 1	CCB85	-204	-0.0220	-	7470A	PPB	22 Sep 2017 10:15:47	U SMPL
I5339-02MSD - 1	FRAC-TANK-573094MSD	13470	3.9247	-	7470A	PPB	22 Sep 2017 10:17:55	U SMPL
PB102519BL - 1	PBW	-141	-0.0038	-	7470A	PPB	22 Sep 2017 10:20:02	U SMPL
PB102519BS - 1	LCSW	13351	3.8904	-	7470A	PPB	22 Sep 2017 10:22:08	U SMPL
I5321-01 - 1	20170610-COMP-A	-267	-0.0402	-	7470A	PPB	22 Sep 2017 10:24:15	U SMPL
I5321-01DUP - 1	20170610-COMP-ADUP	-178	-0.0145	-	7470A	PPB	22 Sep 2017 10:26:23	U SMPL
I5321-01MS - 1	20170610-COMP-AMS	15409	4.4843	-	7470A	PPB	22 Sep 2017 10:28:31	U SMPL
I5321-01MSD - 1	20170610-COMP-AMSD	15072	4.3871	-	7470A	PPB	22 Sep 2017 10:30:39	U SMPL
I5321-02 - 1	20170611-COMP-B	-265	-0.0396	-	7470A	PPB	22 Sep 2017 10:32:47	U SMPL
I5321-03 - 1	20170530-LOC-6	-175	-0.0136	-	7470A	PPB	22 Sep 2017 10:34:56	U SMPL
I5321-04 - 1	20170610-COMP-A	-188	-0.0174	-	7470A	PPB	22 Sep 2017 10:37:03	U SMPL
CCV86 - 1	CCV86	17200	5.0013	-	7470A	PPB	22 Sep 2017 10:39:10	U SMPL
CCB86 - 1	CCB86	-206	-0.0226	-	7470A	PPB	22 Sep 2017 10:41:17	U SMPL
I5321-05 - 1	20170611-COMP-B	-156	-0.0081	-	7470A	PPB	22 Sep 2017 10:43:24	U SMPL
I5321-06 - 1	20170530-LOC-6	-157	-0.0084	-	7470A	PPB	22 Sep 2017 10:45:31	U SMPL
I5333-01 - 1	SV-30745L	252	0.1096	-	7470A	PPB	22 Sep 2017 10:47:38	U SMPL
I5338-01 - 1	20170920-092236	-162	-0.0099	-	7470A	PPB	22 Sep 2017 10:49:45	U SMPL
I5338-02 - 1	20170920-092832	-185	-0.0165	-	7470A	PPB	22 Sep 2017 10:51:53	U SMPL
I5338-03 - 1	20170920-093042	-168	-0.0116	-	7470A	PPB	22 Sep 2017 10:54:01	U SMPL
I5338-04 - 1	20170920-102115	-157	-0.0084	-	7470A	PPB	22 Sep 2017 10:56:09	U SMPL
I5338-05 - 1	20170920-102516	-141	-0.0038	-	7470A	PPB	22 Sep 2017 10:58:17	U SMPL
I5338-06 - 1	20170920-102714	-148	-0.0058	-	7470A	PPB	22 Sep 2017 11:00:26	U SMPL
I5338-07 - 1	20170920-133206	-133	-0.0015	-	7470A	PPB	22 Sep 2017 11:02:33	U SMPL
CCV87 - 1	CCV87	17622	5.1231	-	7470A	PPB	22 Sep 2017 11:04:40	U SMPL
CCB87 - 1	CCB87	-200	-0.0208	-	7470A	PPB	22 Sep 2017 11:06:47	U SMPL
I5338-08 - 1	20170920-134047	-167	-0.0113	-	7470A	PPB	22 Sep 2017 11:08:55	U SMPL
I5338-09 - 1	20170920-134229	-139	-0.0032	-	7470A	PPB	22 Sep 2017 11:11:02	U SMPL
I5338-10 - 1	20170920-142322	-109	0.0054	-	7470A	PPB	22 Sep 2017 11:13:09	U SMPL
I5338-11 - 1	20170920-142650	-125	0.0008	-	7470A	PPB	22 Sep 2017 11:15:16	U SMPL
I5338-12 - 1	20170920-142809	-189	-0.0176	-	7470A	PPB	22 Sep 2017 11:17:24	U SMPL
I5339-01 - 1	FRAC-TANK-573094	-185	-0.0165	-	7470A	PPB	22 Sep 2017 11:19:31	U SMPL
I5339-02LX5 - 1		-43	0.0245	-	7470A	PPB	22 Sep 2017 11:21:39	U SMPL
I5339-02A - 1		14184	4.1308	-	7470A	PPB	22 Sep 2017 11:23:48	U SMPL
I5321-01LX5 - 1		-79	0.0141	-	7470A	PPB	22 Sep 2017 11:25:56	U SMPL
I5321-01A - 1		15929	4.6344	-	7470A	PPB	22 Sep 2017 11:28:04	U SMPL
CCV88 - 1	CCV88	17743	5.1580	-	7470A	PPB	22 Sep 2017 11:30:12	U SMPL
CCB88 - 1	CCB88	-194	-0.0191	-	7470A	PPB	22 Sep 2017 11:32:20	U SMPL