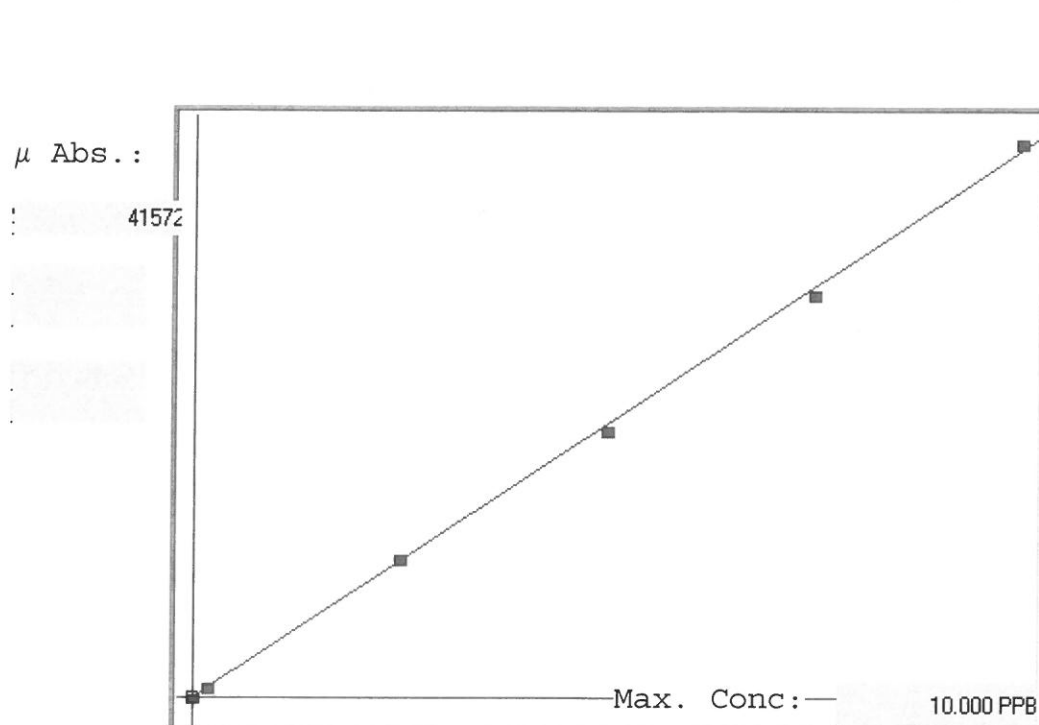


ISM02.4

LB 90431
INSTRUMENT ID: CV 1

Linear

A= 0.0000e+000

B= 2.4337e-004

C= 7.4137e-003

Rho= 0.9997004

Accept=Accepted

slope
y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.036	0.036	119	0.000	119					-
0.2	0.200	0.212	0.012	840	0.0 %	840					6
2.5	2.500	2.563	0.063	10500	0.0 %	10500					3
5.0	5.000	4.875	-0.125	20001	0.0 %	20001					-3
7.5	7.500	7.389	-0.111	30330	0.0 %	30330					-1
10.0	10.000	10.125	0.125	41572	0.0 %	41572					1

N03
9/29/18

LB90431
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	119	-		0 ISM02.4	PPB	9/29/2017 14:31	Std
	0.2 S0.2	840	-		0.2 ISM02.4	PPB	9/29/2017 14:33	Std
	2.5 S2.5	10500	-		2.5 ISM02.4	PPB	9/29/2017 14:35	Std
	5 S5	20001	-		5 ISM02.4	PPB	9/29/2017 14:38	Std
	7.5 S7.5	30330	-		7.5 ISM02.4	PPB	9/29/2017 14:40	Std
	10 S10	41572	-		10 ISM02.4	PPB	9/29/2017 14:45	Std
ICV	ICV	15643	3.8145 -		ISM02.4	PPB	9/29/2017 14:48	SMPL
ICB	ICB	-54	-0.0057 -		ISM02.4	PPB	9/29/2017 14:50	SMPL
CCV064	CCV064	20123	4.9048 -		ISM02.4	PPB	9/29/2017 14:56	SMPL
CCB064	CCB064	-45	-0.0035 -		ISM02.4	PPB	9/29/2017 14:58	SMPL
PB102712BL	PBW003	-1	0.0072 -		ISM02.4	PPB	9/29/2017 15:00	SMPL
I5375-01	MBDA83	-153	-0.0298 -		ISM02.4	PPB	9/29/2017 15:03	SMPL
I5375-02	MBDA84	-98	-0.0164 -		ISM02.4	PPB	9/29/2017 15:05	SMPL
I5375-03	MBDA85	1444	0.3588 -		ISM02.4	PPB	9/29/2017 15:07	SMPL
I5375-04	MBDA86	-221	-0.0464 -		ISM02.4	PPB	9/29/2017 15:09	SMPL
I5375-05	MBDAA2	-180	-0.0364 -		ISM02.4	PPB	9/29/2017 15:12	SMPL
I5375-06	MBDAA2D	-142	-0.0271 -		ISM02.4	PPB	9/29/2017 15:14	SMPL
I5375-07	MBDAA2S	3963	0.9719 -		ISM02.4	PPB	9/29/2017 15:16	SMPL
I5375-08	MBDAA3	-85	-0.0133 -		ISM02.4	PPB	9/29/2017 15:19	SMPL
I5375-09	MBDAA4	-103	-0.0177 -		ISM02.4	PPB	9/29/2017 15:21	SMPL
I5375-10	MBDAA6	-93	-0.0152 -		ISM02.4	PPB	9/29/2017 15:23	SMPL
I5375-11	MBDAA7	-93	-0.0152 -		ISM02.4	PPB	9/29/2017 15:25	SMPL
I5375-12	MBDAA9	-78	-0.0116 -		ISM02.4	PPB	9/29/2017 15:28	SMPL
I5375-13	MBDAB0	-155	-0.0303 -		ISM02.4	PPB	9/29/2017 15:30	SMPL
I5375-14	MBDAB1	-162	-0.032 -		ISM02.4	PPB	9/29/2017 15:32	SMPL
I5375-15	MBDAB2	-84	-0.013 -		ISM02.4	PPB	9/29/2017 15:34	SMPL
I5375-16	MBDAB3	-131	-0.0245 -		ISM02.4	PPB	9/29/2017 15:37	SMPL
I5375-17	MBDAB4	65	0.0232 -		ISM02.4	PPB	9/29/2017 15:39	SMPL
I5375-18	MBDAB6	-128	-0.0237 -		ISM02.4	PPB	9/29/2017 15:41	SMPL
I5375-19	MBDAB7	-103	-0.0177 -		ISM02.4	PPB	9/29/2017 15:44	SMPL
CCV065	CCV065	20078	4.8939 -		ISM02.4	PPB	9/29/2017 15:46	SMPL
CCB065	CCB065	-50	-0.0048 -		ISM02.4	PPB	9/29/2017 15:48	SMPL
I5375-20	MBDAB8	-166	-0.033 -		ISM02.4	PPB	9/29/2017 15:50	SMPL
PB102713BL	PBW003	3	0.0081 -		ISM02.4	PPB	9/29/2017 15:53	SMPL
I5490-11	EQB-1-092717	-161	-0.0318 -		ISM02.4	PPB	9/29/2017 15:55	SMPL
CCV066	CCV066	19934	4.8588 -		ISM02.4	PPB	9/29/2017 15:57	SMPL
CCB066	CCB066	-90	-0.0145 -		ISM02.4	PPB	9/29/2017 15:59	SMPL