


ISM02.4

LB90699
INSTRUMENT ID: CV1

Linear

 μ Abs.:

45090

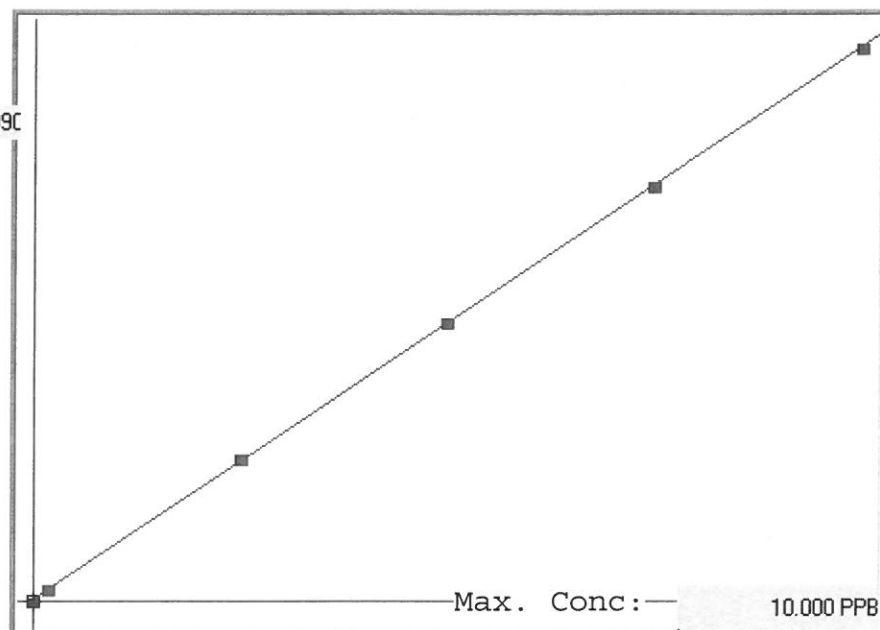

A= 0.0000e+000

B= 2.2186e-004

C= -2.2892e-002

Rho= 0.9999646

Accept=Accepted

Slope
Y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%OD
0.00	0.000	-0.039	-0.039	-72	0.000	-72					-
0.2	0.200	0.188	-0.012	951	0.0 %	951					-6
2.5	2.500	2.559	0.059	11636	0.0 %	11636					2
5.0	5.000	5.017	0.017	22717	0.0 %	22717					0
7.5	7.500	7.494	-0.006	33882	0.0 %	33882					0
10.0	10.000	9.981	-0.019	45090	0.0 %	45090					0

NB
10/10/12

LB90699
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	-72	-		0 ISM02.4	PPB	10/10/2017 14:25	Std
	0.2 S0.2	951	-		0.2 ISM02.4	PPB	10/10/2017 14:27	Std
	2.5 S2.5	11636	-		2.5 ISM02.4	PPB	10/10/2017 14:29	Std
	5 S5	22717	-		5 ISM02.4	PPB	10/10/2017 14:31	Std
	7.5 S7.5	33882	-		7.5 ISM02.4	PPB	10/10/2017 14:34	Std
	10 S10	45090	-		10 ISM02.4	PPB	10/10/2017 14:36	Std
ICV	ICV	16690	3.68	-	ISM02.4	PPB	10/10/2017 14:39	SMPL
ICB	ICB	-276	-0.0841	-	ISM02.4	PPB	10/10/2017 14:41	SMPL
CCV067	CCV067	22744	5.0231	-	ISM02.4	PPB	10/10/2017 14:43	SMPL
CCB067	CCB067	-309	-0.0914	-	ISM02.4	PPB	10/10/2017 14:46	SMPL
PB103101BL	PBS004	-51	-0.0342	-	ISM02.4	PPB	10/10/2017 14:48	SMPL
I5652-01	B-39(0.5-1.5)-100317	10477	2.3015	-	ISM02.4	PPB	10/10/2017 14:50	SMPL
I5652-02	B-39(5-7)-100317	30125	6.6607	-	ISM02.4	PPB	10/10/2017 14:52	SMPL
I5652-03	B-59(FILL)-100317	24695	5.456	-	ISM02.4	PPB	10/10/2017 14:55	SMPL
I5652-04	B-59(FILL)-100317D	22931	5.0646	-	ISM02.4	PPB	10/10/2017 14:57	SMPL
I5652-05	B-59(FILL)-100317S	36268	8.0235	-	ISM02.4	PPB	10/10/2017 14:59	SMPL
I5652-06	B-59(5-7)-100317	65157	14.4329	-	ISM02.4	PPB	10/10/2017 15:02	SMPL
I5652-07	B-59(12-13.5)-100317	3251	0.6984	-	ISM02.4	PPB	10/10/2017 15:04	SMPL
I5652-08	B-57(1-2)-100317	57684	12.7749	-	ISM02.4	PPB	10/10/2017 15:06	SMPL
I5652-09	B-57(2-4)-100317	13965	3.0754	-	ISM02.4	PPB	10/10/2017 15:09	SMPL
I5652-10	DUP-2	63806	14.1331	-	ISM02.4	PPB	10/10/2017 15:11	SMPL
I5652-11	B-42(7-9)-100217	207776	46.0744	-	ISM02.4	PPB	10/10/2017 15:13	SMPL
PB103102BL	PBS004	-59	-0.036	-	ISM02.4	PPB	10/10/2017 15:18	SMPL
I5720-01	B-36(0-1)-100417	9843	2.1609	-	ISM02.4	PPB	10/10/2017 15:21	SMPL
I5720-02	B-36(3-3.7)-100417	3417	0.7352	-	ISM02.4	PPB	10/10/2017 15:23	SMPL
I5720-03	B-35(1-2)-100417	7504	1.6419	-	ISM02.4	PPB	10/10/2017 15:25	SMPL
I5720-04	B-35(2-3.8)-100417	23318	5.1505	-	ISM02.4	PPB	10/10/2017 15:27	SMPL
I5720-05	B-37(0-1)-100417	8113	1.7771	-	ISM02.4	PPB	10/10/2017 15:30	SMPL
I5720-06	B-37(1-3)-100417	4096	0.8858	-	ISM02.4	PPB	10/10/2017 15:32	SMPL
I5720-07	B-25(0.5-1.5)-100517	3679	0.7933	-	ISM02.4	PPB	10/10/2017 15:34	SMPL
CCV068	CCV068	22930	5.0644	-	ISM02.4	PPB	10/10/2017 15:37	SMPL
CCB068	CCB068	-291	-0.0875	-	ISM02.4	PPB	10/10/2017 15:39	SMPL
I5720-08	B-25(0.5-1.5)-100517D	3188	0.6844	-	ISM02.4	PPB	10/10/2017 15:41	SMPL
I5720-09	B-25(0.5-1.5)-100517S	15465	3.4082	-	ISM02.4	PPB	10/10/2017 15:43	SMPL
I5720-10	B-25(5-5.5)-100517	273085	60.5639	-	ISM02.4	PPB	10/10/2017 15:46	SMPL
I5720-11	B-24(0.5-1.5)-100517	6490	1.417	-	ISM02.4	PPB	10/10/2017 15:48	SMPL
I5720-12	B-24(1.5-3.5)-100517	31363	6.9353	-	ISM02.4	PPB	10/10/2017 15:51	SMPL
I5720-13	B-27(0.5-1.5)-100517	7424	1.6242	-	ISM02.4	PPB	10/10/2017 15:53	SMPL
I5720-14	B-27(5-5.5)-100517	10086	2.2148	-	ISM02.4	PPB	10/10/2017 15:55	SMPL
I5720-15	B-26(5-5.8)-100517	756	0.1448	-	ISM02.4	PPB	10/10/2017 15:58	SMPL
I5720-16	B-26(0.5-1.5)-100517	4105	0.8878	-	ISM02.4	PPB	10/10/2017 16:00	SMPL
I5720-17	DUP-3	28019	6.1934	-	ISM02.4	PPB	10/10/2017 16:05	SMPL
PB103103BL	PBS004	-43	-0.0324	-	ISM02.4	PPB	10/10/2017 16:07	SMPL
I5747-01	B-23(0-1)-100517	9493	2.0832	-	ISM02.4	PPB	10/10/2017 16:10	SMPL
I5747-01D	B-23(0-1)-100517D	10524	2.312	-	ISM02.4	PPB	10/10/2017 16:12	SMPL
I5747-01S	B-23(0-1)-100517S	21411	4.7274	-	ISM02.4	PPB	10/10/2017 16:19	SMPL
I5747-02	B-23(1-3)-100517	10404	2.2853	-	ISM02.4	PPB	10/10/2017 16:21	SMPL
I5747-03	B-22(0-1)-100617	10961	2.4089	-	ISM02.4	PPB	10/10/2017 16:23	SMPL

LB90699
INSTRUMENT ID : CV1

I5747-04	B-22(1-3)-100617	5214	1.1339 -	ISM02.4	PPB	10/10/2017 16:26	SMPL
I5747-05	B-4(0-1)-100617	28474	6.2944 -	ISM02.4	PPB	10/10/2017 16:28	SMPL
I5747-06	B-4(1-3)-100617	30756	6.8006 -	ISM02.4	PPB	10/10/2017 16:30	SMPL
I5747-07	B-34(0-1)-100617	23107	5.1036 -	ISM02.4	PPB	10/10/2017 16:32	SMPL
CCV069	CCV069	22608	4.9929 -	ISM02.4	PPB	10/10/2017 16:35	SMPL
CCB069	CCB069	-317	-0.0932 -	ISM02.4	PPB	10/10/2017 16:37	SMPL
I5747-08	B-34(5-5.5)-100617	16597	3.6593 -	ISM02.4	PPB	10/10/2017 16:39	SMPL
I5652-06DLX5	B-59(5-7)-100317	13276	2.9225 -	ISM02.4	PPB	10/10/2017 16:42	SMPL
I5652-08DLX2	B-57(1-2)-100317	28731	6.3514 -	ISM02.4	PPB	10/10/2017 16:44	SMPL
I5652-10DLX5	DUP-2	12820	2.8214 -	ISM02.4	PPB	10/10/2017 16:46	SMPL
I5652-11DLX10	B-42(7-9)-100217	21932	4.843 -	ISM02.4	PPB	10/10/2017 16:48	SMPL
I5720-10DLX10	B-25(5-5.5)-100517	29109	6.4352 -	ISM02.4	PPB	10/10/2017 16:51	SMPL
CCV070	CCV070	22831	5.0424 -	ISM02.4	PPB	10/10/2017 16:53	SMPL
CCB070	CCB070	-315	-0.0928 -	ISM02.4	PPB	10/10/2017 16:55	SMPL