

10/20/2017 10/12/17 AK


Clear table

ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-09-06_	9/6/17 12:53
STD2	0.1880	0.2550	0.2710	0.8530	0.2160	0.2870	1.4360	2017-09-06_	9/6/17 13:24
STD3	0.4490	0.6520	0.6530	2.1870	0.5450	1.1700	3.3250	2017-09-06_	9/6/17 13:55
STD4	0.8330	1.1970	1.1840	3.9870	0.9930	2.0380	5.9400	2017-09-06_	9/6/17 14:26
STD5	1.9340	2.8800	2.8580	9.6380	2.3960	4.7930	14.1690	2017-09-06_	9/6/17 14:57
STD6	3.8580	5.8770	5.9000	19.6860	4.9100	9.9500	29.2520	2017-09-06_	9/6/17 15:28
STD7	5.0850	7.6300	7.6270	25.4170	6.3620	12.4780	38.2290	2017-09-06_	9/6/17 15:59
ICV	2.0270	2.9360	2.9290	9.7850	2.4490	5.2020	14.5930	2017-09-06_	9/6/17 17:32
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-09-06_	9/6/17 18:03
CCV	2.0540	2.9360	2.8910	9.6880	2.4140	4.8230	14.5540	2017-09-19_	9/19/17 9:33
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-09-19_	9/19/17 10:04
LB90750BLS	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-09-19_	9/19/17 10:35
LB90750BSS	2.0290	2.8790	2.8300	9.4880	2.3720	4.9880	14.2200	2017-09-19_	9/19/17 11:06
I5275-01	0.0620	0.1250	0.0000	0.4340	0.1170	-0.0560	0.8080	2017-09-19_	9/19/17 11:37
I5275-02	0.2490	0.3920	0.3830	1.2360	0.3160	0.6160	1.9630	2017-09-19_	9/19/17 12:08
CCV	2.0470	2.9510	2.8890	9.7120	2.4220	5.0980	14.5960	2017-09-19_	9/19/17 12:39
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2017-09-19_	9/19/17 13:10

IC2 AK
Cal 09-06-17

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-090617.mtw
Equation: $Q = 0.0173542 \cdot A + 2.06792$
RSD: 5.692 %
Correlation coefficient: 0.998677

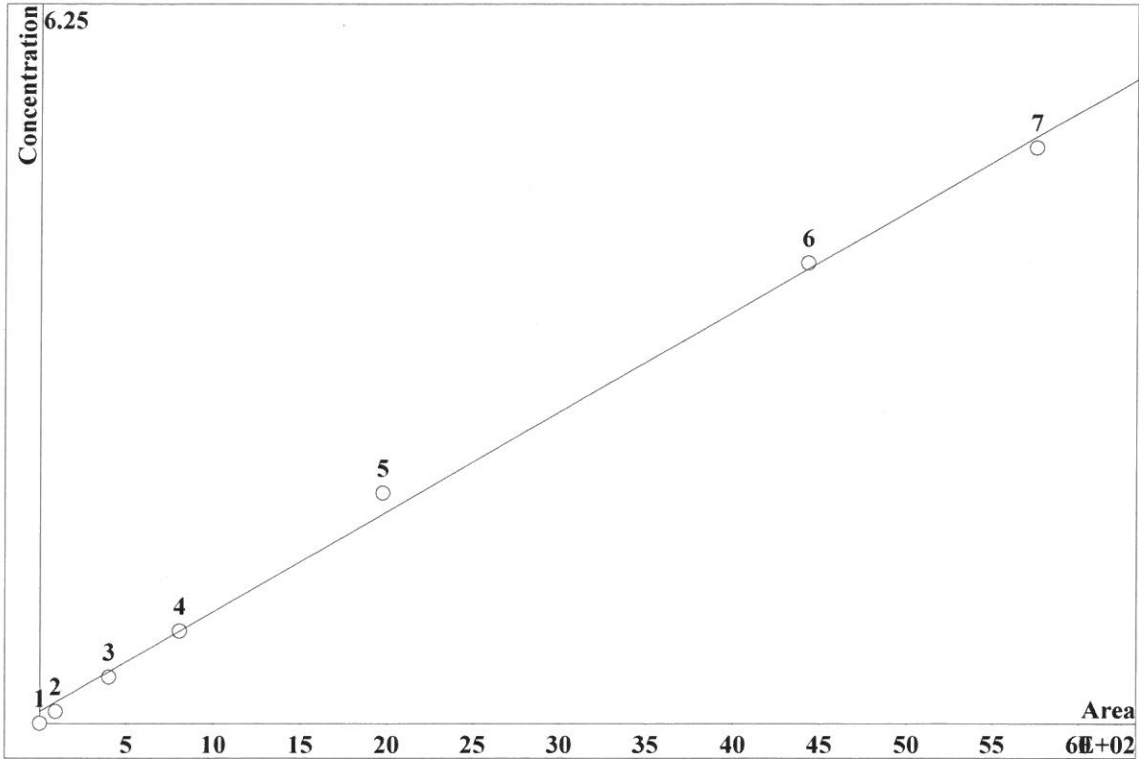


K3 = 0 K2 = 0 K1 = 0.0173542 K0 = 2.06792
Base: Area
Ref.channel: chl
ISTD:
Formula: Linear
Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0	0		
2	3.945	93.38	0.1	20	5.175		
3	17.14	399.1	0.4	20	5.175		
4	34.15	805.3	0.8	20	5.175		
5	85.75	1975	2	20	5.175		
6	181.9	4434	4	20	5.175		
7	227.9	5753	5	20	5.175		

CE

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-090617.mtw
 Equation: $Q = 0.0263015 \cdot A + 2.34303$
 RSD: 4.624 %
 Correlation coefficient: 0.999127

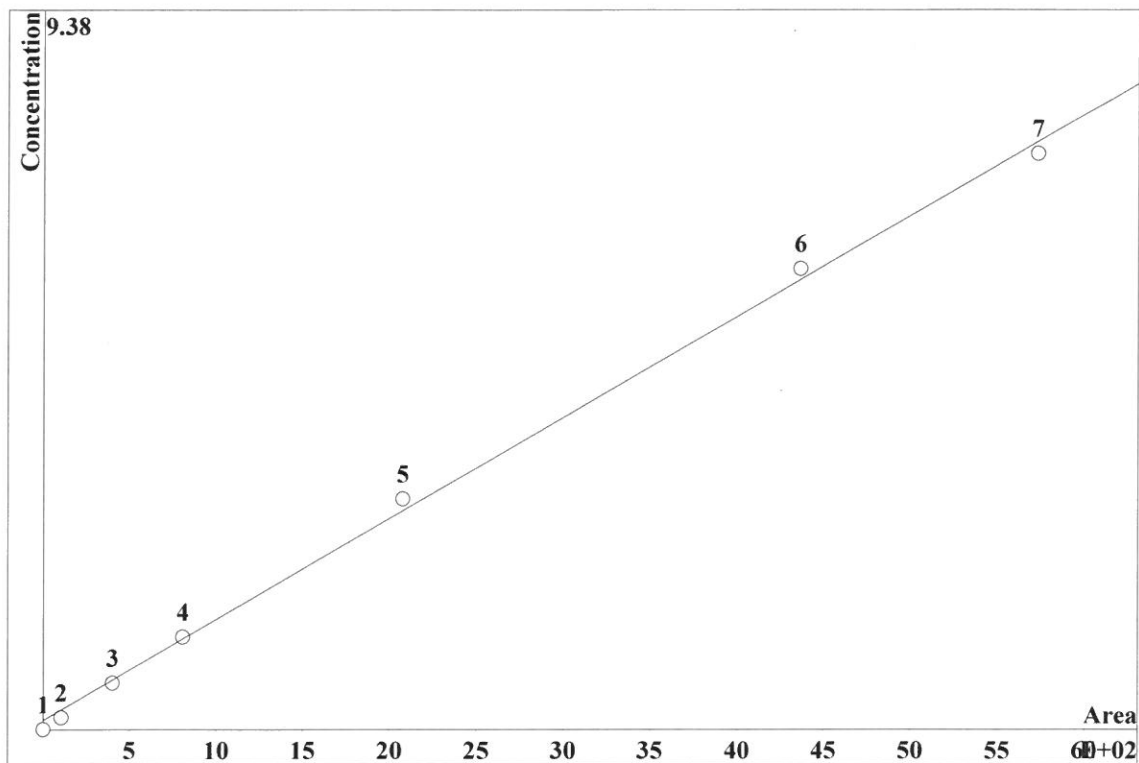


K3 = 0 K2 = 0 K1 = 0.0263015 K0 = 2.34303
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	7.238	105.5	0.15	20	9.032		
3	28.06	401.3	0.6	20	9.032		
4	56.98	808.6	1.2	20	9.032		
5	148.7	2078	3	20	9.032		
6	316.7	4367	6	20	9.032		
7	420.9	5735	7.5	20	9.032		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-090617.mtw
 Equation: $Q = 0.0111582 \cdot A + 3.01119$
 RSD: 4.803 %
 Correlation coefficient: 0.999058

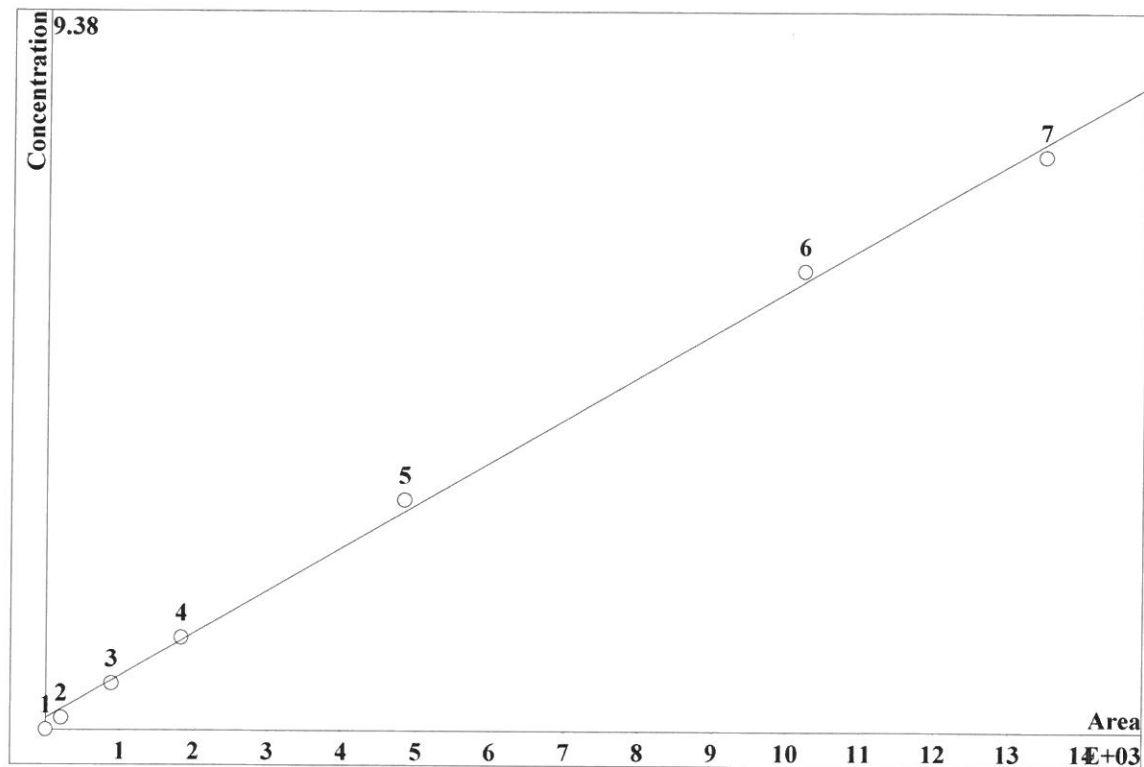


K3 = 0 K2 = 0 K1 = 0.0111582 K0 = 3.01119
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	12.8	213.7	0.15	20	11.72		
3	52.49	886.6	0.6	20	11.72		
4	108.9	1823	1.2	20	11.72		
5	290.5	4833	3	20	11.72		
6	606.6	1.023e+04	6	20	11.72		
7	806.8	1.346e+04	7.5	20	11.72		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-090617.mtw
 Equation: $Q = 0.058529 \cdot A + 8.28559$
 RSD: 4.603 %
 Correlation coefficient: 0.999135

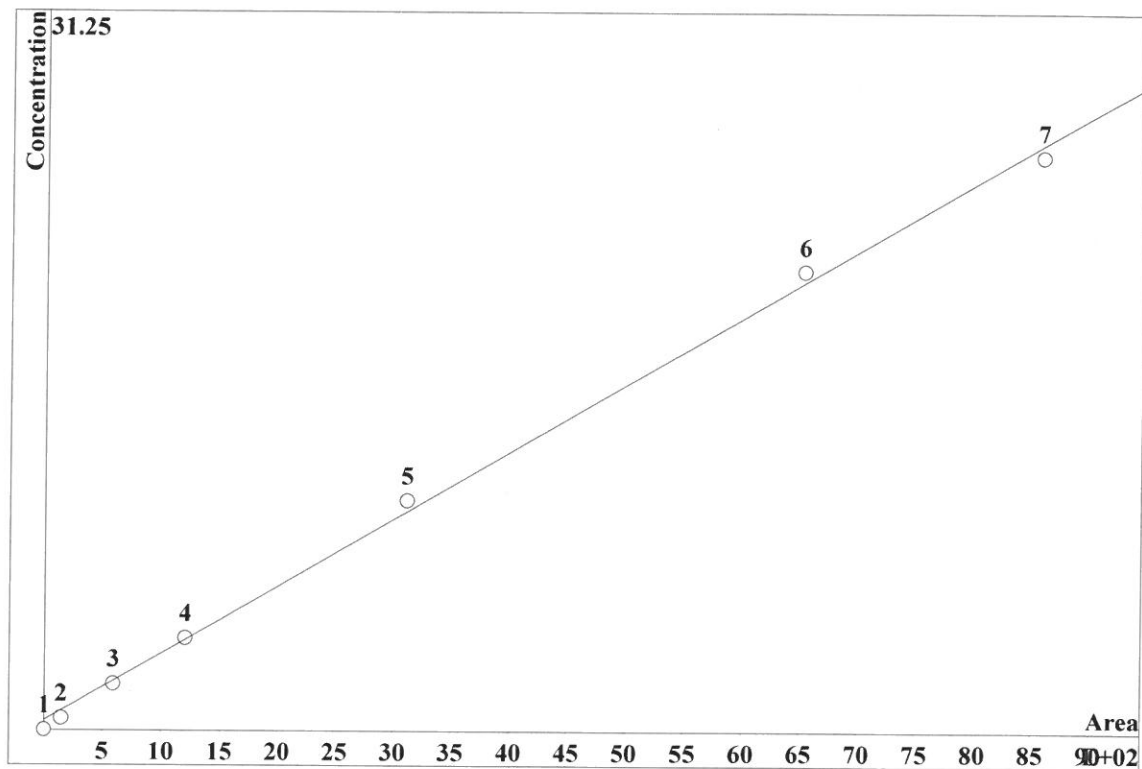

K3 = 0 K2 = 0 K1 = 0.058529 K0 = 8.28559

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.758	148.4	0.5	20	15.11		
3	27.75	590.9	2	20	15.11		
4	56.75	1204	4	20	15.11		
5	148.3	3111	10	20	15.11		
6	313.7	6529	20	20	15.11		
7	415.1	8583	25	20	15.11		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-090617.mtw
 Equation: $Q = 0.0103671 \cdot A + 2.24907$
 RSD: 4.762 %
 Correlation coefficient: 0.999074

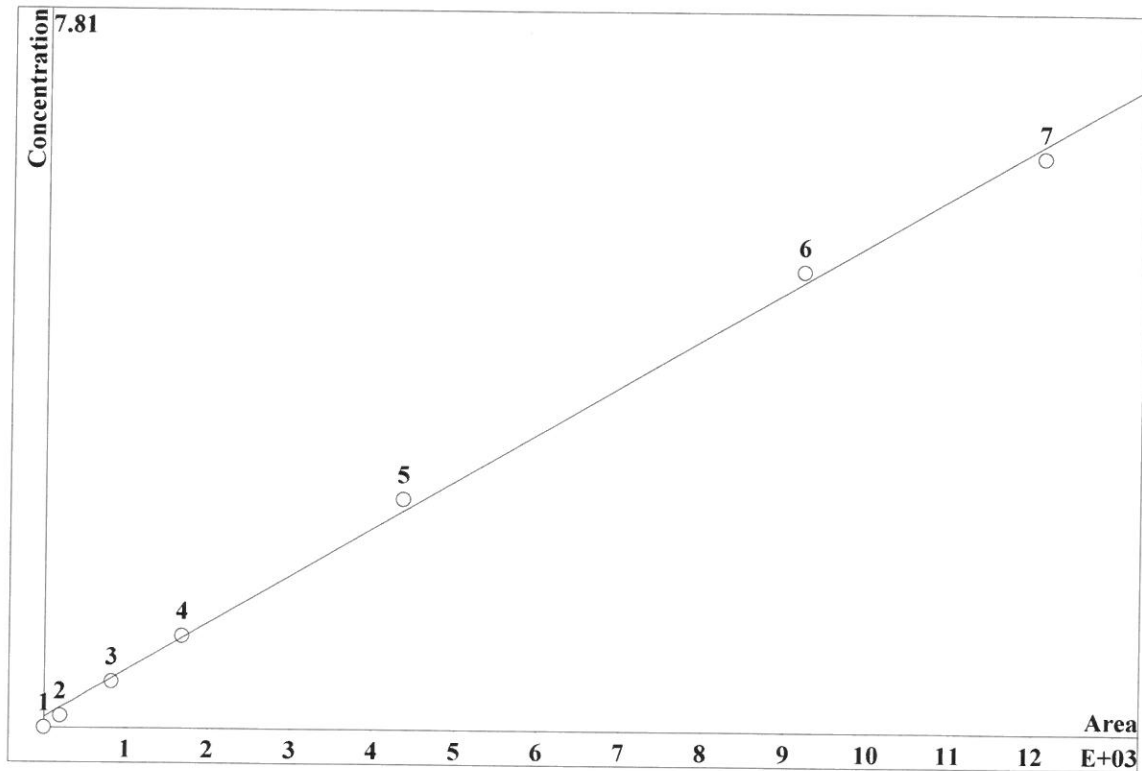

K3 = 0 K2 = 0 K1 = 0.0103671 K0 = 2.24907

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	20		0
2	8.199	202.2	0.125	20	17.96		
3	33.55	821.4	0.5	20	17.96		
4	68.29	1679	1	20	17.96		
5	176.9	4357	2.5	20	17.96		
6	367.9	9199	5	20	17.96		
7	481.3	1.21e+04	6.25	20	17.96		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-090617.mtw
 Equation: $Q = 0.0297833 \cdot A - 2.3432$
 RSD: 3.664 %
 Correlation coefficient: 0.999452

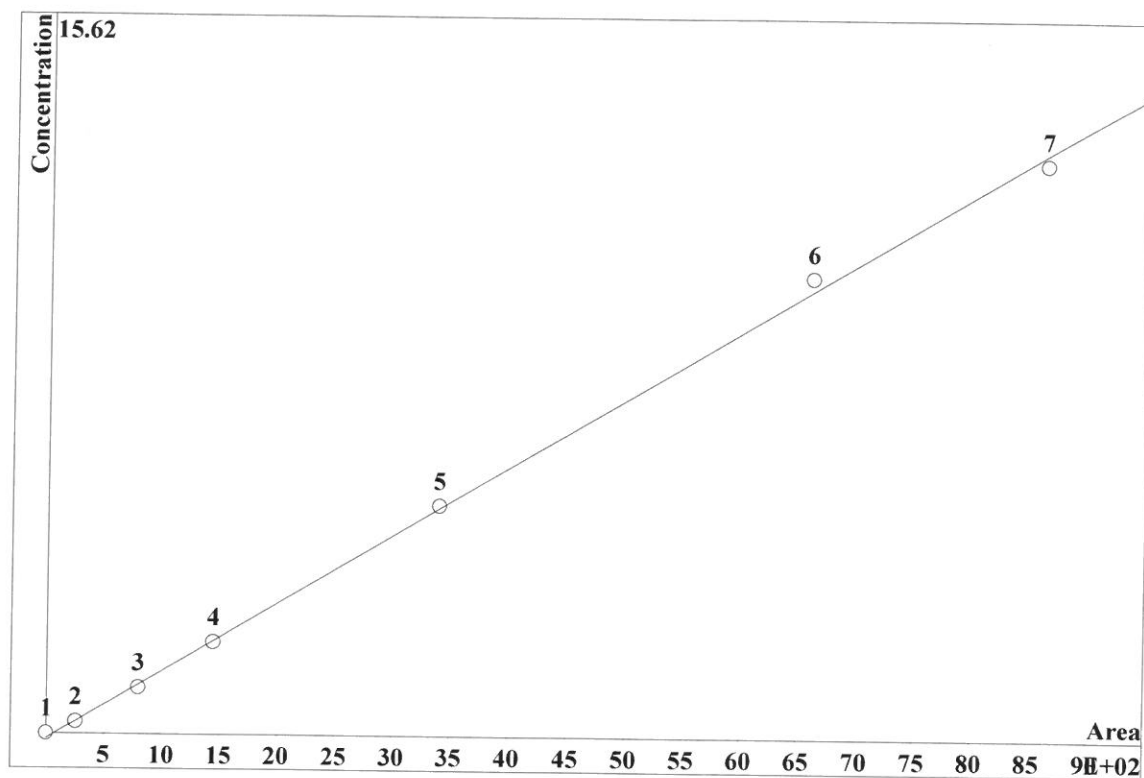

K3 = 0 K2 = 0 K1 = 0.0297833 K0 = -2.3432

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.21	256	0.25	20	23.35		
3	19.95	796.4	1	20	23.35		
4	37.35	1442	2	20	23.35		
5	92.63	3397	5	20	23.35		
6	182.3	6604	10	20	23.35		
7	241.1	8625	12.5	20	23.35		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-090617.mtw
 Equation: $Q = 0.0338478 \cdot A + 16.0388$
 RSD: 5.592 %
 Correlation coefficient: 0.998723

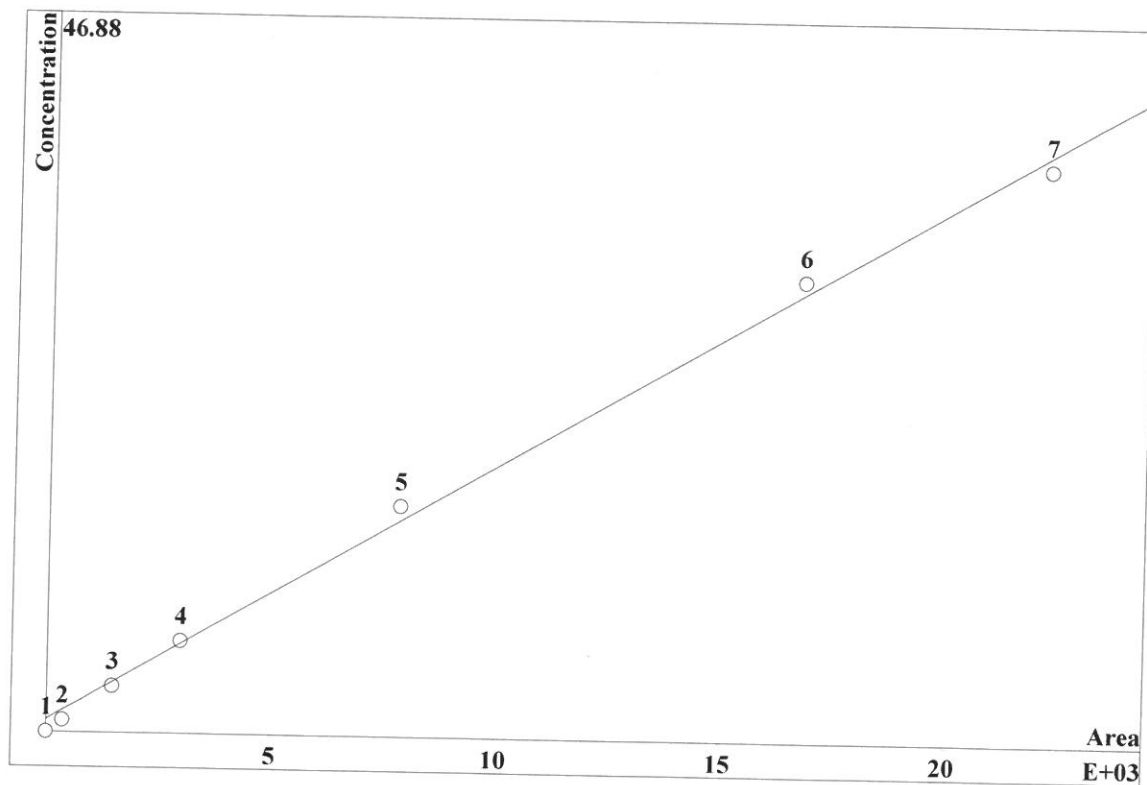

K3 = 0 K2 = 0 K1 = 0.0338478 K0 = 16.0388

Base: Area

Ref.channel: ch1

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	11.04	371.3	0.75	20	25.16		
3	43.8	1467	3	20	25.16		
4	89.18	2984	6	20	25.16		
5	235.8	7832	15	20	25.16		
6	506.5	1.678e+04	30	20	25.16		
7	672.5	2.223e+04	37.5	20	25.16		

Report date: 9/7/2017 9:19:55 AM
Printed by: wet


Ident: STD1
Analysis from: 9/6/2017 12:53:46 PM
File: _2017-09-06_

Last save: 9/6/2017 1:21:46 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14939

Last save: 9/6/2017 11:18:

SAMPLE:
:
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

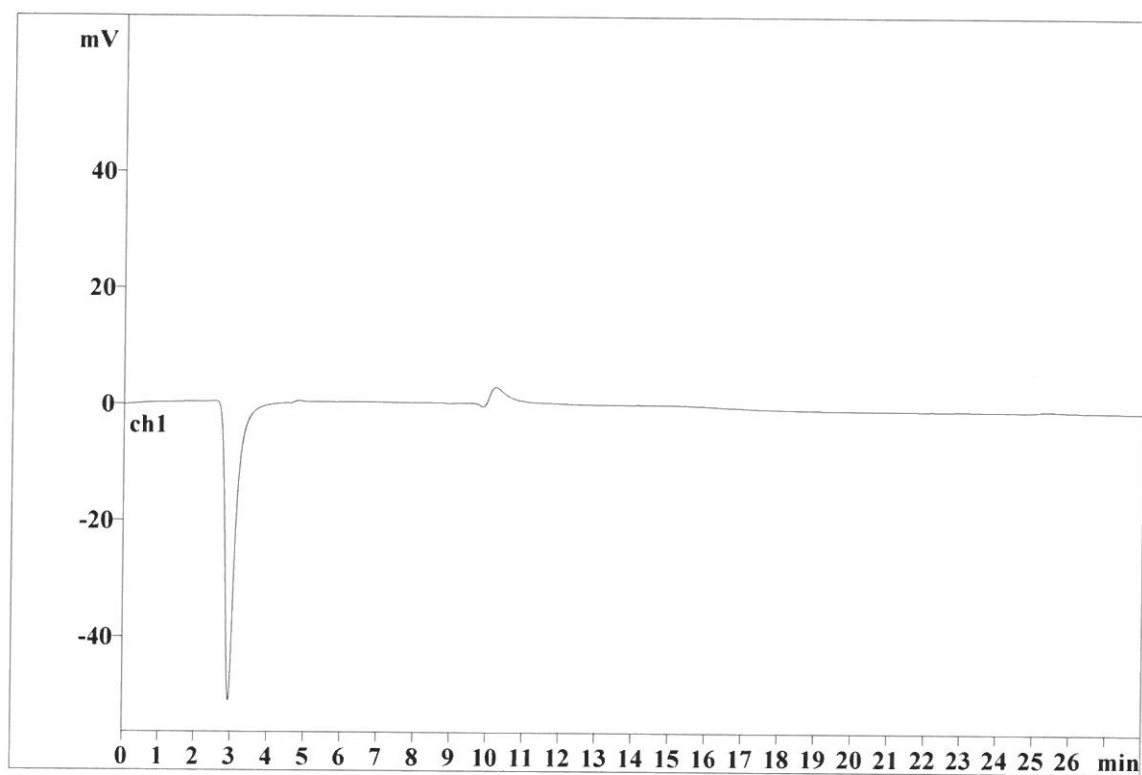

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/7/2017 9:20:38 AM
Printed by: wet


Ident: STD2
Analysis from: 9/6/2017 1:24:44 PM
File: _2017-09-06_

Last save: 9/6/2017 1:52:44 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14940

Last save: 9/6/2017 1:21:4

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

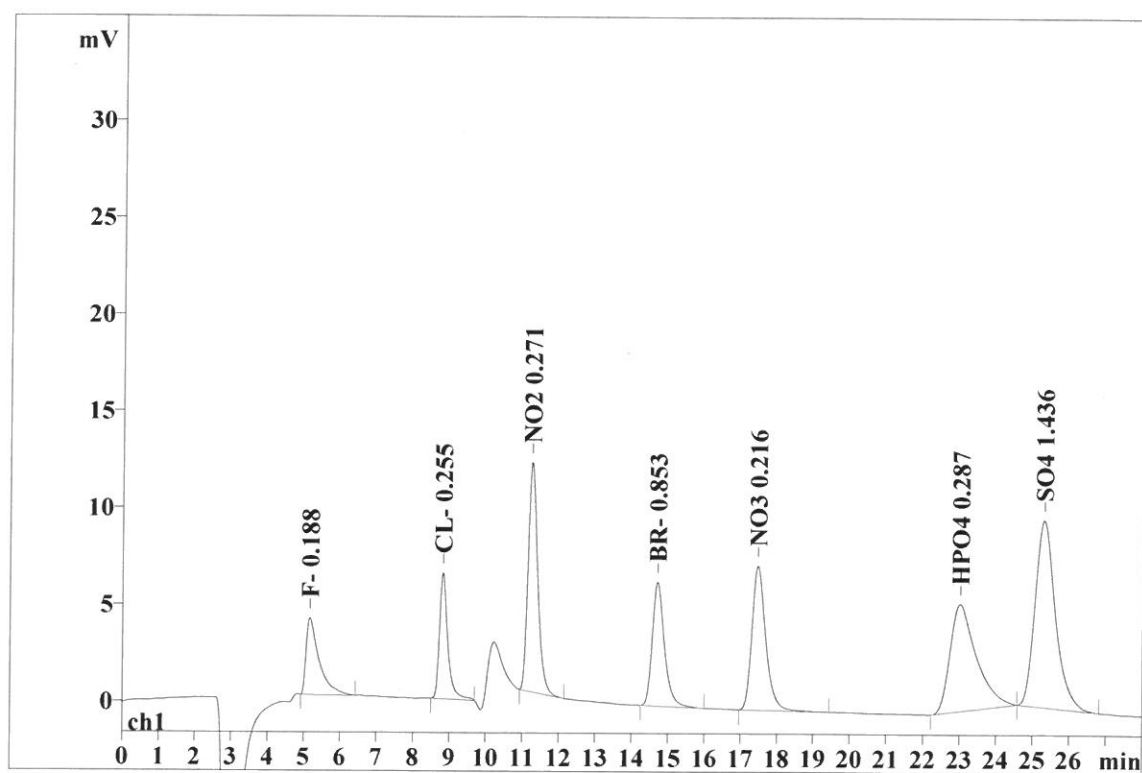

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.16	0.344	3.97	7.73	98.702	6.92
2	8.81	0.226	6.50	12.64	104.138	7.31
3	11.26	0.274	11.85	23.06	216.309	15.18
4	14.70	0.347	6.40	12.46	150.591	10.56
5	17.47	0.397	7.45	14.49	200.017	14.03
6	23.01	0.748	5.55	10.79	279.664	19.62
7	25.30	0.581	9.67	18.81	375.991	26.38
7	28.00	0.417	51.39	99.98	1425.413	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/7/2017 9:21:13 AM
Printed by: wet


Ident: STD3
Analysis from: 9/6/2017 1:55:42 PM
File: _2017-09-06_

Last save: 9/6/2017 2:23:42 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14941

Last save: 9/6/2017 1:52:4

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

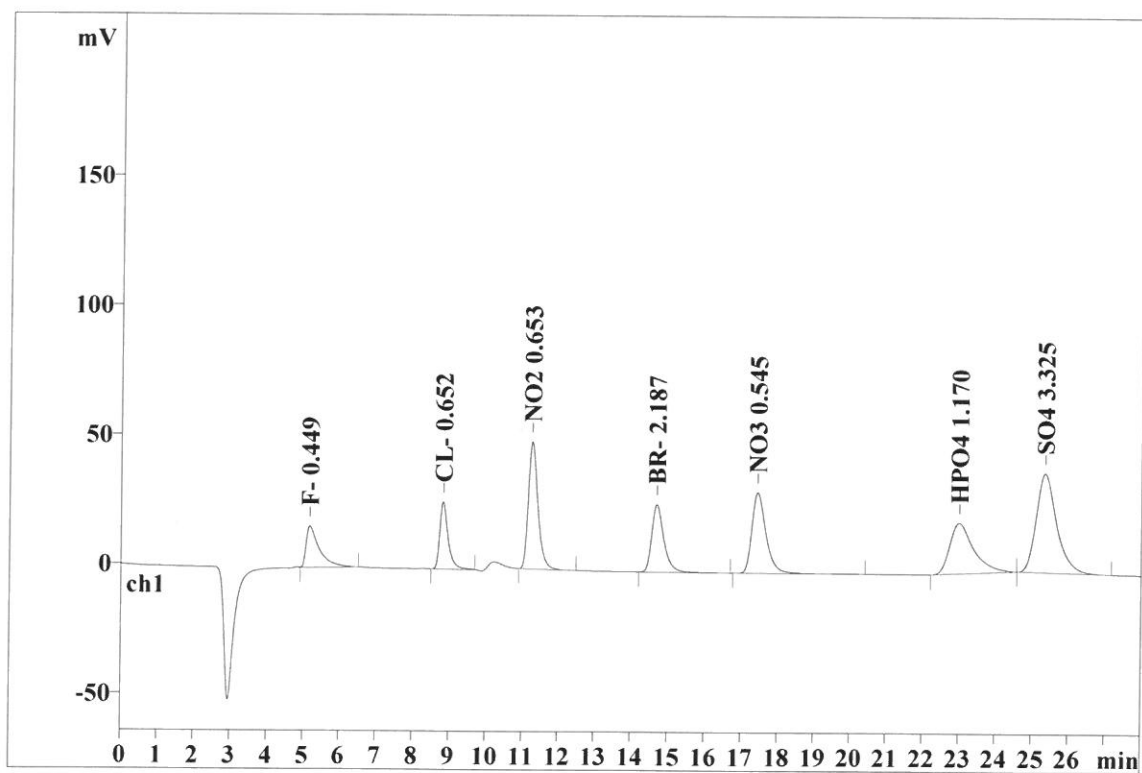

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.17	0.344	15.93	7.72	399.537	7.17
2	8.83	0.226	25.94	12.58	408.636	7.33
3	11.27	0.274	49.19	23.85	907.438	16.29
4	14.69	0.344	26.11	12.66	612.850	11.00
5	17.44	0.396	31.16	15.11	838.344	15.05
6	23.00	0.667	19.61	9.51	902.076	16.19
7	25.36	0.583	38.29	18.56	1502.474	26.97
7	28.00	0.405	206.23	100.00	5571.355	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/7/2017 9:21:30 AM
Printed by: wet


Ident: STD4
Analysis from: 9/6/2017 2:26:40 PM
File: _2017-09-06_

Last save: 9/6/2017 2:54:40 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14942

Last save: 9/6/2017 2:23:4

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

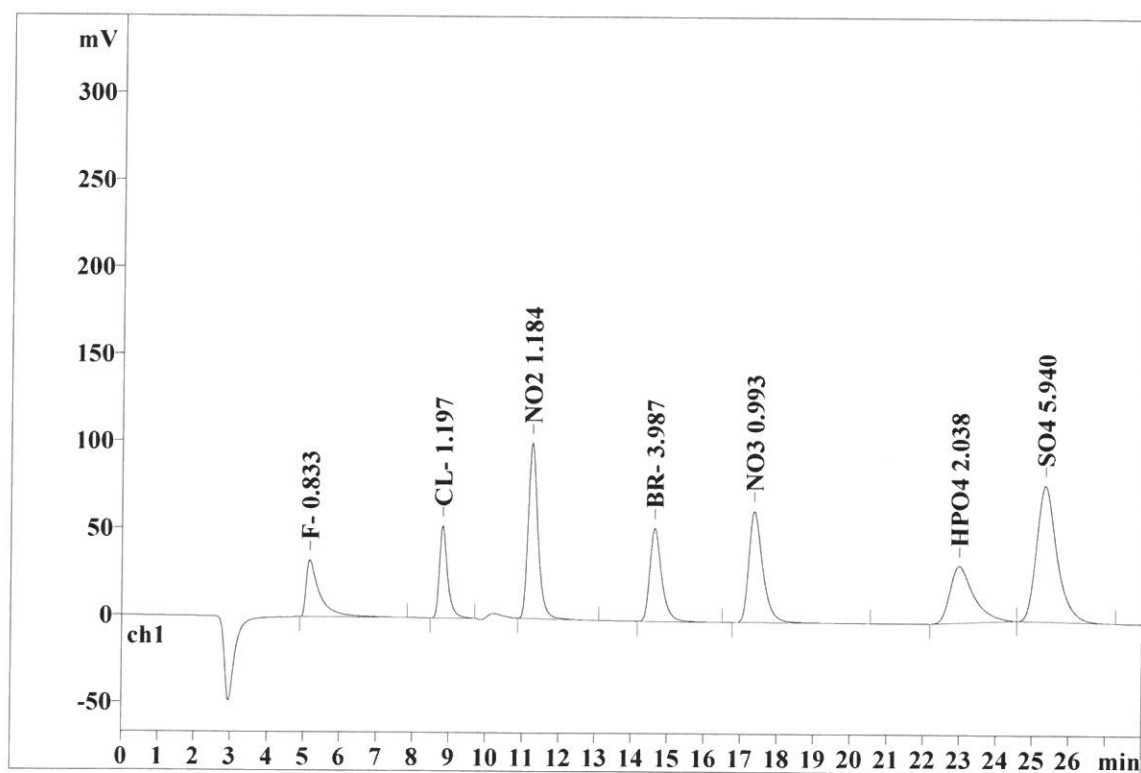

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.16	0.333	32.75	7.90	854.105	7.72
2	8.81	0.224	52.96	12.77	827.206	7.48
3	11.25	0.274	100.77	24.31	1870.039	16.91
4	14.63	0.340	53.42	12.89	1234.737	11.17
5	17.36	0.393	63.91	15.42	1711.595	15.48
6	22.98	0.666	32.62	7.87	1493.413	13.51
7	25.34	0.581	78.11	18.84	3066.798	27.73
7	28.00	0.402	414.54	100.00	11057.893	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/7/2017 9:22:21 AM
Printed by: wet


Ident: STD5
Analysis from: 9/6/2017 2:57:38 PM
File: _2017-09-06_

Last save: 9/6/2017 3:25:38 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14943

Last save: 9/6/2017 2:54:4

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

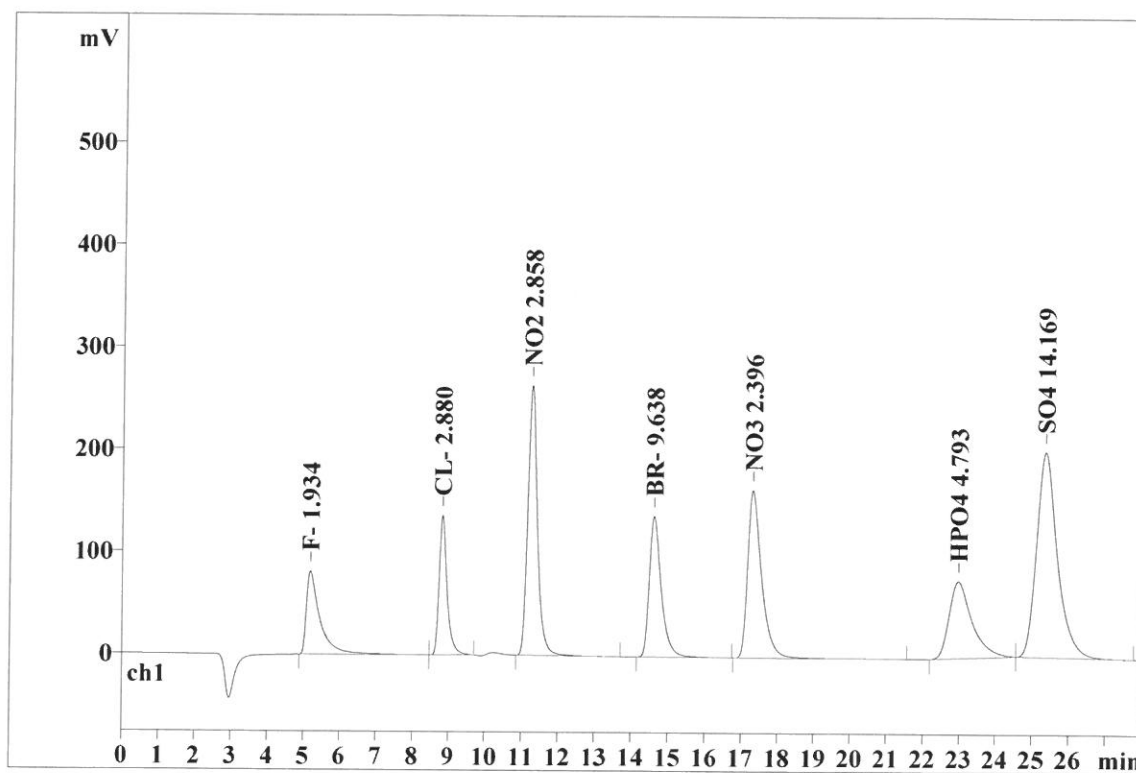

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.18	0.349	81.52	7.69	2148.825	7.68
2	8.81	0.222	136.57	12.89	2110.274	7.54
3	11.26	0.270	264.19	24.93	4871.620	17.41
4	14.60	0.337	137.52	12.97	3171.739	11.34
5	17.31	0.393	163.93	15.47	4424.194	15.81
6	22.96	0.641	75.28	7.10	3315.395	11.85
7	25.35	0.583	200.84	18.95	7937.715	28.37
7	28.00	0.399	1059.85	100.00	27979.762	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/7/2017 9:22:43 AM
Printed by: wet


Ident: STD6
Analysis from: 9/6/2017 3:28:35 PM
File: _2017-09-06_

Last save: 9/6/2017 3:56:36 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14944

Last save: 9/6/2017 3:25:3

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

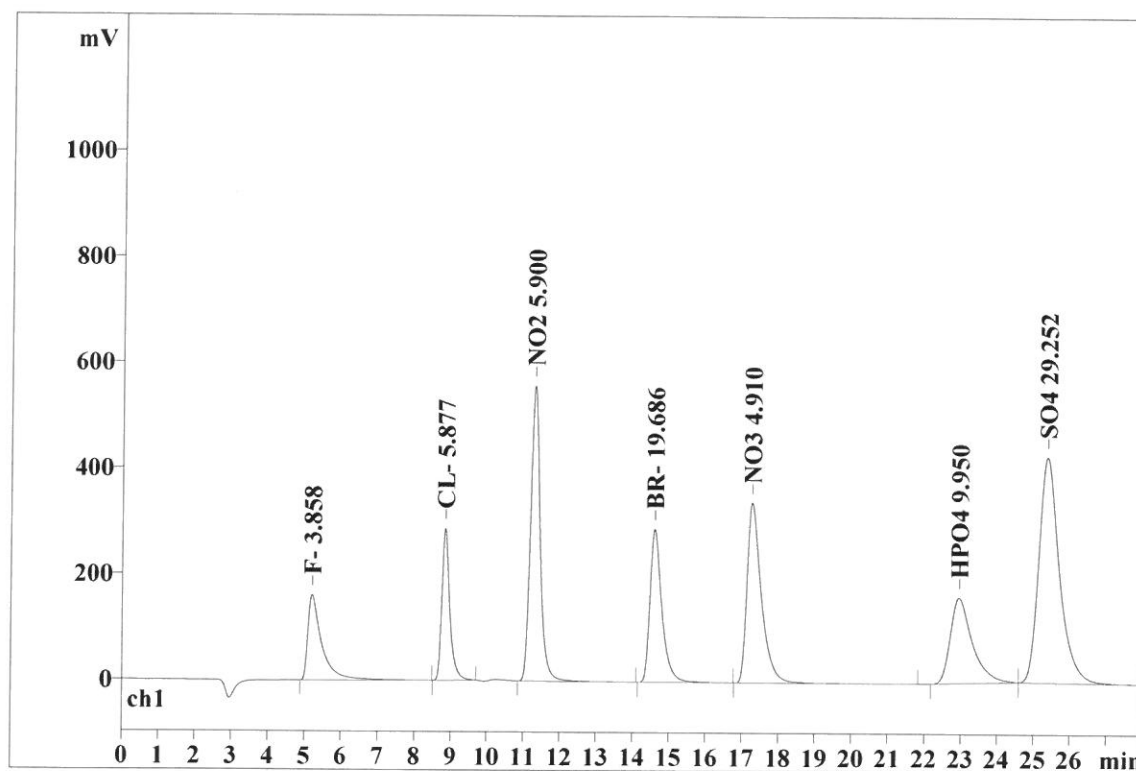

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.20	0.354	161.50	7.26	4316.075	7.36
2	8.83	0.219	287.48	12.92	4394.234	7.49
3	11.30	0.272	559.06	25.12	10355.943	17.65
4	14.59	0.333	288.97	12.98	6629.607	11.30
5	17.27	0.395	340.28	15.29	9300.655	15.85
6	22.94	0.612	162.03	7.28	6828.181	11.64
7	25.36	0.582	426.39	19.16	16855.186	28.72
7	28.00	0.395	2225.72	100.00	58679.880	100.00

Report date: 9/7/2017 9:22:58 AM
Printed by: wet


Ident: STD7
Analysis from: 9/6/2017 3:59:35 PM
File: _2017-09-06_

Last save: 9/6/2017 4:27:36 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14945

Last save: 9/6/2017 3:56:3

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

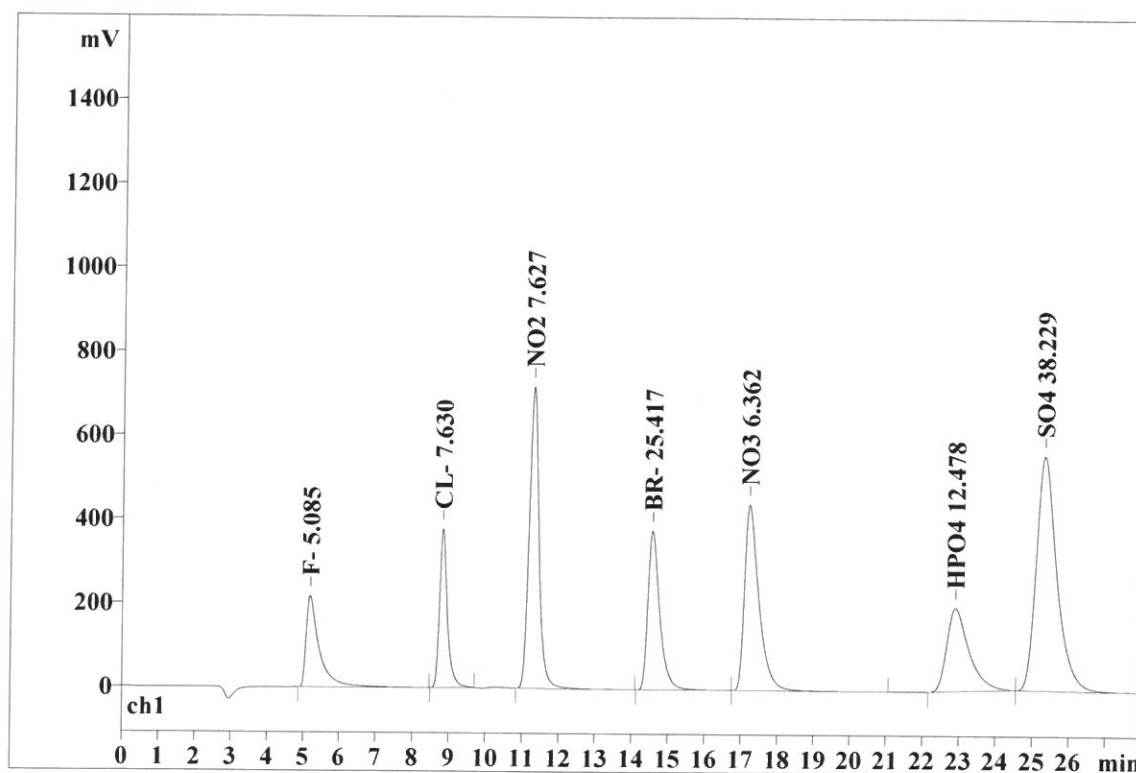

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.19	0.339	217.54	7.52	5639.351	7.42
2	8.81	0.217	378.11	13.07	5717.883	7.53
3	11.29	0.276	719.34	24.86	13447.469	17.70
4	14.56	0.330	378.80	13.09	8608.982	11.33
5	17.21	0.395	442.58	15.29	12119.055	15.96
6	22.89	0.617	198.45	6.86	8398.010	11.06
7	25.32	0.581	558.93	19.31	22023.051	29.00
7	28.00	0.393	2893.76	100.00	75953.801	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/7/2017 9:23:28 AM
Printed by: wet


Ident: ICV
Analysis from: 9/6/2017 5:32:53 PM
File: _2017-09-06_

Last save: 9/6/2017 6:00:54 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14948

Last save: 9/6/2017 4:27:3

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

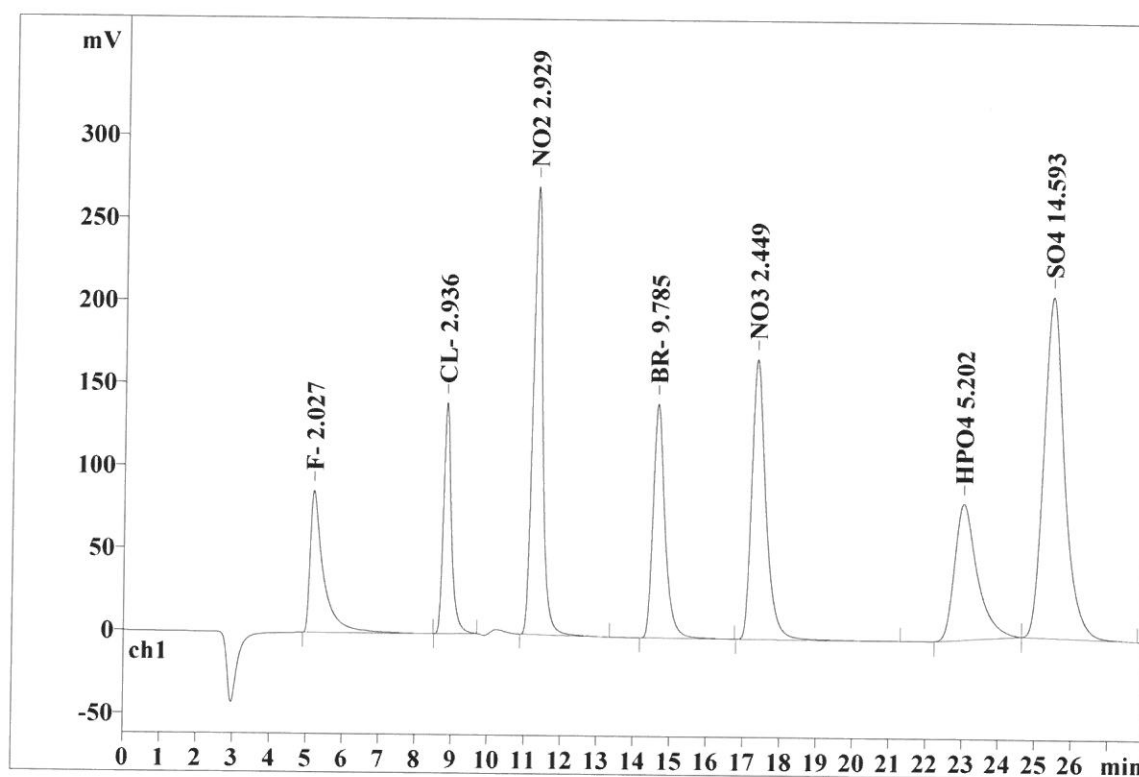

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.18	0.331	85.87	7.83	2217.221	7.66
2	8.83	0.222	139.76	12.74	2155.216	7.45
3	11.29	0.272	271.26	24.73	5015.309	17.34
4	14.62	0.335	141.70	12.92	3241.735	11.21
5	17.33	0.391	169.53	15.45	4545.414	15.71
6	23.01	0.633	82.29	7.50	3586.874	12.40
7	25.43	0.585	206.51	18.83	8168.246	28.23
7	28.00	0.396	1096.92	100.00	28930.015	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/7/2017 9:23:44 AM
Printed by: wet


Ident: ICB
Analysis from: 9/6/2017 6:03:51 PM
File: _2017-09-06_

Last save: 9/6/2017 6:31:51 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 14949

Last save: 9/6/2017 4:27:3

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

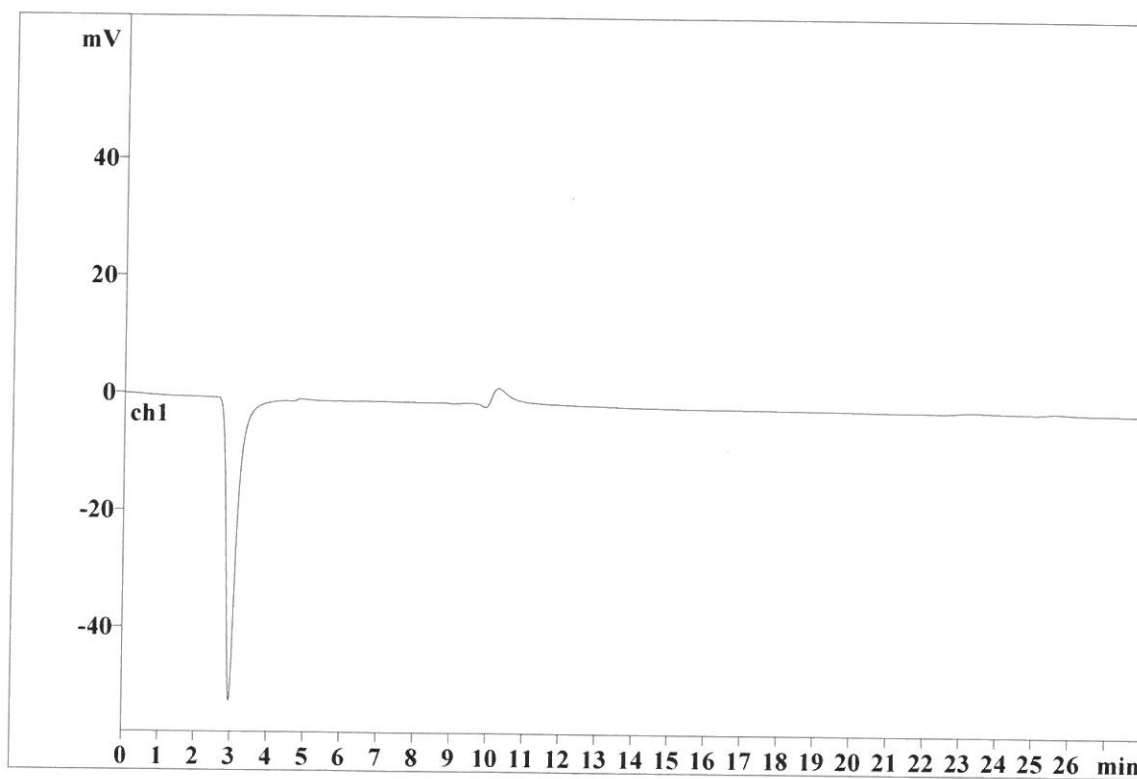

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:19:01 PM
Printed by: wet


Ident: CCV
Analysis from: 9/19/2017 9:33:56 AM
File: _2017-09-19_

Last save: 10/11/2017 5:19:01 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15025

Last save: 9/6/2017 4:27:3

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

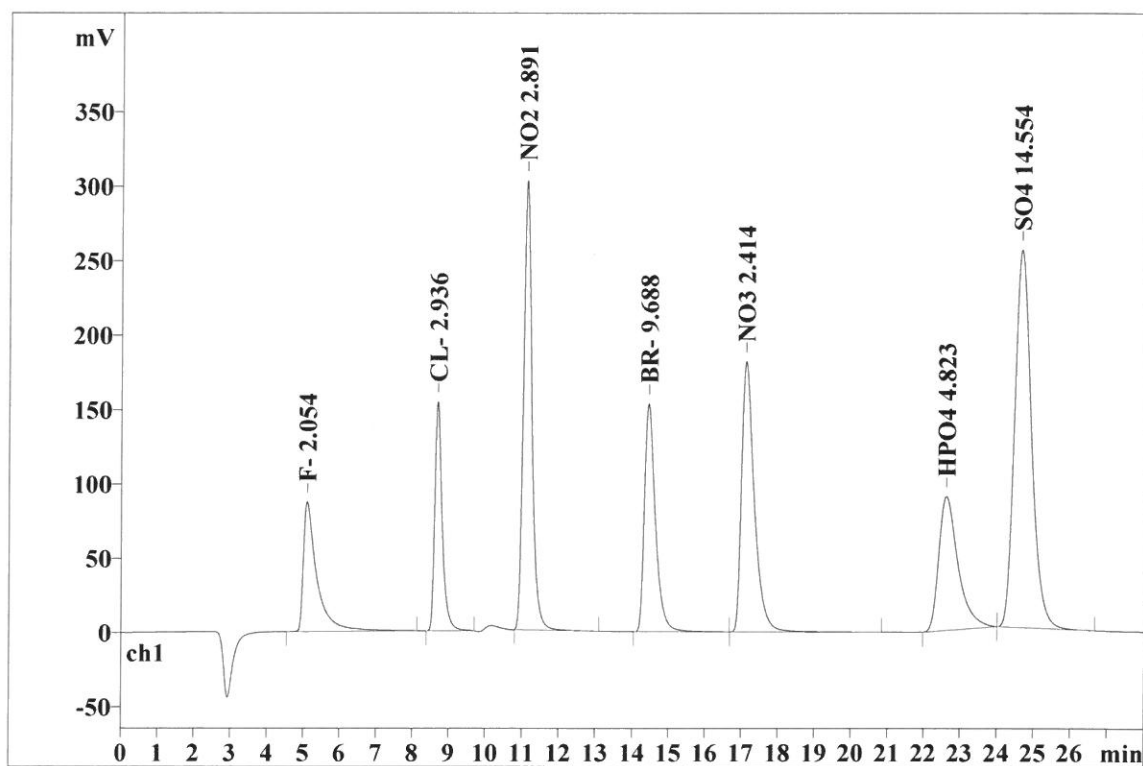

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.334	87.30	7.14	2246.726	7.88
2	8.69	0.201	154.28	12.61	2154.793	7.56
3	11.12	0.243	302.14	24.70	4947.219	17.35
4	14.44	0.308	153.40	12.54	3208.492	11.25
5	17.12	0.364	181.67	14.85	4477.342	15.70
6	22.62	0.543	90.21	7.38	3336.310	11.70
7	24.67	0.486	253.99	20.77	8145.680	28.56
7	28.00	0.354	1222.98	100.00	28516.562	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:19:07 PM
Printed by: wet


Ident: CCB
Analysis from: 9/19/2017 10:04:51 AM
File: _2017-09-19_

Last save: 9/19/2017 10:32:51 AM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15026

Last save: 9/6/2017 4:27:3

SAMPLE:
:
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

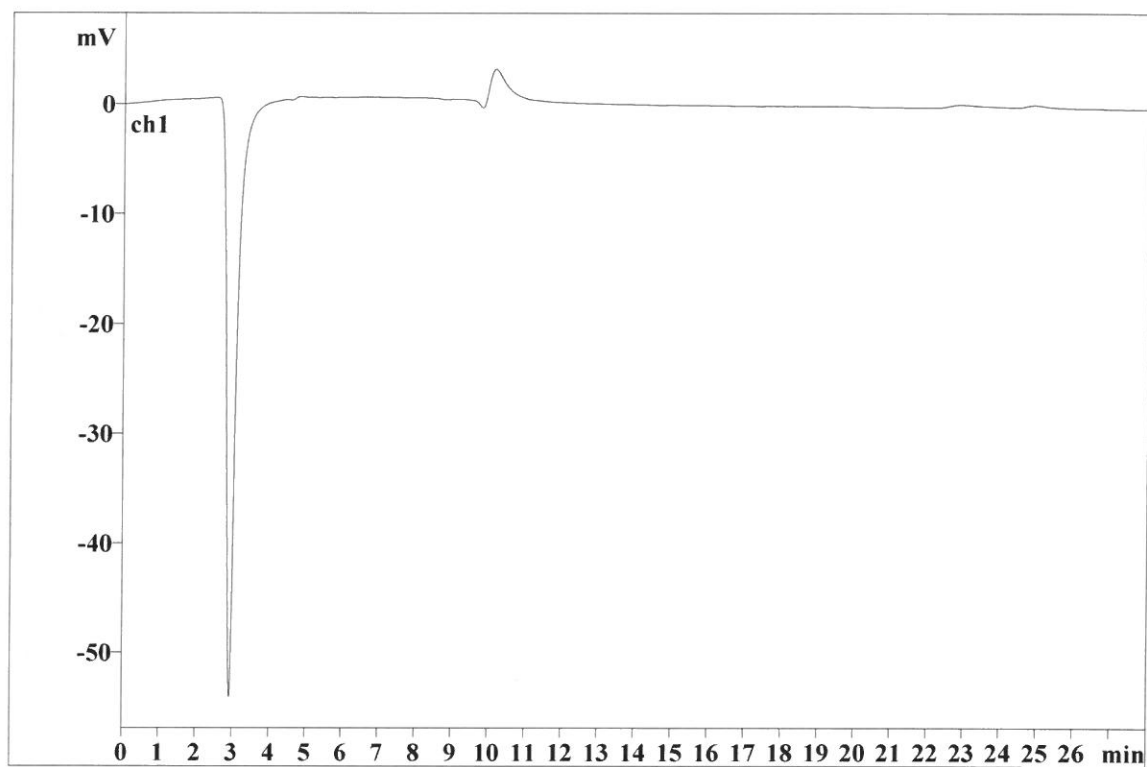

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:19:13 PM
Printed by: wet


Ident: LB90750BLS
Analysis from: 9/19/2017 10:35:46 AM
File: _2017-09-19_

Last save: 10/11/2017 5:18:46 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15027

Last save: 9/6/2017 4:27:3

SAMPLE: 5.01g
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

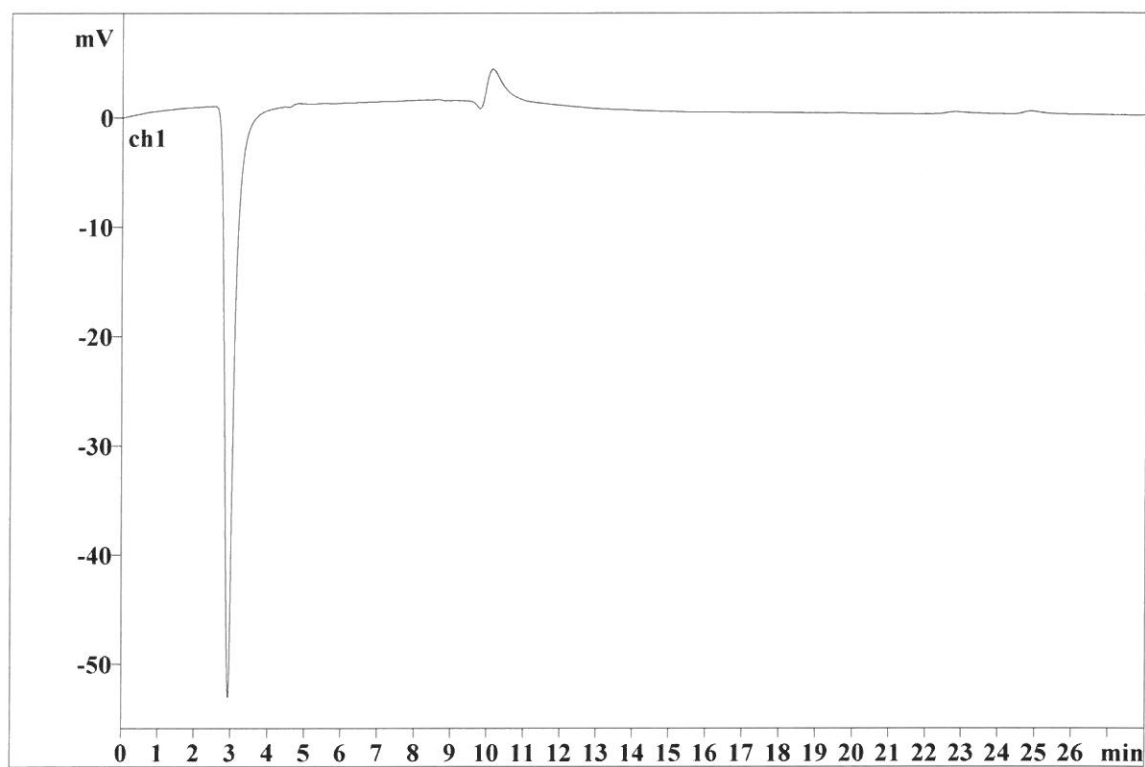

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:19:20 PM
Printed by: wet


Ident: LB90750BSS
Analysis from: 9/19/2017 11:06:42 AM
File: _2017-09-19_

Last save: 10/11/2017 5:18:46 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15028

Last save: 9/6/2017 4:27:3

SAMPLE: 5.00g
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

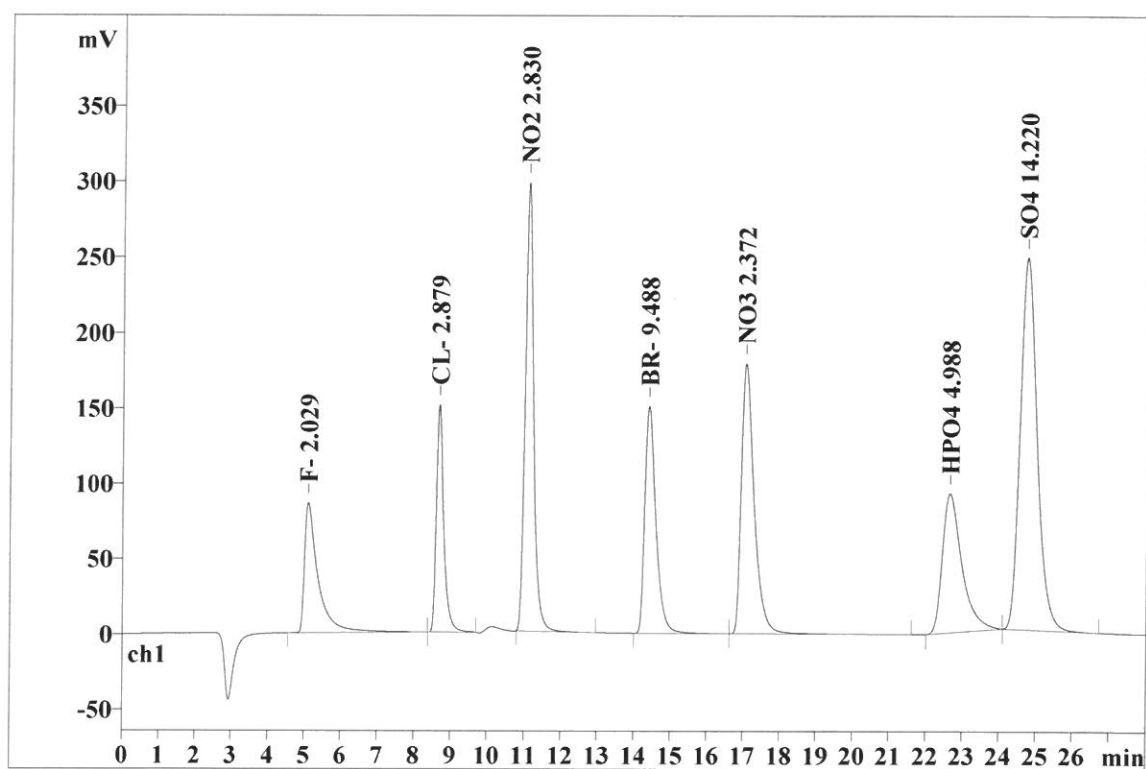

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.330	86.52	7.19	2219.777	7.90
2	8.69	0.200	151.24	12.56	2111.433	7.51
3	11.11	0.241	297.06	24.68	4838.320	17.22
4	14.40	0.307	150.81	12.53	3139.764	11.17
5	17.06	0.361	179.26	14.89	4396.774	15.65
6	22.66	0.545	92.37	7.67	3445.286	12.26
7	24.75	0.488	246.51	20.48	7949.957	28.29
7	28.00	0.353	1203.77	100.00	28101.311	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:19:39 PM
Printed by: wet


Ident: I5275-01
Analysis from: 9/19/2017 11:37:40 AM
File: _2017-09-19_

Last save: 10/11/2017 5:14:13 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15029

Last save: 9/6/2017 4:27:3

SAMPLE: 5.02g
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

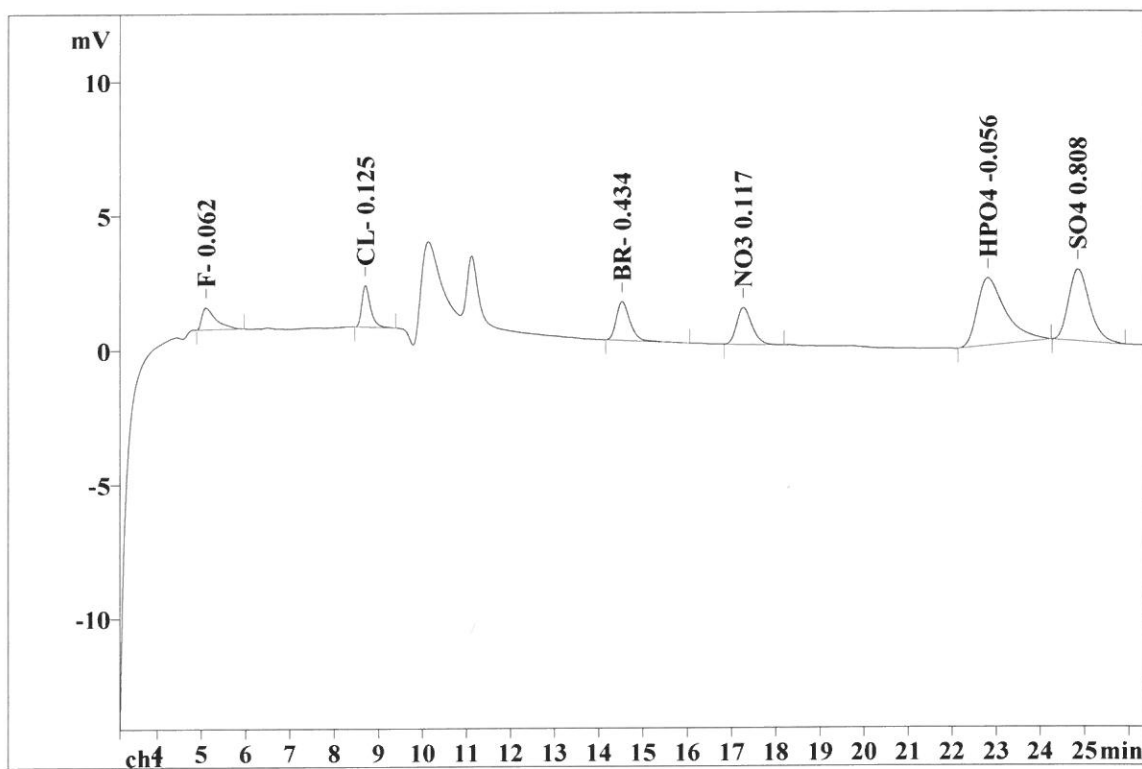

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.307	0.82	7.90	18.143	6.01
2	8.70	0.201	1.54	14.92	21.193	7.01
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.53	0.321	1.43	13.89	31.105	10.30
5	17.26	0.367	1.37	13.24	32.861	10.88
6	22.80	0.644	2.50	24.22	110.699	36.64
7	24.85	0.507	2.66	25.72	88.122	29.17
7	28.00	0.335	10.31	99.88	302.122	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:19:53 PM
Printed by: wet


Ident: I5275-02
Analysis from: 9/19/2017 12:08:36 PM
File: _2017-09-19_

Last save: 10/11/2017 5:19:52 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15030

Last save: 9/6/2017 4:27:3

SAMPLE: 5.01g
: AK/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

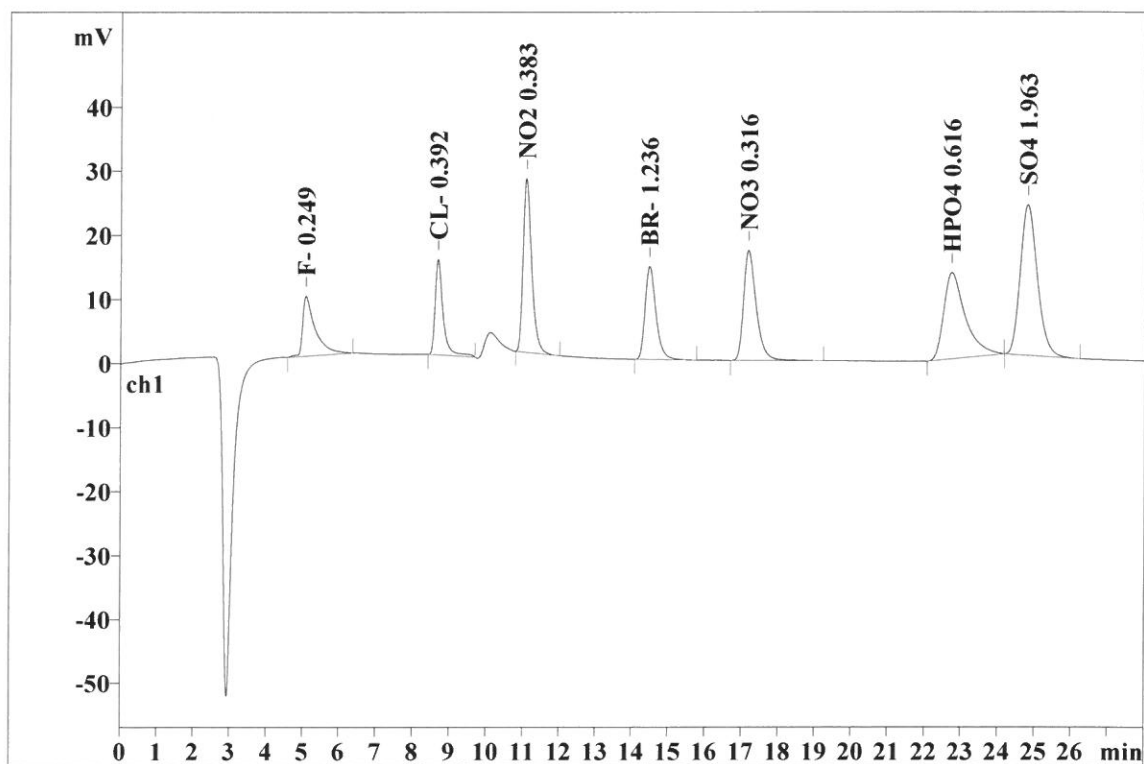

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.317	9.37	7.80	227.334	7.72
2	8.69	0.206	14.90	12.41	224.143	7.61
3	11.10	0.247	27.11	22.57	447.609	15.21
4	14.48	0.314	14.54	12.11	306.333	10.41
5	17.19	0.362	17.18	14.31	418.533	14.22
6	22.75	0.598	13.48	11.23	554.477	18.84
7	24.81	0.497	23.49	19.56	765.284	26.00
7	28.00	0.363	120.07	100.00	2943.712	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:19:58 PM
Printed by: wet


Ident: CCV
Analysis from: 9/19/2017 12:39:38 PM
File: _2017-09-19_

Last save: 9/19/2017 2:30:49 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15031

Last save: 9/6/2017 4:27:3

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

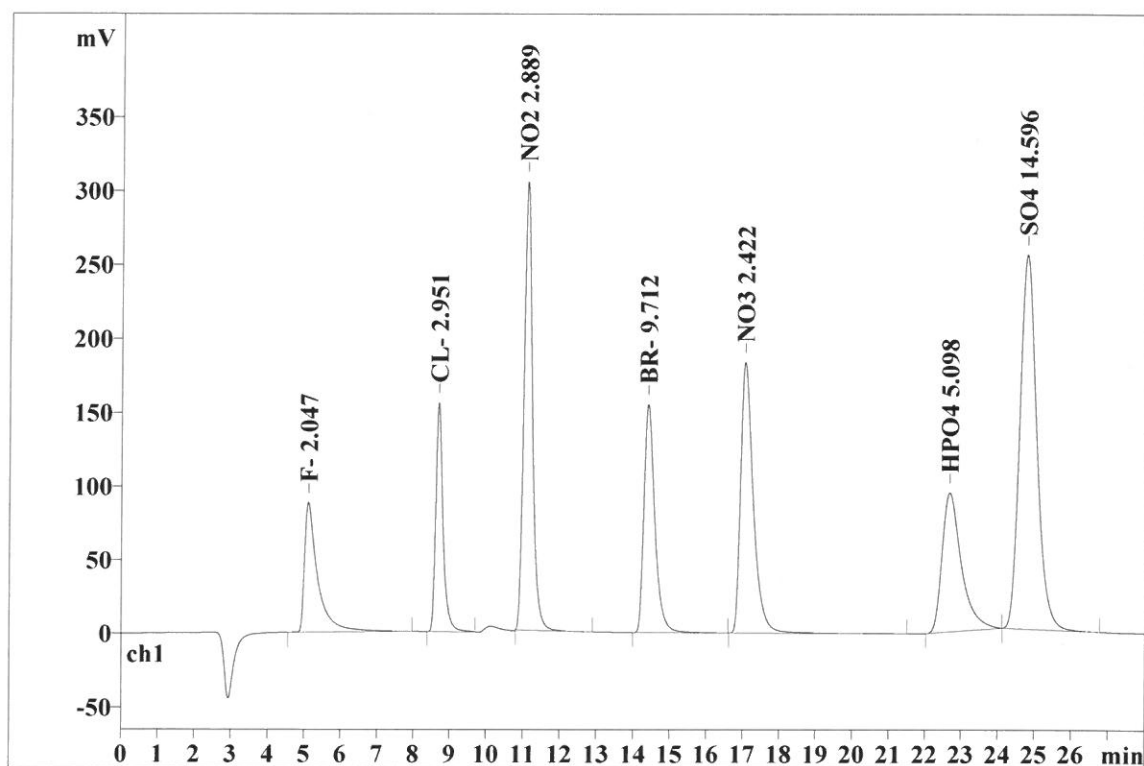

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.328	88.43	7.15	2238.939	7.79
2	8.69	0.200	155.76	12.60	2166.296	7.54
3	11.11	0.241	304.53	24.64	4944.384	17.20
4	14.40	0.306	155.12	12.55	3216.708	11.19
5	17.05	0.361	183.80	14.87	4493.850	15.63
6	22.67	0.543	94.71	7.66	3518.449	12.24
7	24.78	0.488	253.60	20.52	8170.010	28.42
7	28.00	0.352	1235.95	100.00	28748.635	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2017 5:20:04 PM
Printed by: wet


Ident: CCB
Analysis from: 9/19/2017 1:10:33 PM
File: _2017-09-19_

Last save: 9/19/2017 1:38:33 PM

Method: AnionsIC2-090617.mtw
Run operator: wet
Analysis number: 15032

Last save: 9/6/2017 4:27:3

SAMPLE:
:
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

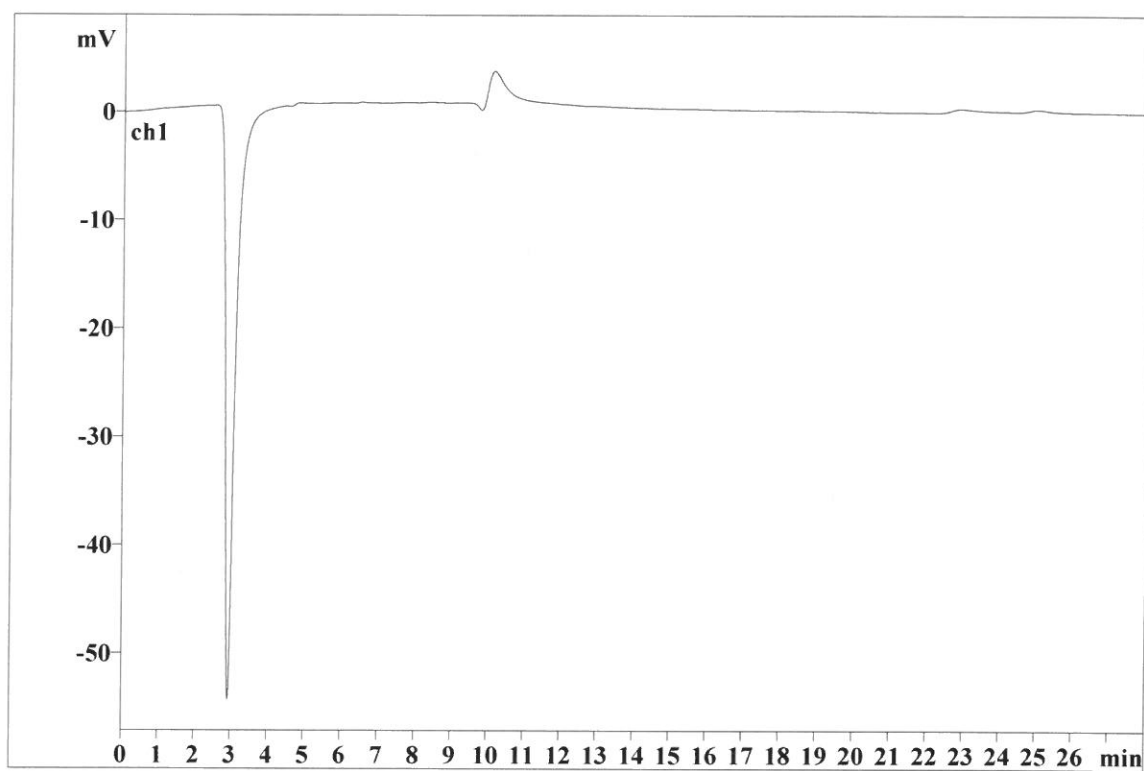

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD