

7470A


LB 90 865

INSTRUMENT ID: CW-1

Linear

 μ Abs.:

34090

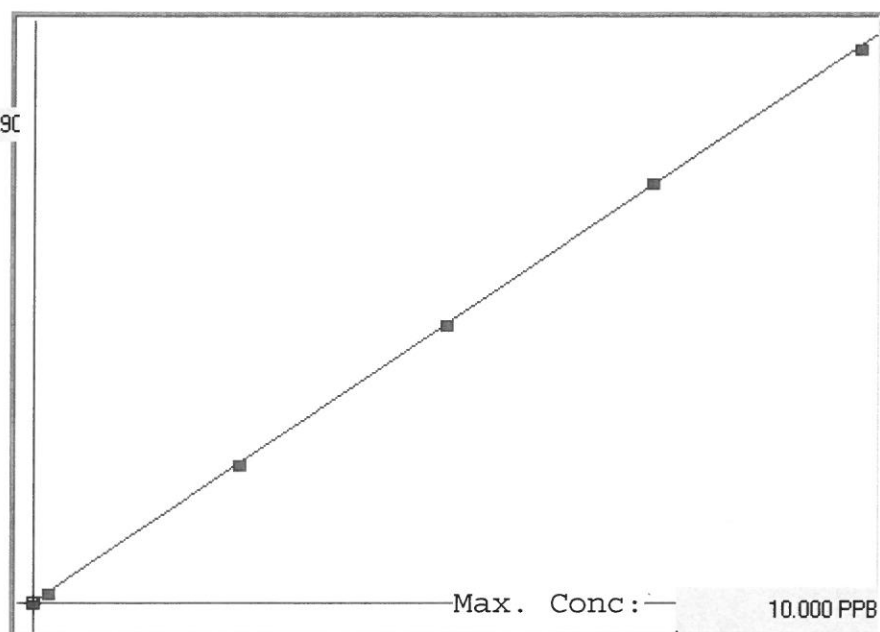

A= 0.0000e+000

B= 2.9214e-004

C= -8.5149e-003

Rho= 0.9999570

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.008	0.008	58	0.000	58				
0.2	0.200	0.180	-0.020	644	0.0 %	644				
2.5	2.500	2.488	-0.012	8547	0.0 %	8547				
5.0	5.000	5.011	0.011	17181	0.0 %	17181				
7.5	7.500	7.562	0.062	25914	0.0 %	25914				
10.0	10.000	9.951	-0.049	34090	0.0 %	34090				

LB90865 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Oct 2017 09:28:41

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	58	-	0.00007470A	PPB	17 Oct 2017 09:49:32	S	Std
0.2 - 1	50.2	644	-	0.20007470A	PPB	17 Oct 2017 09:51:41	S	Std
2.5 - 1	52.5	8547	-	2.50007470A	PPB	17 Oct 2017 09:53:49	S	Std
5.0 - 1	55	17181	-	5.00007470A	PPB	17 Oct 2017 09:55:57	S	Std
7.5 - 1	57.5	25914	-	7.50007470A	PPB	17 Oct 2017 09:58:05	S	Std
10.0 - 1	510	34090	-	10.00007470A	PPB	17 Oct 2017 10:00:13	S	Std
ICV13 - 1	ICV13	13335	3.8872	-7470A	PPB	17 Oct 2017 10:02:50	U	SMPL
ICB13 - 1	ICB13	-104	-0.0389	-7470A	PPB	17 Oct 2017 10:04:56	U	SMPL
CCV23 - 1	CCV23	17863	5.2100	-7470A	PPB	17 Oct 2017 10:07:03	U	SMPL
CCB23 - 1	CCB23	-118	-0.0430	-7470A	PPB	17 Oct 2017 10:09:10	U	SMPL
CRA - 1	CRA	656	0.1831	-7470A	PPB	17 Oct 2017 10:11:17	U	SMPL
HighStd - 1	HighStd	33922	9.9016	-7470A	PPB	17 Oct 2017 10:13:23	U	SMPL
ChkStd - 1	ChkStd	23460	6.8452	-7470A	PPB	17 Oct 2017 10:17:59	U	SMPL
PB103343BL - 1	PBW	-155	-0.0538	-7470A	PPB	17 Oct 2017 10:20:06	U	SMPL
PB103343BS - 1	LCSW	12636	3.6830	-7470A	PPB	17 Oct 2017 10:22:15	U	SMPL
PB103343TB - 1	PB103228TB	-67	-0.0281	-7470A	PPB	17 Oct 2017 10:24:23	U	SMPL
I5833-04 - 1	WC-101117-SOIL	32	0.0008	-7470A	PPB	17 Oct 2017 10:26:31	U	SMPL
I5841-03 - 1	TR-04-101217	32	0.0008	-7470A	PPB	17 Oct 2017 10:28:39	U	SMPL
I5841-03DUP - 1	TR-04-101217DUP	48	0.0055	-7470A	PPB	17 Oct 2017 10:30:48	U	SMPL
I5841-03MS - 1	TR-04-101217MS	12645	3.6856	-7470A	PPB	17 Oct 2017 10:32:55	U	SMPL
CCV24 - 1	CCV24	17509	5.1066	-7470A	PPB	17 Oct 2017 10:35:01	U	SMPL
CCB24 - 1	CCB24	-96	-0.0366	-7470A	PPB	17 Oct 2017 10:37:08	U	SMPL
I5841-03MSD - 1	TR-04-101217MSD	12426	3.6217	-7470A	PPB	17 Oct 2017 10:39:15	U	SMPL
I5875-02 - 1	TK2064L-T1-T2-T3	-73	-0.0298	-7470A	PPB	17 Oct 2017 10:41:22	U	SMPL
I5890-18 - 1	ENGERT-COMP-1	40	0.0032	-7470A	PPB	17 Oct 2017 10:43:29	U	SMPL
I5890-19 - 1	ENGERT-COMP-2	104	0.0219	-7470A	PPB	17 Oct 2017 10:45:36	U	SMPL
I5896-03 - 1	B-19(0-10)COMP	49	0.0058	-7470A	PPB	17 Oct 2017 10:47:44	U	SMPL
I5898-03 - 1	OR-02-101317	37	0.0023	-7470A	PPB	17 Oct 2017 10:49:52	U	SMPL
I5899-02 - 1	72-12020	43	0.0040	-7470A	PPB	17 Oct 2017 10:52:00	U	SMPL
I5905-01 - 1	SOIL-CUTTINGS-9601	46	0.0049	-7470A	PPB	17 Oct 2017 10:54:08	U	SMPL
I5905-02 - 1	SOIL-CUTTINGS-9698	50	0.0061	-7470A	PPB	17 Oct 2017 10:56:17	U	SMPL
I5907-02 - 1	CONCRETE-FOUNDATION-COMP	73	0.0128	-7470A	PPB	17 Oct 2017 10:58:24	U	SMPL
CCV25 - 1	CCV25	17383	5.0698	-7470A	PPB	17 Oct 2017 11:00:31	U	SMPL
CCB25 - 1	CCB25	-89	-0.0345	-7470A	PPB	17 Oct 2017 11:02:38	U	SMPL
I5908-03 - 1	T2-T3-COMP	42	0.0038	-7470A	PPB	17 Oct 2017 11:04:46	U	SMPL
PB103344BL - 1	PBW	60	0.0090	-7470A	PPB	17 Oct 2017 11:06:53	U	SMPL
PB103344BS - 1	LCSW	12492	3.6409	-7470A	PPB	17 Oct 2017 11:09:00	U	SMPL
PB103344TB - 1	PB103269TB	-41	-0.0205	-7470A	PPB	17 Oct 2017 11:11:07	U	SMPL
I5906-11 - 1	WH-TWS-01	66	0.0108	-7470A	PPB	17 Oct 2017 11:13:15	U	SMPL
I5906-12 - 1	WH-TWS-02	61	0.0093	-7470A	PPB	17 Oct 2017 11:15:22	U	SMPL
I5906-13 - 1	WH-TWS-03	58	0.0084	-7470A	PPB	17 Oct 2017 11:17:31	U	SMPL
I5906-14 - 1	WH-TWS-04	98	0.0201	-7470A	PPB	17 Oct 2017 11:19:39	U	SMPL
I5906-15 - 1	WH-TWS-05	82	0.0154	-7470A	PPB	17 Oct 2017 11:21:48	U	SMPL
I5906-16 - 1	WH-TWS-06	66	0.0108	-7470A	PPB	17 Oct 2017 11:23:55	U	SMPL
CCV26 - 1	CCV26	17102	4.9877	-7470A	PPB	17 Oct 2017 11:26:02	U	SMPL
CCB26 - 1	CCB26	-90	-0.0348	-7470A	PPB	17 Oct 2017 11:28:09	U	SMPL
I5906-17 - 1	WH-TWS-07	19	-0.0030	-7470A	PPB	17 Oct 2017 11:30:16	U	SMPL
I5906-18 - 1	WH-TWS-08	29	-0.0000	-7470A	PPB	17 Oct 2017 11:32:23	U	SMPL
I5906-19 - 1	WH-TWS-09	52	0.0067	-7470A	PPB	17 Oct 2017 11:34:31	U	SMPL
I5906-20 - 1	WH-TWS-10	122	0.0271	-7470A	PPB	17 Oct 2017 11:36:38	U	SMPL
I5906-20DUP - 1	WH-TWS-10DUP	130	0.0295	-7470A	PPB	17 Oct 2017 11:38:45	U	SMPL
I5906-20MS - 1	WH-TWS-10MS	12455	3.6301	-7470A	PPB	17 Oct 2017 11:40:53	U	SMPL
I5906-20MSD - 1	WH-TWS-10MSD	12162	3.5445	-7470A	PPB	17 Oct 2017 11:43:01	U	SMPL
CCV27 - 1	CCV27	17192	5.0140	-7470A	PPB	17 Oct 2017 11:45:10	U	SMPL
CCB27 - 1	CCB27	-91	-0.0351	-7470A	PPB	17 Oct 2017 11:47:18	U	SMPL
I5841-03LX5 - 1		60	0.0090	-7470A	PPB	17 Oct 2017 11:49:26	U	SMPL
I5841-03A - 1		13334	3.8869	-7470A	PPB	17 Oct 2017 11:51:33	U	SMPL
I5906-20LX5 - 1		-67	-0.0281	-7470A	PPB	17 Oct 2017 11:53:41	U	SMPL
I5906-20A - 1		13554	3.9512	-7470A	PPB	17 Oct 2017 11:55:48	U	SMPL
CCV28 - 1	CCV28	17304	5.0467	-7470A	PPB	17 Oct 2017 11:57:56	U	SMPL
CCB28 - 1	CCB28	-113	-0.0415	-7470A	PPB	17 Oct 2017 12:00:03	U	SMPL