


ISM02.4

LB 90878
INSTRUMENT ID: CV1

Linear

 μ Abs.:

45492

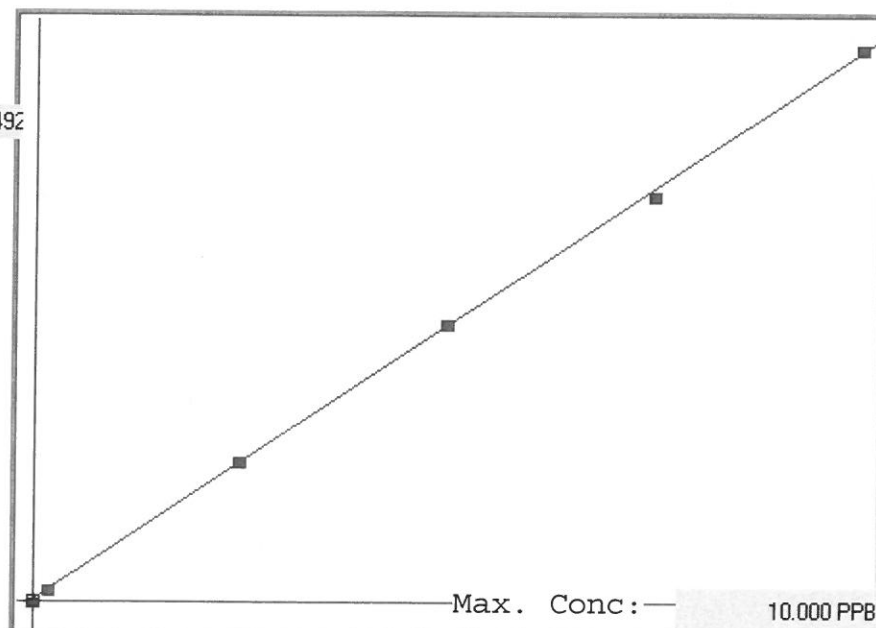

A= 0.0000e+000

B= 2.2153e-004

C= -2.5242e-002

Rho= 0.9999069

Accept=Accepted

done
y=1.51e5x

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	-0.011	-0.011	63	0.000	63					1
0.2	0.200	0.201	0.001	1023	0.0 %	1023					1
2.5	2.500	2.528	0.028	11527	0.0 %	11527					1
5.0	5.000	5.032	0.032	22828	0.0 %	22828					1
7.5	7.500	7.397	-0.103	33507	0.0 %	33507					1
10.0	10.000	10.052	0.052	45492	0.0 %	45492					1

NB
10/17/13

LB90878
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	63	-		0 ISM02.4	PPB	10/17/2017 15:07	Std
	0.2 S0.2	1023	-		0.2 ISM02.4	PPB	10/17/2017 15:09	Std
	2.5 S2.5	11527	-		2.5 ISM02.4	PPB	10/17/2017 15:11	Std
	5 S5	22828	-		5 ISM02.4	PPB	10/17/2017 15:14	Std
	7.5 S7.5	33507	-		7.5 ISM02.4	PPB	10/17/2017 15:16	Std
	10 S10	45492	-		10 ISM02.4	PPB	10/17/2017 15:21	Std
ICV	ICV	17475	3.8459	-	ISM02.4	PPB	10/17/2017 15:24	SMPL
ICB	ICB	-126	-0.0532	-	ISM02.4	PPB	10/17/2017 15:26	SMPL
CCV032	CCV032	22837	5.0338	-	ISM02.4	PPB	10/17/2017 15:28	SMPL
CCB032	CCB032	-122	-0.0523	-	ISM02.4	PPB	10/17/2017 15:30	SMPL
PB103283BL	PBS004	14	-0.0221	-	ISM02.4	PPB	10/17/2017 15:33	SMPL
I5826-01	B-67(2.5-3.8)-101017	5990	1.3017	-	ISM02.4	PPB	10/17/2017 15:35	SMPL
I5826-02	B-63(0-1)-101117	8133	1.7764	-	ISM02.4	PPB	10/17/2017 15:37	SMPL
I5826-03	B-63(1-3)-101117	3324	0.7111	-	ISM02.4	PPB	10/17/2017 15:39	SMPL
I5826-04	B-61(0-1)-101117	8437	1.8438	-	ISM02.4	PPB	10/17/2017 15:42	SMPL
I5826-05	B-61(5-6)-101117	1292	0.261	-	ISM02.4	PPB	10/17/2017 15:44	SMPL
I5826-06	B-62(0-1)-101117	6852	1.4927	-	ISM02.4	PPB	10/17/2017 15:46	SMPL
I5826-07	B-62(5-5.5)-101117	4797	1.0374	-	ISM02.4	PPB	10/17/2017 15:49	SMPL
I5826-08	B-64(1.5-2.5)-101117	7494	1.6349	-	ISM02.4	PPB	10/17/2017 15:51	SMPL
I5826-09	B-64(2.5-4.5)-101117	6257	1.3608	-	ISM02.4	PPB	10/17/2017 15:53	SMPL
I5826-10	DUP-5	8221	1.7959	-	ISM02.4	PPB	10/17/2017 15:55	SMPL
I5826-12	B-19(0-1)-101117	7568	1.6513	-	ISM02.4	PPB	10/17/2017 15:58	SMPL
I5826-13	B-19(0-1)-101117D	7676	1.6752	-	ISM02.4	PPB	10/17/2017 16:03	SMPL
I5826-14	B-19(0-1)-101117S	19807	4.3625	-	ISM02.4	PPB	10/17/2017 16:05	SMPL
PB103284BL	PBS004	-141	-0.0565	-	ISM02.4	PPB	10/17/2017 16:07	SMPL
I5873-01	B-19(2-4)_101117	7792	1.7009	-	ISM02.4	PPB	10/17/2017 16:10	SMPL
I5873-02	B-13(0-1)_101117	4810	1.0403	-	ISM02.4	PPB	10/17/2017 16:12	SMPL
I5873-03	B-13(1-3)_101117	26463	5.837	-	ISM02.4	PPB	10/17/2017 16:14	SMPL
I5873-04	B-16(0-1)_101217	5960	1.2951	-	ISM02.4	PPB	10/17/2017 16:17	SMPL
I5873-05	B-16(7-7.75)_1012117	7	-0.0237	-	ISM02.4	PPB	10/17/2017 16:19	SMPL
CCV033	CCV033	23215	5.1175	-	ISM02.4	PPB	10/17/2017 16:21	SMPL
CCB033	CCB033	-146	-0.0576	-	ISM02.4	PPB	10/17/2017 16:23	SMPL
I5873-06	B-18(0-1)_101217	13779	3.0272	-	ISM02.4	PPB	10/17/2017 16:26	SMPL
I5873-07	B-18(5-6)_101217	7988	1.7443	-	ISM02.4	PPB	10/17/2017 16:28	SMPL
I5902-01	B-5(0.5-1.5)-101317	5883	1.278	-	ISM02.4	PPB	10/17/2017 16:30	SMPL
I5902-02	B-5(5-6.5)-101317	2046	0.428	-	ISM02.4	PPB	10/17/2017 16:33	SMPL
I5902-03	B-12(0-1)-101317	37896	8.3697	-	ISM02.4	PPB	10/17/2017 16:35	SMPL
I5902-04	B-12(1-3)-101317	6248	1.3589	-	ISM02.4	PPB	10/17/2017 16:37	SMPL
I5902-05	B-65(0.5-1.5)-101317	2151	0.4513	-	ISM02.4	PPB	10/17/2017 16:39	SMPL
I5902-06	B-65(1.5-2.7)-101317	8076	1.7638	-	ISM02.4	PPB	10/17/2017 16:42	SMPL
CCV034	CCV034	22649	4.9921	-	ISM02.4	PPB	10/17/2017 16:44	SMPL
CCB034	CCB034	-148	-0.058	-	ISM02.4	PPB	10/17/2017 16:46	SMPL