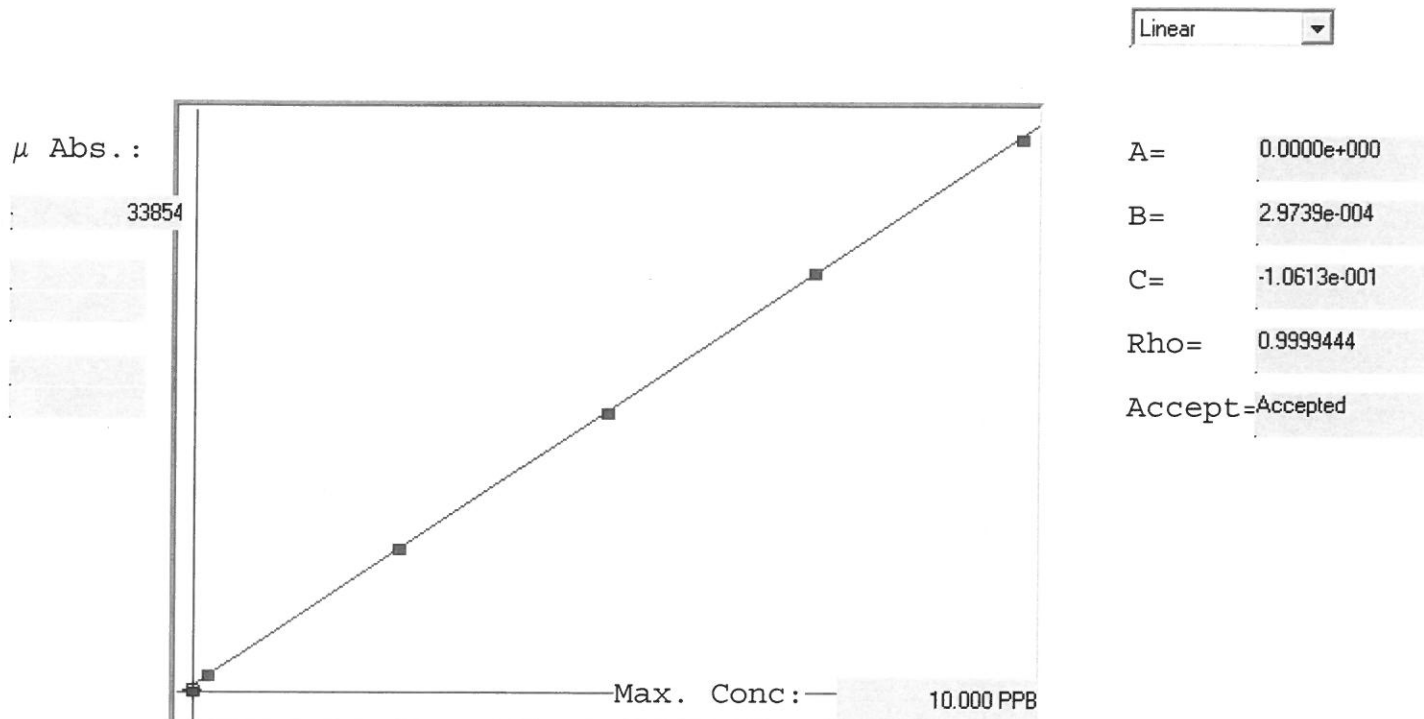


7470A

LB90905
INSTRUMENT ID: CV1

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.067	-0.067	132	0.000	132				
0.2	0.200	0.228	0.028	1122	0.0 %	1122				
2.5	2.500	2.538	0.038	8890	0.0 %	8890				
5.0	5.000	5.010	0.010	17204	0.0 %	17204				
7.5	7.500	7.529	0.029	25675	0.0 %	25675				
10.0	10.000	9.962	-0.038	33854	0.0 %	33854				

LB90905 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 18 Oct 2017 11:47:54

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	132	-	0.00007470A	PPB	18 Oct 2017 12:00:34	S	Std
0.2 - 1	56.2	1122	-	0.20007470A	PPB	18 Oct 2017 12:02:42	S	Std
2.5 - 1	52.5	8890	-	2.50007470A	PPB	18 Oct 2017 12:04:51	S	Std
5.0 - 1	55	17204	-	5.00007470A	PPB	18 Oct 2017 12:06:59	S	Std
7.5 - 1	57.5	25675	-	7.50007470A	PPB	18 Oct 2017 12:09:07	S	Std
10.0 - 1	57.5	33854	-	10.00007470A	PPB	18 Oct 2017 12:13:43	S	Std
ICV16 - 1	ICV16	13575	3.9310	-7470A	PPB	18 Oct 2017 12:16:18	U	SMPL
ICB16 - 1	ICB16	80	-0.0823	-7470A	PPB	18 Oct 2017 12:20:53	U	SMPL
CCV44 - 1	CCV44	17281	5.0332	-7470A	PPB	18 Oct 2017 12:22:59	U	SMPL
CCB44 - 1	CCB44	90	-0.0794	-7470A	PPB	18 Oct 2017 12:29:35	U	SMPL
CRA - 1	CRA	1069	0.2118	-7470A	PPB	18 Oct 2017 12:31:41	U	SMPL
HighStd - 1	HighStd	34114	10.0392	-7470A	PPB	18 Oct 2017 12:33:48	U	SMPL
ChkStd - 1	ChkStd	24849	7.2838	-7470A	PPB	18 Oct 2017 12:35:55	U	SMPL
PB103390BL - 1	PBW	49	-0.0916	-7470A	PPB	18 Oct 2017 12:40:58	U	SMPL
PB103390BS - 1	LCSW	13436	3.8897	-7470A	PPB	18 Oct 2017 12:45:30	U	SMPL
I5936-01 - 1	GROUNDWATER-432-B	882	0.1562	-7470A	PPB	18 Oct 2017 12:52:10	U	SMPL
I5936-01DUP - 1	GROUNDWATER-432-BDUP	895	0.1600	-7470A	PPB	18 Oct 2017 12:54:17	U	SMPL
I5936-01MS - 1	GROUNDWATER-432-BMS	15089	4.3813	-7470A	PPB	18 Oct 2017 12:56:26	U	SMPL
I5936-01MSD - 1	GROUNDWATER-432-BMSD	14604	4.2370	-7470A	PPB	18 Oct 2017 12:58:34	U	SMPL
PB103391BL - 1	PBW	88	-0.0800	-7470A	PPB	18 Oct 2017 13:03:03	U	SMPL
CCV45 - 1	CCV45	17157	4.9963	-7470A	PPB	18 Oct 2017 13:05:09	U	SMPL
CCB45 - 1	CCB45	82	-0.0817	-7470A	PPB	18 Oct 2017 13:09:42	U	SMPL
PB103391BS - 1	LCSW	13998	4.0568	-7470A	PPB	18 Oct 2017 13:11:48	U	SMPL
PB103391TB - 1	PB103348TB	28	-0.0978	-7470A	PPB	18 Oct 2017 13:16:19	U	SMPL
I5929-04 - 1	TP-1-COMP	42	-0.0936	-7470A	PPB	18 Oct 2017 13:18:25	U	SMPL
I5929-08 - 1	TP-2-COMP	43	-0.0933	-7470A	PPB	18 Oct 2017 13:20:32	U	SMPL
I5929-12 - 1	TP-1-2-COMP	25	-0.0987	-7470A	PPB	18 Oct 2017 13:22:40	U	SMPL
I5931-03 - 1	BU-01-101617	64	-0.0871	-7470A	PPB	18 Oct 2017 13:24:48	U	SMPL
I5935-03 - 1	CL-02-101617-A	35	-0.0957	-7470A	PPB	18 Oct 2017 13:26:56	U	SMPL
I5935-06 - 1	CL-02-101617-B	17	-0.1011	-7470A	PPB	18 Oct 2017 13:29:04	U	SMPL
I5935-09 - 1	CL-02-101617-C	47	-0.0921	-7470A	PPB	18 Oct 2017 13:31:13	U	SMPL
I5935-12 - 1	CL-02-101617-D	40	-0.0942	-7470A	PPB	18 Oct 2017 13:33:20	U	SMPL
CCV46 - 1	CCV46	17347	5.0528	-7470A	PPB	18 Oct 2017 13:35:26	U	SMPL
CCB46 - 1	CCB46	81	-0.0820	-7470A	PPB	18 Oct 2017 13:39:41	U	SMPL
I5935-15 - 1	CL-02-101617-E	21	-0.0999	-7470A	PPB	18 Oct 2017 13:41:48	U	SMPL
I5935-15DUP - 1	CL-02-101617-EDUP	38	-0.0948	-7470A	PPB	18 Oct 2017 13:43:55	U	SMPL
I5935-15MS - 1	CL-02-101617-EMS	13056	3.7767	-7470A	PPB	18 Oct 2017 13:46:02	U	SMPL
I5935-15MSD - 1	CL-02-101617-EMSD	12431	3.5908	-7470A	PPB	18 Oct 2017 13:48:09	U	SMPL
I5936-01LX5 - 1		432	0.0223	-7470A	PPB	18 Oct 2017 13:50:17	U	SMPL
I5936-01A - 1		13988	4.0538	-7470A	PPB	18 Oct 2017 13:52:25	U	SMPL
I5935-15LX5 - 1		-24	-0.1133	-7470A	PPB	18 Oct 2017 13:54:33	U	SMPL
I5935-15A - 1		13978	4.0509	-7470A	PPB	18 Oct 2017 13:56:42	U	SMPL
CCV47 - 1	CCV47	16926	4.9276	-7470A	PPB	18 Oct 2017 13:58:49	U	SMPL
CCB47 - 1	CCB47	70	-0.0853	-7470A	PPB	18 Oct 2017 14:03:23	U	SMPL