


ISM02.4

LB 90951
INSTRUMENT ID: CV1

Linear

 μ Abs.:

44295

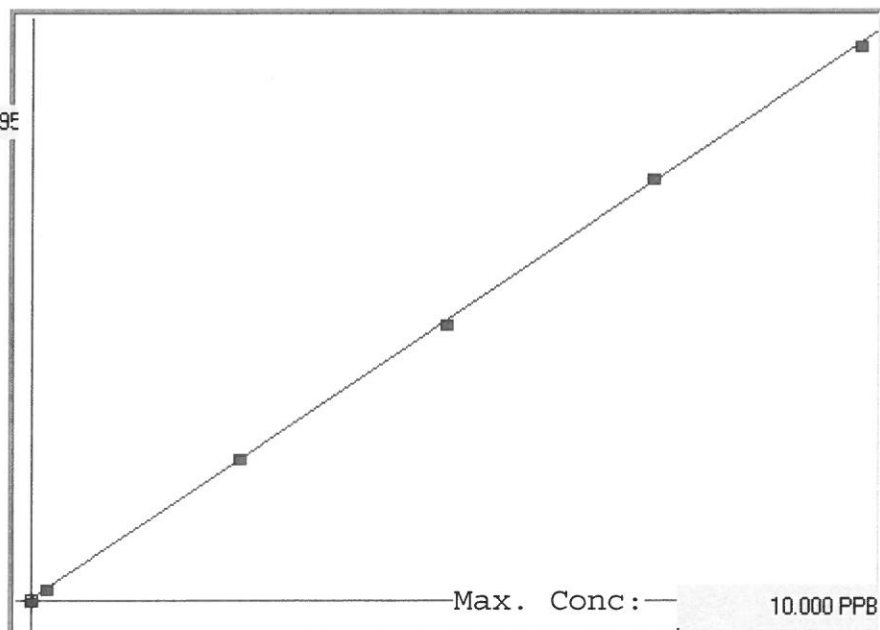

A= 0.0000e+000

B= 2.2526e-004

C= -3.0358e-002

Rho= 0.9999197

Accept=Accepted

slope
y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.00	0.000	-0.015	-0.015	67	0.000	67				
0.2	0.200	0.194	-0.006	997	0.0 %	997				
2.5	2.500	2.529	0.029	11360	0.0 %	11360				
5.0	5.000	4.958	-0.042	22146	0.0 %	22146				
7.5	7.500	7.587	0.087	33815	0.0 %	33815				
10.0	10.000	9.947	-0.053	44295	0.0 %	44295				

0/00

3

1

1

1

1

NB

10/13/18

LB90951
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	67	-		0 ISM02.4	PPB	10/19/2017 16:18	Std
	0.2 S0.2	997	-		0.2 ISM02.4	PPB	10/19/2017 16:20	Std
	2.5 S2.5	11360	-		2.5 ISM02.4	PPB	10/19/2017 16:22	Std
	5 S5	22146	-		5 ISM02.4	PPB	10/19/2017 16:27	Std
	7.5 S7.5	33815	-		7.5 ISM02.4	PPB	10/19/2017 16:29	Std
	10 S10	44295	-		10 ISM02.4	PPB	10/19/2017 16:31	Std
ICV	ICV	17599	3.934	-	ISM02.4	PPB	10/19/2017 16:34	SMPL
ICB	ICB	-156	-0.0655	-	ISM02.4	PPB	10/19/2017 16:36	SMPL
CCV063	CCV063	21565	4.8273	-	ISM02.4	PPB	10/19/2017 16:39	SMPL
CCB063	CCB063	-147	-0.0635	-	ISM02.4	PPB	10/19/2017 16:41	SMPL
PB103421BL	PBS004	6	-0.029	-	ISM02.4	PPB	10/19/2017 16:43	SMPL
I5933-01	B-9(0-1)_101617	15735	3.5141	-	ISM02.4	PPB	10/19/2017 16:45	SMPL
I5933-02	B-9(5-6)_101617	211171	47.5377	-	ISM02.4	PPB	10/19/2017 16:48	SMPL
I5958-01	B-71(3-5)-101617	577	0.0996	-	ISM02.4	PPB	10/19/2017 16:50	SMPL
I5958-02	B-10(3-5)-101617	5198	1.1405	-	ISM02.4	PPB	10/19/2017 16:53	SMPL
I5958-03	B-17(0.25-1.25)-101717	5332	1.1707	-	ISM02.4	PPB	10/19/2017 16:55	SMPL
I5958-04	B-17(5-6.5)-101717	2290	0.4855	-	ISM02.4	PPB	10/19/2017 16:57	SMPL
I5958-05	B-15(0.25-1.25)-101717	12786	2.8498	-	ISM02.4	PPB	10/19/2017 16:59	SMPL
I5958-06	B-15(0.25-1.25)-101717D	11784	2.6241	-	ISM02.4	PPB	10/19/2017 17:02	SMPL
I5958-07	B-15(0.25-1.25)-101717S	21929	4.9093	-	ISM02.4	PPB	10/19/2017 17:09	SMPL
I5958-08	B-15(5-6)-101717	1019	0.1992	-	ISM02.4	PPB	10/19/2017 17:11	SMPL
I5958-09	B-14(0-1)-101717	1226	0.2458	-	ISM02.4	PPB	10/19/2017 17:14	SMPL
I5958-10	DUP-6	2627	0.5614	-	ISM02.4	PPB	10/19/2017 17:16	SMPL
I5958-11	B-14(7-7.5)-101717	75	-0.0135	-	ISM02.4	PPB	10/19/2017 17:18	SMPL
I5958-13	B-6(3.5-4.5)-101717	547	0.0929	-	ISM02.4	PPB	10/19/2017 17:20	SMPL
I5958-14	B-6(5-5.5)-101717	4504	0.9842	-	ISM02.4	PPB	10/19/2017 17:23	SMPL
I5976-01	B-20(3.5-4)-101817	14702	3.2814	-	ISM02.4	PPB	10/19/2017 17:25	SMPL
I5976-02	B-20(5-6)-101817	1340	0.2715	-	ISM02.4	PPB	10/19/2017 17:27	SMPL
I5933-02DLX10	B-9(5-6)_101617	21156	4.7352	-	ISM02.4	PPB	10/19/2017 17:30	SMPL
CCV064	CCV064	21962	4.9168	-	ISM02.4	PPB	10/19/2017 17:32	SMPL
CCB064	CCB064	-145	-0.063	-	ISM02.4	PPB	10/19/2017 17:34	SMPL