


ISM02.4

LB91147
INSTRUMENT ID: CV1

Linear

 μ Abs.:

45384

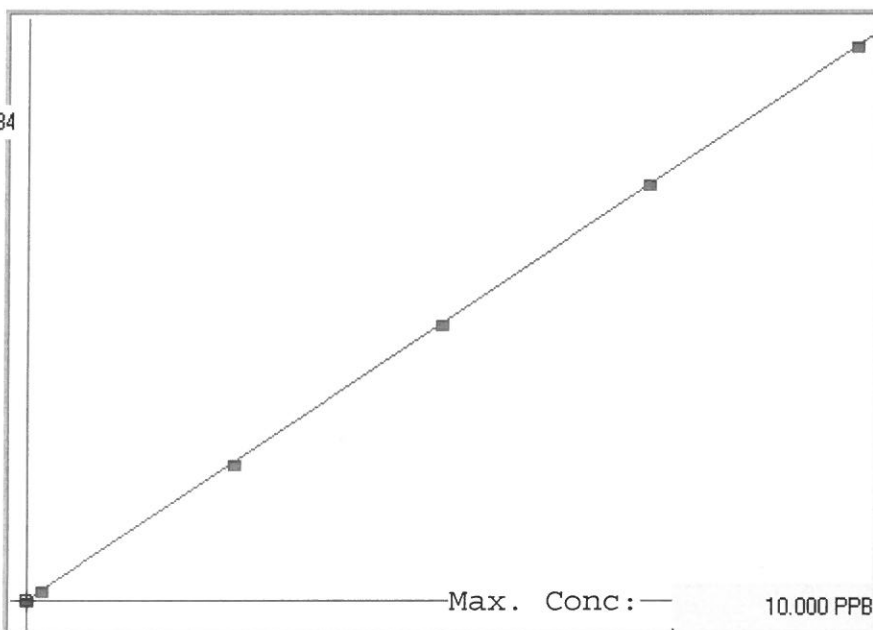

A= 0.0000e+000

B= 2.2024e-004

C= 2.7184e-003

Rho= 0.9999957

Accept=Accepted

slope
y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.005	0.005	9	0.000	9					1
0.2	0.200	0.209	0.009	935	0.0 %	935					4
2.5	2.500	2.486	-0.014	11274	0.0 %	11274					1
5.0	5.000	4.988	-0.012	22634	0.0 %	22634					0
7.5	7.500	7.515	0.015	34112	0.0 %	34112					0
10.0	10.000	9.998	-0.002	45384	0.0 %	45384					0

NB
10/27/18

LB91147
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	9	-		0 ISM02.4	PPB	10/27/2017 9:52	Std
	0.2 S0.2	935	-		0.2 ISM02.4	PPB	10/27/2017 9:54	Std
	2.5 S2.5	11274	-		2.5 ISM02.4	PPB	10/27/2017 9:56	Std
	5 S5	22634	-		5 ISM02.4	PPB	10/27/2017 9:59	Std
	7.5 S7.5	34112	-		7.5 ISM02.4	PPB	10/27/2017 10:01	Std
	10 S10	45384	-		10 ISM02.4	PPB	10/27/2017 10:03	Std
ICV	ICV	17758	3.9137 -		ISM02.4	PPB	10/27/2017 10:06	SMPL
ICB	ICB	182	0.0428 -		ISM02.4	PPB	10/27/2017 10:08	SMPL
CCV028	CCV028	22671	4.9957 -		ISM02.4	PPB	10/27/2017 10:11	SMPL
CCB028	CCB028	184	0.0432 -		ISM02.4	PPB	10/27/2017 10:13	SMPL
PB103663BL	PBS004	327	0.0747 -		ISM02.4	PPB	10/27/2017 10:15	SMPL
I6032-01	B-31(1-2)-101817	132308	29.1419 -		ISM02.4	PPB	10/27/2017 10:17	SMPL
I6032-02	B-31(5-5.5)-101817	90020	19.8285 -		ISM02.4	PPB	10/27/2017 10:20	SMPL
I6097-01	B-76(0-1)-102317	154636	34.0593 -		ISM02.4	PPB	10/27/2017 10:22	SMPL
I6097-02	B-31(5-5.5)-101817	252057	55.5151 -		ISM02.4	PPB	10/27/2017 10:24	SMPL
I6097-03	B-52(0-1)-102317	39045	8.6019 -		ISM02.4	PPB	10/27/2017 10:27	SMPL
I6097-04	B-52(0-1)-102317D	39830	8.7748 -		ISM02.4	PPB	10/27/2017 10:30	SMPL
I6097-05	B-52(0-1)-102317S	48704	10.7292 -		ISM02.4	PPB	10/27/2017 10:32	SMPL
I6097-06	B-52(1-3)-102317	125884	27.7271 -		ISM02.4	PPB	10/27/2017 10:34	SMPL
I6120-04	B-68(1-2)-102417	16208	3.5723 -		ISM02.4	PPB	10/27/2017 10:38	SMPL
CCV029	CCV029	22603	4.9807 -		ISM02.4	PPB	10/27/2017 10:41	SMPL
CCB029	CCB029	135	0.0325 -		ISM02.4	PPB	10/27/2017 10:43	SMPL
I6032-01DLX5	B-31(1-2)-101817	27513	6.0621 -		ISM02.4	PPB	10/27/2017 10:45	SMPL
I6032-02DLX5	B-31(5-5.5)-101817	18492	4.0753 -		ISM02.4	PPB	10/27/2017 10:48	SMPL
I6097-01DLX5	B-76(0-1)-102317	32136	7.0803 -		ISM02.4	PPB	10/27/2017 10:50	SMPL
I6097-02DLX10	B-31(5-5.5)-101817	27504	6.0601 -		ISM02.4	PPB	10/27/2017 10:52	SMPL
I6097-03DLX2	B-52(0-1)-102317	20333	4.4808 -		ISM02.4	PPB	10/27/2017 10:55	SMPL
I6097-04DLX2	B-52(0-1)-102317D	20320	4.4779 -		ISM02.4	PPB	10/27/2017 10:57	SMPL
I6097-05DLX2	B-52(0-1)-102317S	24977	5.5036 -		ISM02.4	PPB	10/27/2017 10:59	SMPL
I6097-06DLX5	B-52(1-3)-102317	26020	5.7333 -		ISM02.4	PPB	10/27/2017 11:02	SMPL
I6097-07	DUP-7	277946	61.2168 -		ISM02.4	PPB	10/27/2017 11:06	SMPL
I6097-07DLX10	DUP-7	28891	6.3656 -		ISM02.4	PPB	10/27/2017 11:08	SMPL
CCV030	CCV030	22414	4.9391 -		ISM02.4	PPB	10/27/2017 11:11	SMPL
CCB030	CCB030	-167	-0.0341 -		ISM02.4	PPB	10/27/2017 11:13	SMPL