

LB 91291

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/1/2017 14:58

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.111	0.0	0.104	
ICB1	-1.565	0.0	0.003	
CCV1	249.620	0.0	0.260	
CCB1	-1.345	0.0	0.003	
PB103879BL	-1.571	0.0	0.003	
I6247-03	-1.441	0.0	0.003	
I6247-03DUP	-1.641	0.0	0.003	
I6249-02	-1.595	0.0	0.003	
I6249-04	-1.717	0.0	0.003	
I6252-02	-1.722	0.0	0.003	
I6253-02	-1.688	0.0	0.003	
I6254-03	-1.546	0.0	0.003	
CCV2	255.519	0.0	0.266	
CCB2	-1.469	0.0	0.003	

N	14
Mean	41.782
SD	93.0746
CV%	222.76

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed Nov 01 14:41:58 2017

Wed Nov 01 14:47:47 2017

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-1.6764	µg/l	11/1/2017 11:27:07	
5.OPPBCN	A	Reactive CN	P	4.11	µg/l	11/1/2017 11:27:08	
10PPBCN	A	Reactive CN	P	8.8751	µg/l	11/1/2017 11:27:09	
50PPBCN	A	Reactive CN	P	53.5542	µg/l	11/1/2017 11:27:10	
100PPBCN	A	Reactive CN	P	98.1343	µg/l	11/1/2017 11:27:11	
250PPBCN	A	Reactive CN	P	253.9074	µg/l	11/1/2017 11:27:12	
500PPBCN	A	Reactive CN	P	498.0954	µg/l	11/1/2017 11:27:13	
ICV1	S	Reactive CN	P	97.1105	µg/l	11/1/2017 14:41:59	
ICB1	S	Reactive CN	P	-1.5654	µg/l	11/1/2017 14:42:00	
CCV1	S	Reactive CN	P	249.62	µg/l	11/1/2017 14:42:03	
CCB1	S	Reactive CN	P	-1.3452	µg/l	11/1/2017 14:42:04	
PB103879BL	S	Reactive CN	P	-1.5705	µg/l	11/1/2017 14:42:06	
I6247-03	S	Reactive CN	P	-1.4405	µg/l	11/1/2017 14:42:07	
I6247-03DUP	S	Reactive CN	P	-1.6406	µg/l	11/1/2017 14:42:08	
I6249-02	S	Reactive CN	P	-1.5953	µg/l	11/1/2017 14:47:41	
I6249-04	S	Reactive CN	P	-1.7169	µg/l	11/1/2017 14:47:42	
I6252-02	S	Reactive CN	P	-1.7218	µg/l	11/1/2017 14:47:43	
I6253-02	S	Reactive CN	P	-1.6875	µg/l	11/1/2017 14:47:44	
I6254-03	S	Reactive CN	P	-1.5455	µg/l	11/1/2017 14:47:45	
CCV2	S	Reactive CN	P	255.5193	µg/l	11/1/2017 14:47:46	
CCB2	S	Reactive CN	P	-1.4689	µg/l	11/1/2017 14:47:47	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/1/2017 11:32


Test Total CN

Accepted 11/1/2017 11:32

Factor 978.8
Bias 0.005

Coeff. of det. 0.999806

Errors

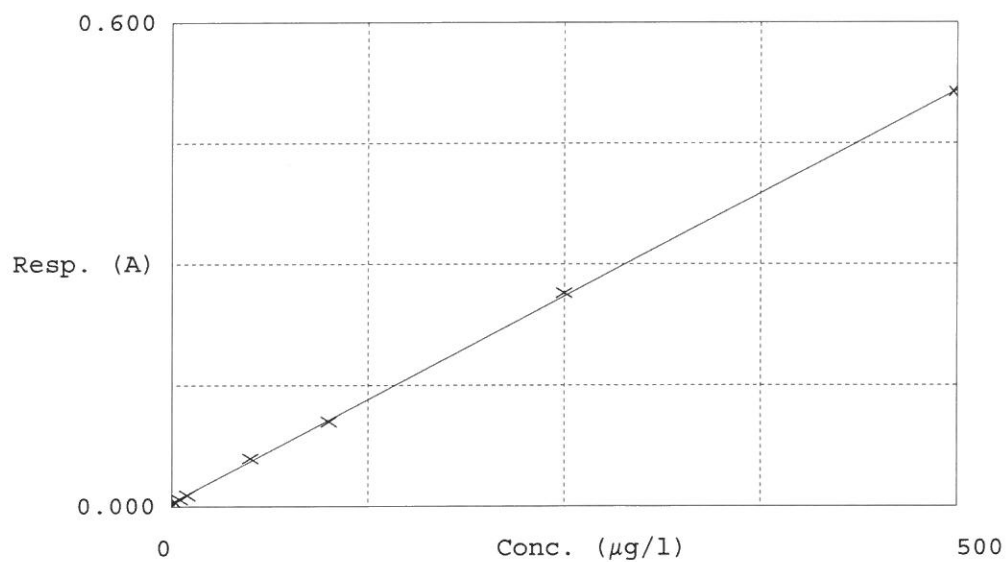

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.6764	0.0000	
2	5.0PPBCN	0.009	4.1100	5.0000	
3	10PPBCN	0.014	8.8751	10.0000	
4	50PPBCN	0.060	53.5542	50.0000	
5	100PPBCN	0.105	98.1343	100.0000	
6	250PPBCN	0.264	253.9074	250.0000	
7	500PPBCN	0.514	498.0954	500.0000	