


ISM02.4

LB 91293
INSTRUMENT ID: CV1

Linear

 μ Abs.:

40275

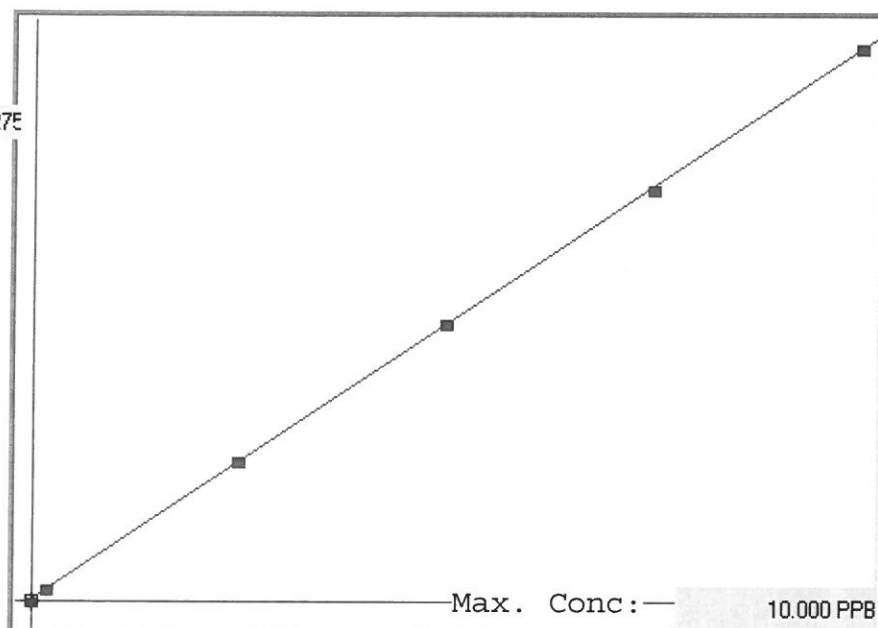

A= 0.0000e+000

B= 2.4906e-004

C= -2.4430e-002

Rho= 0.9999844

Accept=Accepted

slope
y-intercept

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%OD
0.00	0.000	-0.017	-0.017	30	0.000	30					
0.2	0.200	0.194	-0.006	878	0.0 %	878					
2.5	2.500	2.527	0.027	10245	0.0 %	10245					
5.0	5.000	5.021	0.021	20257	0.0 %	20257					
7.5	7.500	7.468	-0.032	30083	0.0 %	30083					
10.0	10.000	10.007	0.007	40275	0.0 %	40275					

NB
11/2/12

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0-0	30	-		0 ISM02.4	PPB	11/2/2017 13:06	Std
	0.2 S0.2	878	-		0.2 ISM02.4	PPB	11/2/2017 13:08	Std
	2.5 S2.5	10245	-		2.5 ISM02.4	PPB	11/2/2017 13:10	Std
	5 S5	20257	-		5 ISM02.4	PPB	11/2/2017 13:13	Std
	7.5 S7.5	30083	-		7.5 ISM02.4	PPB	11/2/2017 13:15	Std
	10 S10	40275	-		10 ISM02.4	PPB	11/2/2017 13:17	Std
ICV	ICV	15759	3.9005 -		ISM02.4	PPB	11/2/2017 13:20	SMPL
ICB	ICB	-134	-0.0578 -		ISM02.4	PPB	11/2/2017 13:22	SMPL
CCV077	CCV077	20371	5.0492 -		ISM02.4	PPB	11/2/2017 13:25	SMPL
CCB077	CCB077	-139	-0.059 -		ISM02.4	PPB	11/2/2017 13:27	SMPL
PB103897BL	PBW003	-14	-0.0279 -		ISM02.4	PPB	11/2/2017 13:29	SMPL
I6104-04	MBDY25	6	-0.0229 -		ISM02.4	PPB	11/2/2017 13:31	SMPL
I6104-05	MBDXK9	4	-0.0234 -		ISM02.4	PPB	11/2/2017 13:34	SMPL
I6104-06	MBDXL0	576	0.119 -		ISM02.4	PPB	11/2/2017 13:36	SMPL
I6104-07	MBDXL1	-4	-0.0254 -		ISM02.4	PPB	11/2/2017 13:38	SMPL
I6104-08	MBDXL5	14	-0.0209 -		ISM02.4	PPB	11/2/2017 13:41	SMPL
I6104-09	MBDY66	-7	-0.0262 -		ISM02.4	PPB	11/2/2017 13:43	SMPL
I6104-10	MBDXL7	-37	-0.0336 -		ISM02.4	PPB	11/2/2017 13:45	SMPL
I6104-11	MBDXL7D	-22	-0.0299 -		ISM02.4	PPB	11/2/2017 13:47	SMPL
I6104-12	MBDXL7S	4566	1.1128 -		ISM02.4	PPB	11/2/2017 13:50	SMPL
I6104-16	MBDY26	-28	-0.0314 -		ISM02.4	PPB	11/2/2017 13:52	SMPL
PB103898BL	PBW003	23	-0.0187 -		ISM02.4	PPB	11/2/2017 13:54	SMPL
I6150-01	TWP-B-68	214	0.0289 -		ISM02.4	PPB	11/2/2017 13:56	SMPL
I6150-02	TWP-B-75	30	-0.017 -		ISM02.4	PPB	11/2/2017 13:59	SMPL
I6150-03	TWP-B-70	4140	1.0067 -		ISM02.4	PPB	11/2/2017 14:01	SMPL
I6175-01	TWP-B-51	2744	0.659 -		ISM02.4	PPB	11/2/2017 14:03	SMPL
I6175-04	TWP-B-30	1129	0.2568 -		ISM02.4	PPB	11/2/2017 14:06	SMPL
CCV078	CCV078	20508	5.0833 -		ISM02.4	PPB	11/2/2017 14:08	SMPL
CCB078	CCB078	-100	-0.0493 -		ISM02.4	PPB	11/2/2017 14:10	SMPL