


7470A

LB 91326
INSTRUMENT ID: CV1

Linear

 μ Abs.:

33890

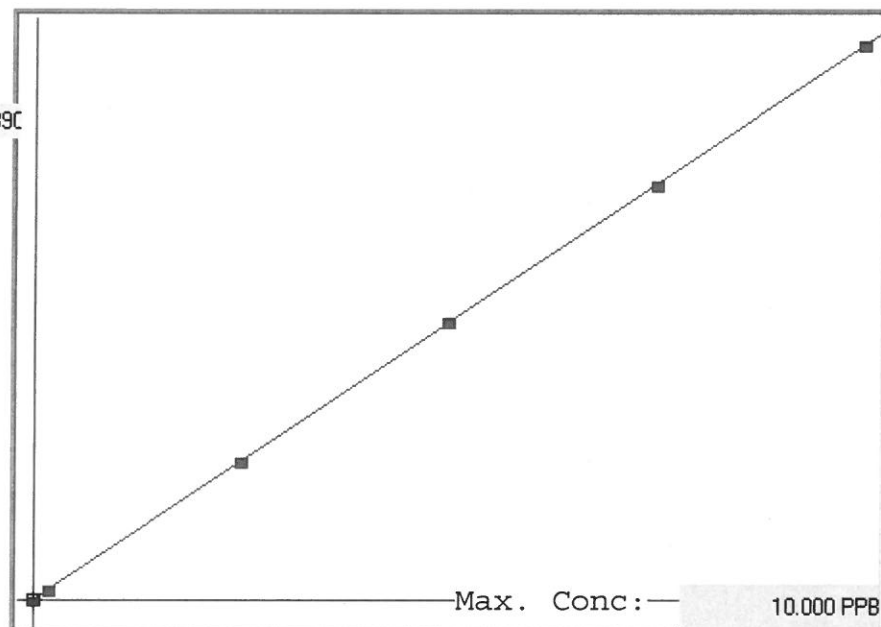

A= 0.0000e+000

B= 2.9516e-004

C= -7.1081e-003

Rho= 0.9999886

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	3	0.000	3				
0.2	0.200	0.193	-0.007	677	0.0 %	677				
2.5	2.500	2.500	-0.000	8493	0.0 %	8493				
5.0	5.000	5.037	0.037	17090	0.0 %	17090				
7.5	7.500	7.481	-0.019	25369	0.0 %	25369				
10.0	10.000	9.996	-0.004	33890	0.0 %	33890				

LB91326 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 03 Nov 2017 10:23:13					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	3	-	0.0000	7470A	PPB	03 Nov 2017 10:32:36	S	Std
0.2 - 1	50.2	677	-	0.2000	7470A	PPB	03 Nov 2017 10:34:45	S	Std
2.5 - 1	52.5	8493	-	2.5000	7470A	PPB	03 Nov 2017 10:36:53	S	Std
5.0 - 1	55	17090	-	5.0000	7470A	PPB	03 Nov 2017 10:39:01	S	Std
7.5 - 1	57.5	25369	-	7.5000	7470A	PPB	03 Nov 2017 10:41:09	S	Std
10.0 - 1	510	33890	-	10.0000	7470A	PPB	03 Nov 2017 10:43:17	S	Std
ICV43 - 1	ICV43	13166	3.8790	-	7470A	PPB	03 Nov 2017 10:46:11	U	SMPL
ICB43 - 1	ICB43	-80	-0.0307	-	7470A	PPB	03 Nov 2017 10:48:17	U	SMPL
CCV86 - 1	CCV86	17128	5.0484	-	7470A	PPB	03 Nov 2017 10:50:24	U	SMPL
CCB86 - 1	CCB86	-142	-0.0490	-	7470A	PPB	03 Nov 2017 10:52:30	U	SMPL
CRA - 1	CRA	633	0.1797	-	7470A	PPB	03 Nov 2017 10:54:38	U	SMPL
HighStd - 1	HighStd	33376	9.8441	-	7470A	PPB	03 Nov 2017 10:56:45	U	SMPL
ChkStd - 1	ChkStd	24807	7.3149	-	7470A	PPB	03 Nov 2017 10:58:52	U	SMPL
PB103941BL - 1	PBW	-202	-0.0667	-	7470A	PPB	03 Nov 2017 11:01:01	U	SMPL
PB103941BS - 1	LCSW	13176	3.8819	-	7470A	PPB	03 Nov 2017 11:03:10	U	SMPL
PB103941TB - 1	PB103900	-122	-0.0431	-	7470A	PPB	03 Nov 2017 11:05:18	U	SMPL
I6189-02 - 1	LEONIA-GEN	-20	-0.0130	-	7470A	PPB	03 Nov 2017 11:07:27	U	SMPL
I6189-02DUP - 1	LEONIA-GENDUP	-12	-0.0106	-	7470A	PPB	03 Nov 2017 11:09:35	U	SMPL
I6189-02MS - 1	LEONIA-GENMS	12893	3.7984	-	7470A	PPB	03 Nov 2017 11:11:43	U	SMPL
I6189-02MSD - 1	LEONIA-GENMSD	12968	3.8205	-	7470A	PPB	03 Nov 2017 11:13:50	U	SMPL
CCV87 - 1	CCV87	17298	5.0986	-	7470A	PPB	03 Nov 2017 11:15:57	U	SMPL
CCB87 - 1	CCB87	-158	-0.0537	-	7470A	PPB	03 Nov 2017 11:18:04	U	SMPL
I6243-02 - 1	N35799	-14	-0.0112	-	7470A	PPB	03 Nov 2017 11:20:12	U	SMPL
I6258-03 - 1	WOODLAKE-DR-2-14-18	-3	-0.0080	-	7470A	PPB	03 Nov 2017 11:22:18	U	SMPL
I6258-06 - 1	BOXWOOD-DR-2-4-12-14	-23	-0.0139	-	7470A	PPB	03 Nov 2017 11:24:25	U	SMPL
I6261-02 - 1	HOMESTEAD-AISLE-SWITCHGEAR	-11	-0.0104	-	7470A	PPB	03 Nov 2017 11:26:33	U	SMPL
I6265-03 - 1	COMP-1	17	-0.0021	-	7470A	PPB	03 Nov 2017 11:28:40	U	SMPL
I6265-04 - 1	COMP-2	33	0.0026	-	7470A	PPB	03 Nov 2017 11:30:48	U	SMPL
I6275-02 - 1	DRUM(1-2)	7	-0.0050	-	7470A	PPB	03 Nov 2017 11:32:56	U	SMPL
I6275-04 - 1	DRUM-2	-6	-0.0089	-	7470A	PPB	03 Nov 2017 11:35:04	U	SMPL
I6275-07 - 1	CONCRETE-PILE	-9	-0.0098	-	7470A	PPB	03 Nov 2017 11:37:13	U	SMPL
I6275-10 - 1	2727	182	0.0466	-	7470A	PPB	03 Nov 2017 11:39:20	U	SMPL
CCV88 - 1	CCV88	17067	5.0304	-	7470A	PPB	03 Nov 2017 11:41:27	U	SMPL
CCB88 - 1	CCB88	-146	-0.0502	-	7470A	PPB	03 Nov 2017 11:43:34	U	SMPL
I6277-02 - 1	FADW4807L	6	-0.0053	-	7470A	PPB	03 Nov 2017 11:45:41	U	SMPL
I6189-02LX5 - 1		18	-0.0018	-	7470A	PPB	03 Nov 2017 11:47:48	U	SMPL
I6189-02A - 1		13800	4.0661	-	7470A	PPB	03 Nov 2017 11:49:55	U	SMPL
CCV89 - 1	CCV89	17386	5.1245	-	7470A	PPB	03 Nov 2017 11:52:02	U	SMPL
CCB89 - 1	CCB89	-164	-0.0555	-	7470A	PPB	03 Nov 2017 11:54:10	U	SMPL