

=====

Test results

Aquakem 7.2AQ1

LB91339
Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/3/2017 14:26

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.137	0.0	0.095	
ICB1	-0.165	0.0	0.003	
CCV1	244.056	0.0	0.231	
CCB1	0.229	0.0	0.004	
PB103931BL	-0.273	0.0	0.003	
PB103931BS	96.687	0.0	0.094	
MIDPB103931	246.928	0.0	0.233	
I6276-01	0.219	0.0	0.004	
I6276-01DUP	0.457	0.0	0.004	
I6276-01MS	37.313	0.0	0.038	
I6276-01MSD	37.995	0.0	0.039	
CCV2	258.111	0.0	0.244	
CCB2	0.066	0.0	0.004	

N	13
Mean	78.443
SD	103.6743
CV%	132.17

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Nov 03 13:59:51 2017

Fri Nov 03 14:05:11 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.433	µg/l	11/3/2017 10:28:34	
5.OPPBCN	A	Total CN	P	4.7648	µg/l	11/3/2017 10:28:35	
10PPBCN	A	Total CN	P	9.6572	µg/l	11/3/2017 10:28:36	
50PPBCN	A	Total CN	P	50.0702	µg/l	11/3/2017 10:28:37	
100PPBCN	A	Total CN	P	101.0255	µg/l	11/3/2017 10:28:38	
250PPBCN	A	Total CN	P	250.2367	µg/l	11/3/2017 10:28:39	
500PPBCN	A	Total CN	P	499.6787	µg/l	11/3/2017 10:28:40	
ICV1	S	Total CN	P	98.1367	µg/l	11/3/2017 13:59:52	
ICB1	S	Total CN	P	-0.1651	µg/l	11/3/2017 13:59:53	
CCV1	S	Total CN	P	244.0558	µg/l	11/3/2017 13:59:56	
CCB1	S	Total CN	P	0.2293	µg/l	11/3/2017 13:59:57	
PB103931BL	S	Total CN	P	-0.2734	µg/l	11/3/2017 13:59:59	
PB103931BS	S	Total CN	P	96.6869	µg/l	11/3/2017 14:00:00	
MIDPB103931	S	Total CN	P	246.9276	µg/l	11/3/2017 14:00:01	
I6276-01	S	Total CN	P	0.2189	µg/l	11/3/2017 14:05:06	
I6276-01DUP	S	Total CN	P	0.4574	µg/l	11/3/2017 14:05:07	
I6276-01MS	S	Total CN	P	37.3131	µg/l	11/3/2017 14:05:08	
I6276-01MSD	S	Total CN	P	37.9949	µg/l	11/3/2017 14:05:09	
CCV2	S	Total CN	P	258.1111	µg/l	11/3/2017 14:05:10	
CCB2	S	Total CN	P	0.0658	µg/l	11/3/2017 14:05:11	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

11/3/2017 10:33


Test Total CN

Accepted 11/3/2017 10:33

Factor 1074
Bias 0.003

Coeff. of det. 0.999992

Errors

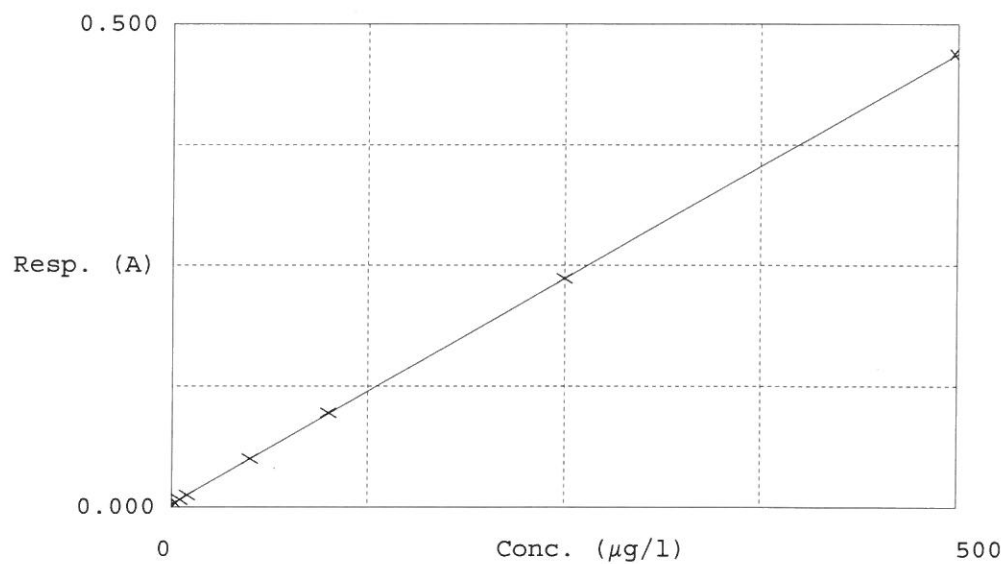

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.4330	0.0000	
2	5.0PPBCN	0.008	4.7648	5.0000	
3	10PPBCN	0.012	9.6572	10.0000	
4	50PPBCN	0.050	50.0702	50.0000	
5	100PPBCN	0.098	101.0255	100.0000	
6	250PPBCN	0.237	250.2367	250.0000	
7	500PPBCN	0.469	499.6787	500.0000	