

7471A


LB91421

INSTRUMENT ID: CV1

Linear

 μ Abs.:

40991

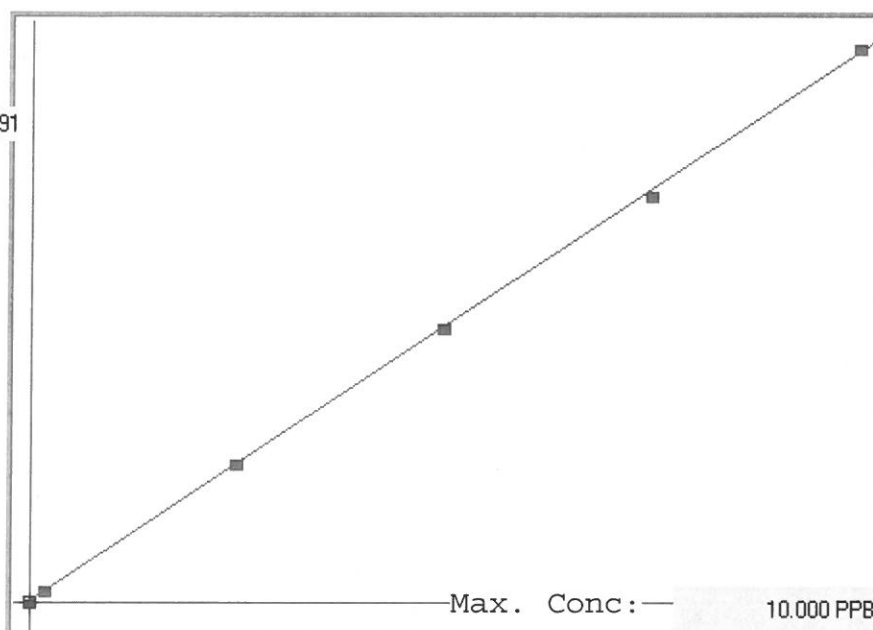

A= 0.0000e+000

B= 2.4596e-004

C= -1.6013e-002

Rho= 0.9999169

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.017	0.017	133	0.000	133				
0.2	0.200	0.202	0.002	887	0.0 %	887				
2.5	2.500	2.506	0.006	10255	0.0 %	10255				
5.0	5.000	5.003	0.003	20404	0.0 %	20404				
7.5	7.500	7.406	-0.094	30175	0.0 %	30175	0			
10.0	10.000	10.066	0.066	40991	0.0 %	40991				

Method: 7471A		Operator: Admin		Date of Analysis: 07 Nov 2017 15:34:46					
Sample ID	Extended ID	µ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	133	-	0.0000	7471A	PPB	07 Nov 2017 15:36:05	S	Std
0.2 - 1	50.2	887	-	0.2000	7471A	PPB	07 Nov 2017 15:38:23	S	Std
2.5 - 1	52.5	10255	-	2.5000	7471A	PPB	07 Nov 2017 15:40:40	S	Std
5.0 - 1	55	20404	-	5.0000	7471A	PPB	07 Nov 2017 15:42:58	S	Std
7.5 - 1	57.5	30175	-	7.5000	7471A	PPB	07 Nov 2017 15:45:15	S	Std
10.0 - 1	510	40991	-	10.0000	7471A	PPB	07 Nov 2017 15:47:33	S	Std
ICV50 - 1	ICV50	15431	3.7794	-	7471A	PPB	07 Nov 2017 15:50:20	U	SMPL
ICB50 - 1	ICB50	28	-0.0091	-	7471A	PPB	07 Nov 2017 15:52:35	U	SMPL
CCV18 - 1	CCV18	20761	5.0904	-	7471A	PPB	07 Nov 2017 15:54:52	U	SMPL
CCB18 - 1	CCB18	16	-0.0121	-	7471A	PPB	07 Nov 2017 15:57:08	U	SMPL
CRA - 1	CRA	861	0.1958	-	7471A	PPB	07 Nov 2017 15:59:25	U	SMPL
HighStd - 1	HighStd	41041	10.0786	-	7471A	PPB	07 Nov 2017 16:01:41	U	SMPL
ChkStd - 1	ChkStd	28663	7.0340	-	7471A	PPB	07 Nov 2017 16:03:57	U	SMPL
PB104032BL - 1	PBS	-164	-0.0564	-	7471A	PPB	07 Nov 2017 16:06:16	U	SMPL
PB104032BS - 1	LCSS	14403	3.5266	-	7471A	PPB	07 Nov 2017 16:08:34	U	SMPL
I6300-01 - 1	OR-02-110617	4656	1.1292	-	7471A	PPB	07 Nov 2017 16:10:51	U	SMPL
I6311-01 - 1	TR-04-110617	3130	0.7539	-	7471A	PPB	07 Nov 2017 16:13:08	U	SMPL
I6343-07 - 1	HL-DAM	374	0.0760	-	7471A	PPB	07 Nov 2017 16:15:26	U	SMPL
I6346-01 - 1	EPE-120-5(0-5)	1611	0.3802	-	7471A	PPB	07 Nov 2017 16:17:43	U	SMPL
I6346-02 - 1	EPE-120-5(5-10)	2016	0.4798	-	7471A	PPB	07 Nov 2017 16:19:59	U	SMPL
CCV19 - 1	CCV19	20672	5.0685	-	7471A	PPB	07 Nov 2017 16:22:15	U	SMPL
CCB19 - 1	CCB19	18	-0.0116	-	7471A	PPB	07 Nov 2017 16:24:31	U	SMPL
I6346-03 - 1	EPE-120-5(10-12)	1808	0.4287	-	7471A	PPB	07 Nov 2017 16:26:47	U	SMPL
I6346-04 - 1	EPE-120-5(20-22)	266	0.0494	-	7471A	PPB	07 Nov 2017 16:29:03	U	SMPL
I6346-05 - 1	EPE-120-5(25-27)	213	0.0364	-	7471A	PPB	07 Nov 2017 16:31:19	U	SMPL
I6346-06 - 1	EPE-120-5(30-32)	199	0.0329	-	7471A	PPB	07 Nov 2017 16:33:36	U	SMPL
I6346-07 - 1	EPE-120-5(40-42)	190	0.0307	-	7471A	PPB	07 Nov 2017 16:35:52	U	SMPL
I6346-08 - 1	EPE-120-5(50-52)	424	0.0883	-	7471A	PPB	07 Nov 2017 16:38:10	U	SMPL
I6353-01 - 1	ROLLOFF-292	244	0.0440	-	7471A	PPB	07 Nov 2017 16:40:27	U	SMPL
I6354-01 - 1	POOL-5001-0001-01	4028	0.9747	-	7471A	PPB	07 Nov 2017 16:42:44	U	SMPL
I6354-01DUP - 1	POOL-5001-0001-01DUP	3668	0.8862	-	7471A	PPB	07 Nov 2017 16:45:03	U	SMPL
I6354-02 - 1	I6354-01MS	18524	4.5402	-	7471A	PPB	07 Nov 2017 16:47:19	U	SMPL
CCV20 - 1	CCV20	20431	5.0093	-	7471A	PPB	07 Nov 2017 16:49:35	U	SMPL